

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083019\
Data File : FB022268.D
Signal(s) : FID2B.CH
Acq On : 30 Aug 2019 12:18
Operator : DD/AJ
Sample : K4608-01
Misc : 5.02/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 30 14:03:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.988	413785	19.481 ng/ml
Target Compounds			
4) t Benzene	8.050	3849	0.086 ng/ml
6) t Toluene	10.834	15171	0.493 ng/ml
7) t Ethylbenzene	13.251	3915	0.192 ng/ml
8) t m-Xylene	13.399	9052	0.430 ng/ml
9) t O-Xylene	14.128	11838	0.529 ng/ml
10) t 1,2,4-Trimethylbenzene	16.420	18671	0.728 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083019\
Data File : FB022268.D
Signal(s) : FID2B.CH
Acq On : 30 Aug 2019 12:18
Operator : DD/AJ
Sample : K4608-01
Misc : 5.02/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 30 14:03:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

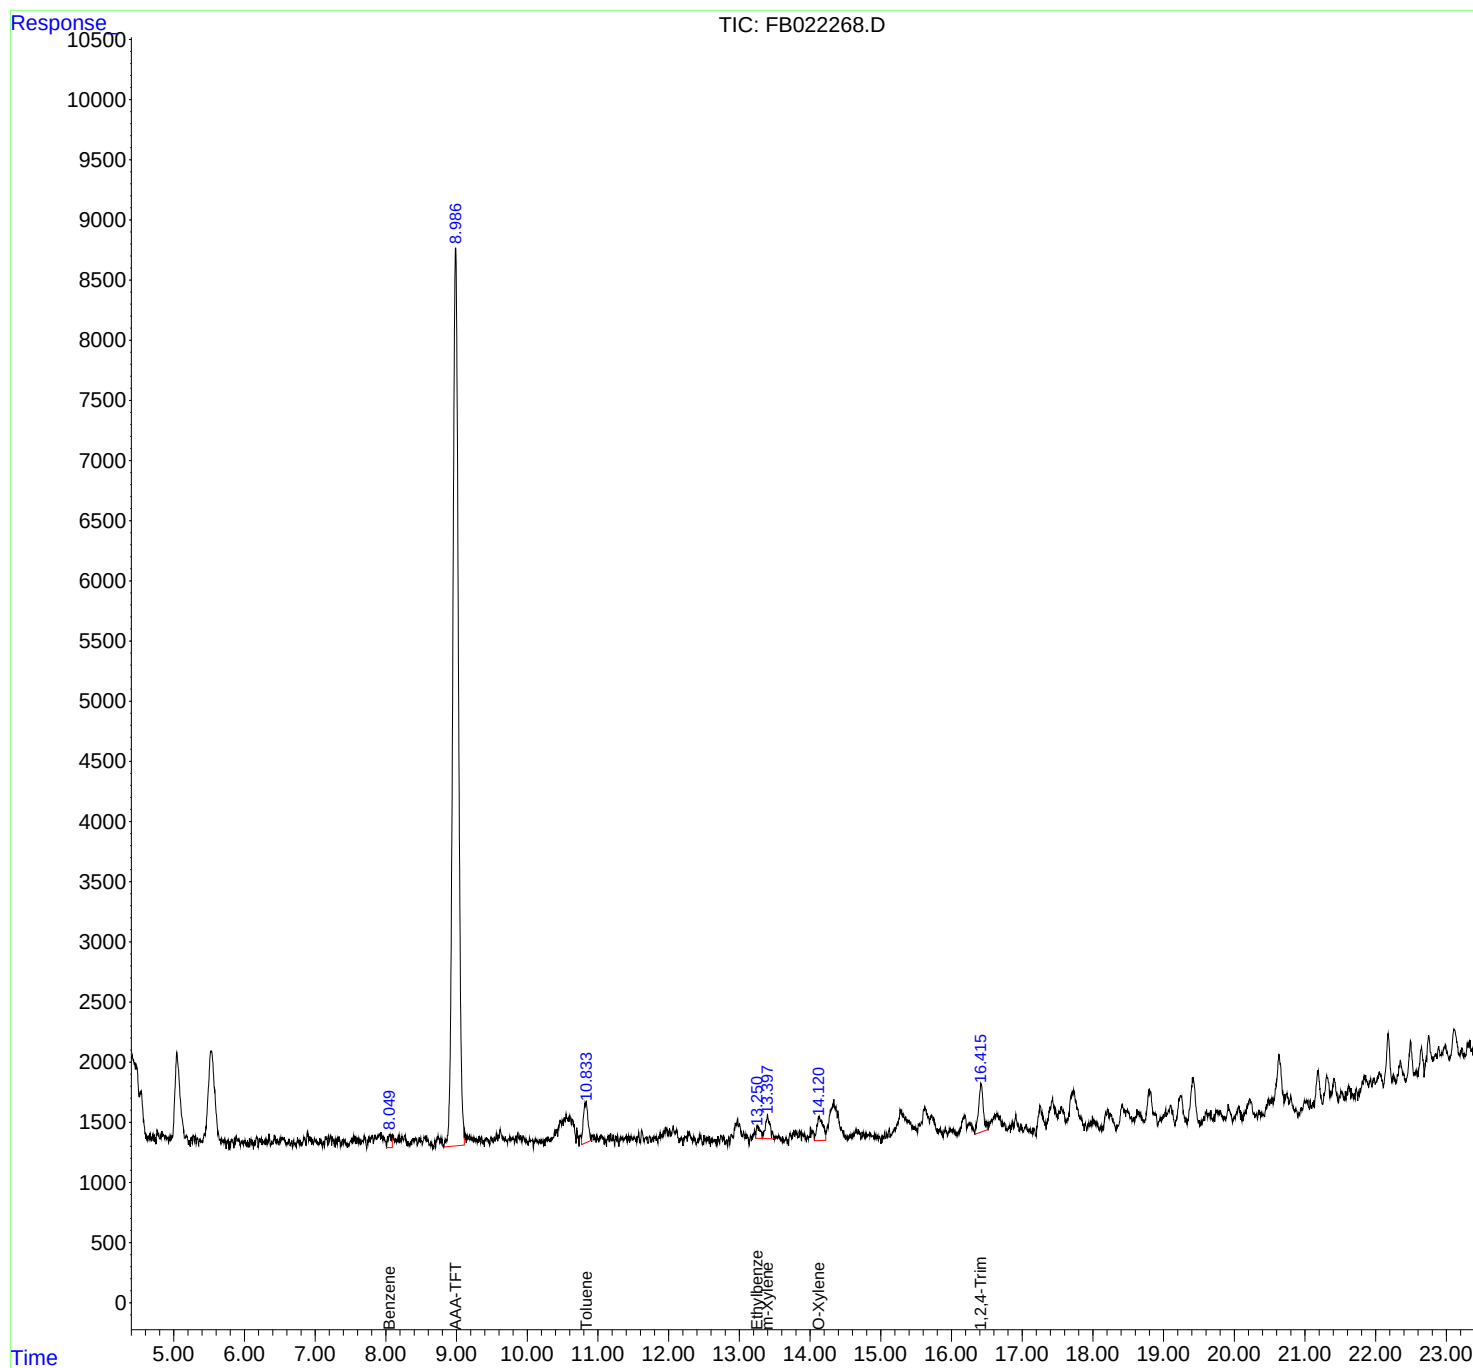


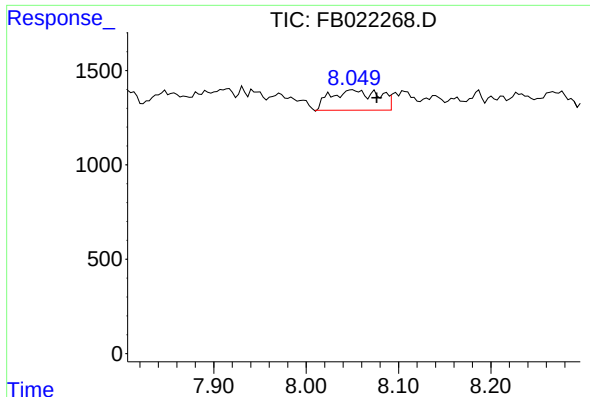

#4 Benzene


R.T.: 8.050 min
Delta R.T.: -0.026 min
Response: 3849
Conc: 0.09 ng/ml

Instrument :
FID_B
ClientSampleId :

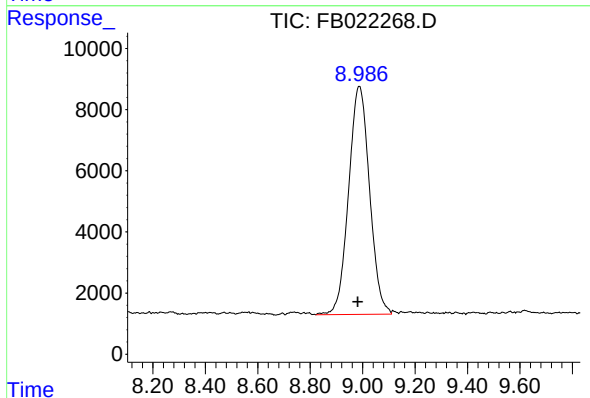


#5 AAA-TFT

R.T.: 8.988 min
Delta R.T.: 0.006 min
Response: 413785
Conc: 19.48 ng/ml

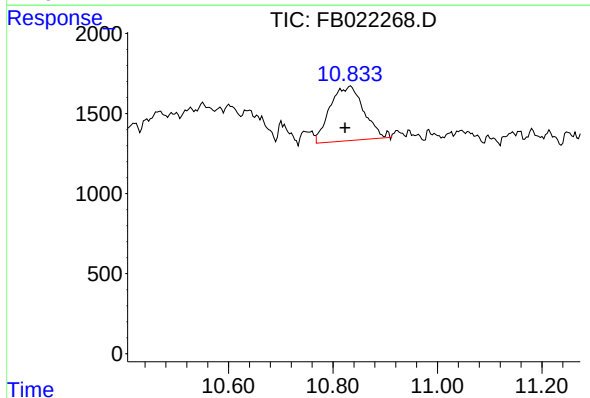


#6 Toluene

R.T.: 10.834 min
Delta R.T.: 0.011 min
Response: 15171
Conc: 0.49 ng/ml

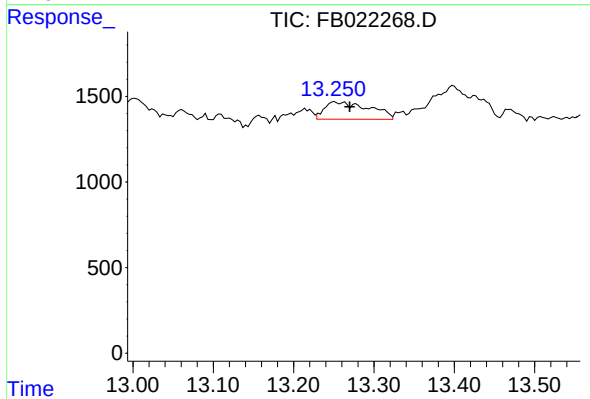

#7 Ethylbenzene


R.T.: 13.251 min
Delta R.T.: -0.019 min
Response: 3915
Conc: 0.19 ng/ml

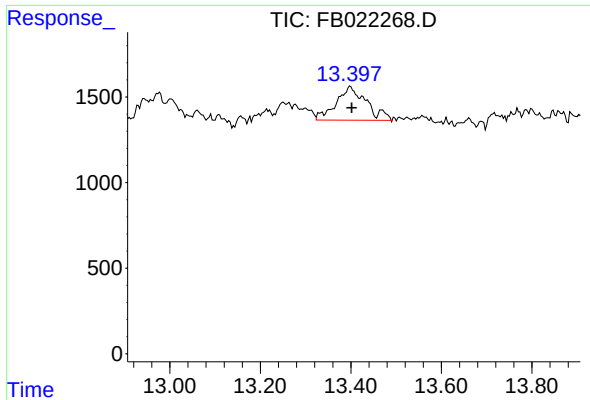

#8 m-Xylene


R.T.: 13.399 min
Delta R.T.: -0.002 min
Response: 9052
Conc: 0.43 ng/ml

Instrument :
FID_B
ClientSampleId :

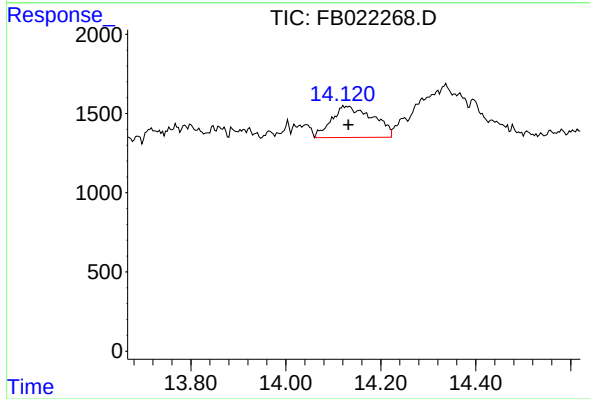

#9 O-Xylene

R.T.: 14.128 min
Delta R.T.: -0.003 min
Response: 11838
Conc: 0.53 ng/ml

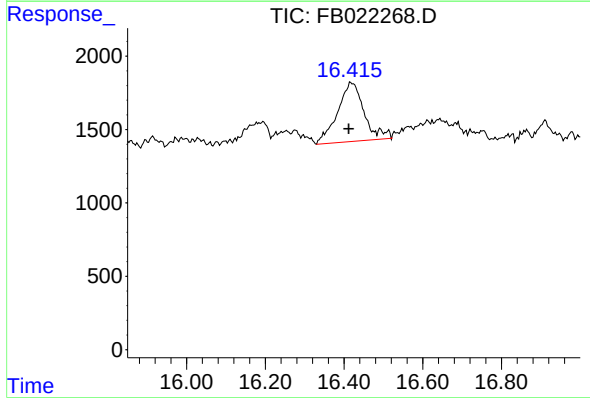

#10 1,2,4-Trimethylbenzene

R.T.: 16.420 min
Delta R.T.: 0.008 min
Response: 18671
Conc: 0.73 ng/ml