

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083019\
 Data File : FB022263.D
 Signal(s) : FID2B.CH
 Acq On : 30 Aug 2019 9:44
 Operator : DD/AJ
 Sample : BSF0830S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0830S1

Integration File: Calibration.e
 Quant Time: Aug 30 14:03:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.987	406756	19.150 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.856	1143166	28.563 ng/ml
2) t	2,2,4-Trimethylpentane	7.606	1086580	26.977 ng/ml
3) t	n-Heptane	7.946	343829	9.001 ng/ml
4) t	Benzene	8.080	416939	9.287 ng/ml
6) t	Toluene	10.827	807651	26.272 ng/ml
7) t	Ethylbenzene	13.273	214534	10.513 ng/ml
8) t	m-Xylene	13.406	454830	21.596 ng/ml
9) t	O-Xylene	14.135	478344	21.388 ng/ml
10) t	1,2,4-Trimethylbenzene	16.415	512682	19.991 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083019\
Data File : FB022263.D
Signal(s) : FID2B.CH
Acq On : 30 Aug 2019 9:44
Operator : DD/AJ
Sample : BSF0830S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0830S1

Integration File: Calibration.e
Quant Time: Aug 30 14:03:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

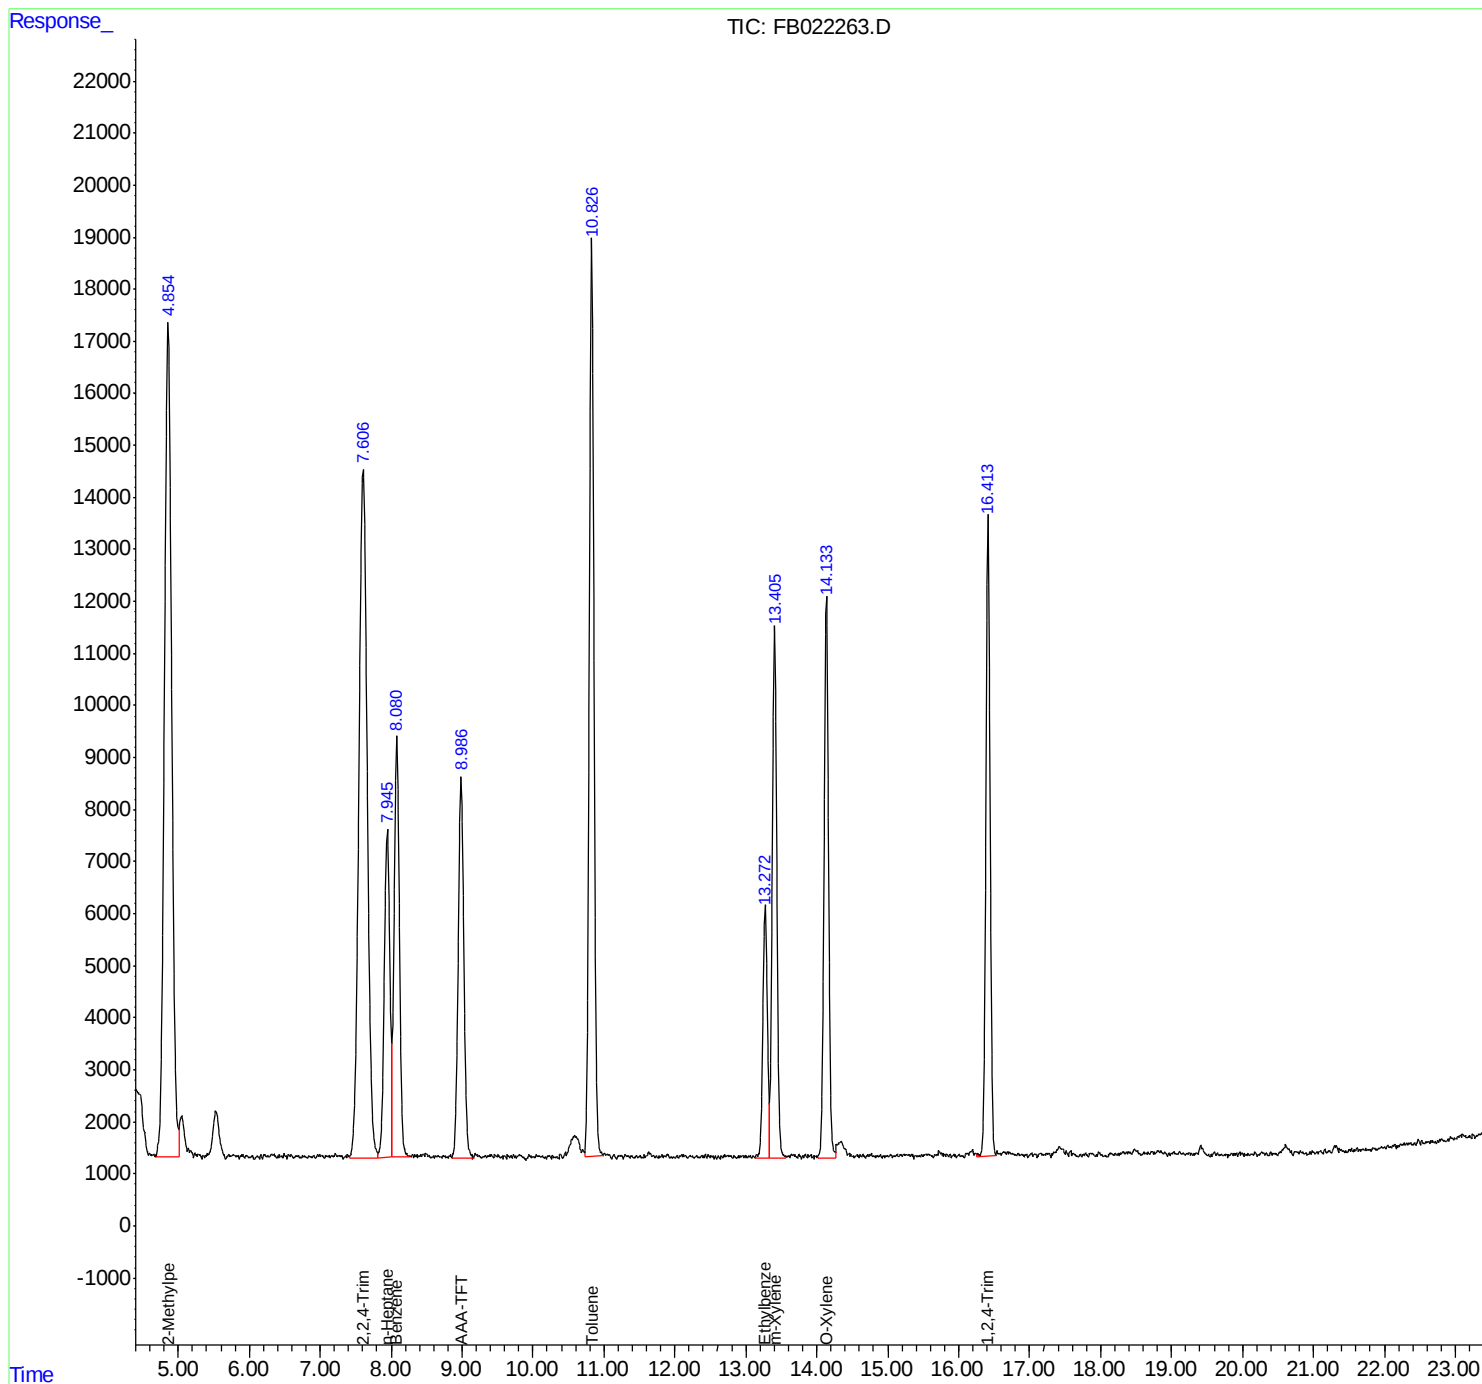


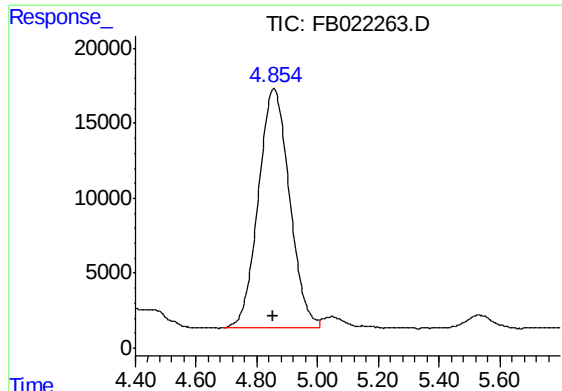

#1 2-Methylpentane


R.T.: 4.856 min
Delta R.T.: 0.004 min
Response: 1143166
Conc: 28.56 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0830S1

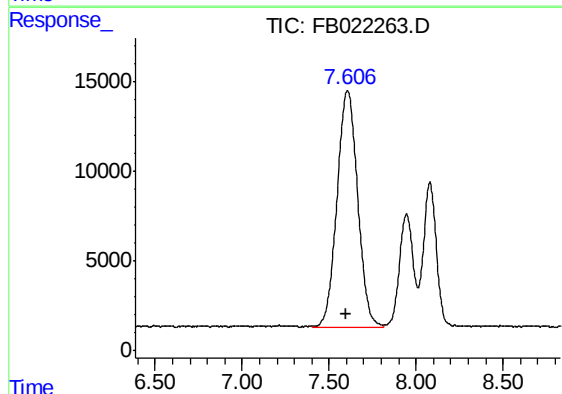


#2 2,2,4-Trimethylpentane

R.T.: 7.606 min
Delta R.T.: 0.007 min
Response: 1086580
Conc: 26.98 ng/ml

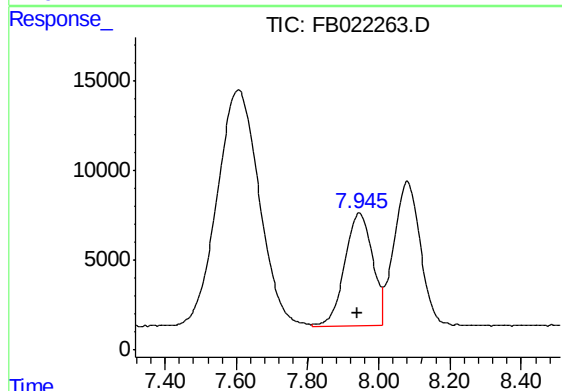


#3 n-Heptane

R.T.: 7.946 min
Delta R.T.: 0.005 min
Response: 343829
Conc: 9.00 ng/ml

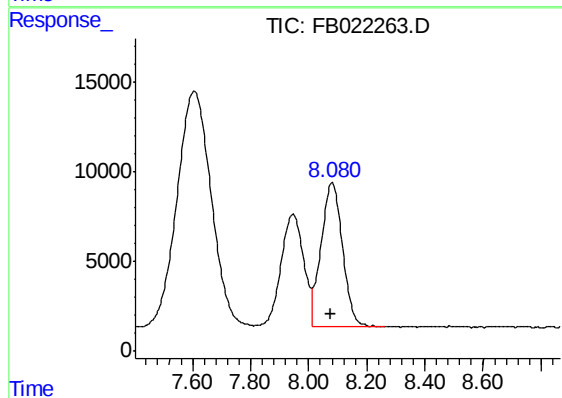

#4 Benzene


R.T.: 8.080 min
Delta R.T.: 0.004 min
Response: 416939
Conc: 9.29 ng/ml

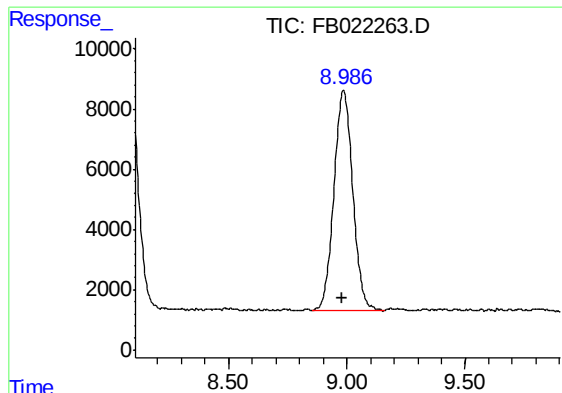

#5 AAA-TFT


R.T.: 8.987 min
Delta R.T.: 0.005 min
Response: 406756
Conc: 19.15 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0830S1

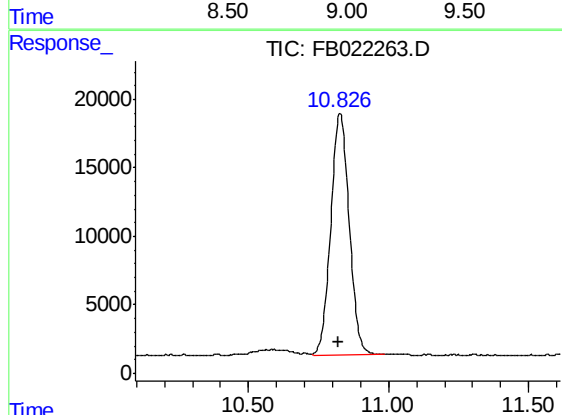


#6 Toluene

R.T.: 10.827 min
Delta R.T.: 0.005 min
Response: 807651
Conc: 26.27 ng/ml

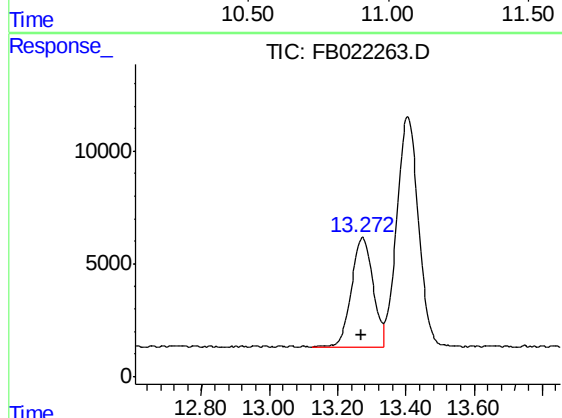


#7 Ethylbenzene

R.T.: 13.273 min
Delta R.T.: 0.004 min
Response: 214534
Conc: 10.51 ng/ml

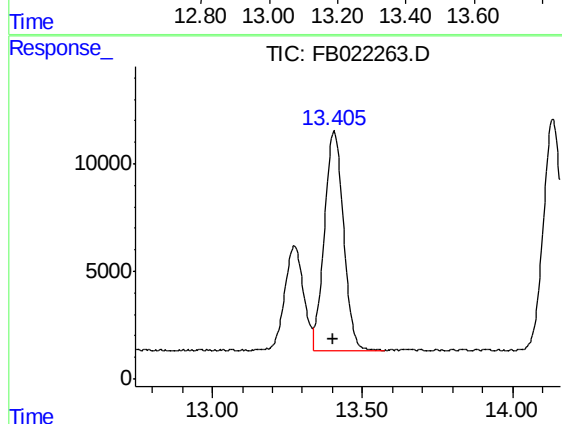

#8 m-Xylene


R.T.: 13.406 min
Delta R.T.: 0.004 min
Response: 454830
Conc: 21.60 ng/ml

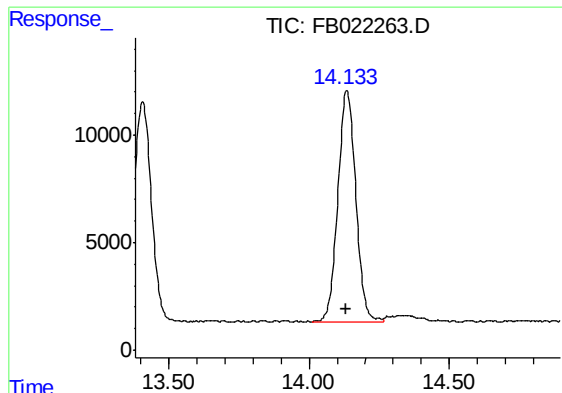

#9 O-Xylene

R.T.: 14.135 min
Delta R.T.: 0.003 min
Response: 478344
Conc: 21.39 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0830S1

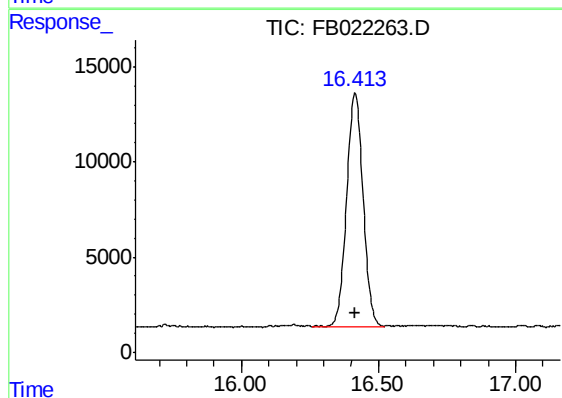

#10 1,2,4-Trimethylbenzene

R.T.: 16.415 min
Delta R.T.: 0.003 min
Response: 512682
Conc: 19.99 ng/ml