

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083019\
 Data File : FB022265.D
 Signal(s) : FID2B.CH
 Acq On : 30 Aug 2019 10:46
 Operator : DD/AJ
 Sample : K4090-18MS
 Misc : 5.00/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OR-02-082919-1MS

Integration File: Calibration.e
 Quant Time: Aug 30 14:03:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.987	429911	20.240 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.856	1035780	25.880 ng/ml
2) t 2,2,4-Trimethylpentane	7.606	996693	24.746 ng/ml
3) t n-Heptane	7.945	310144	8.119 ng/ml
4) t Benzene	8.080	398028	8.866 ng/ml
6) t Toluene	10.828	789301	25.675 ng/ml
7) t Ethylbenzene	13.273	198818	9.743 ng/ml
8) t m-Xylene	13.405	422209	20.048 ng/ml
9) t O-Xylene	14.135	449225	20.086 ng/ml
10) t 1,2,4-Trimethylbenzene	16.415	483065	18.836 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083019\
Data File : FB022265.D
Signal(s) : FID2B.CH
Acq On : 30 Aug 2019 10:46
Operator : DD/AJ
Sample : K4090-18MS
Misc : 5.00/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OR-02-082919-1MS

Integration File: Calibration.e
Quant Time: Aug 30 14:03:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

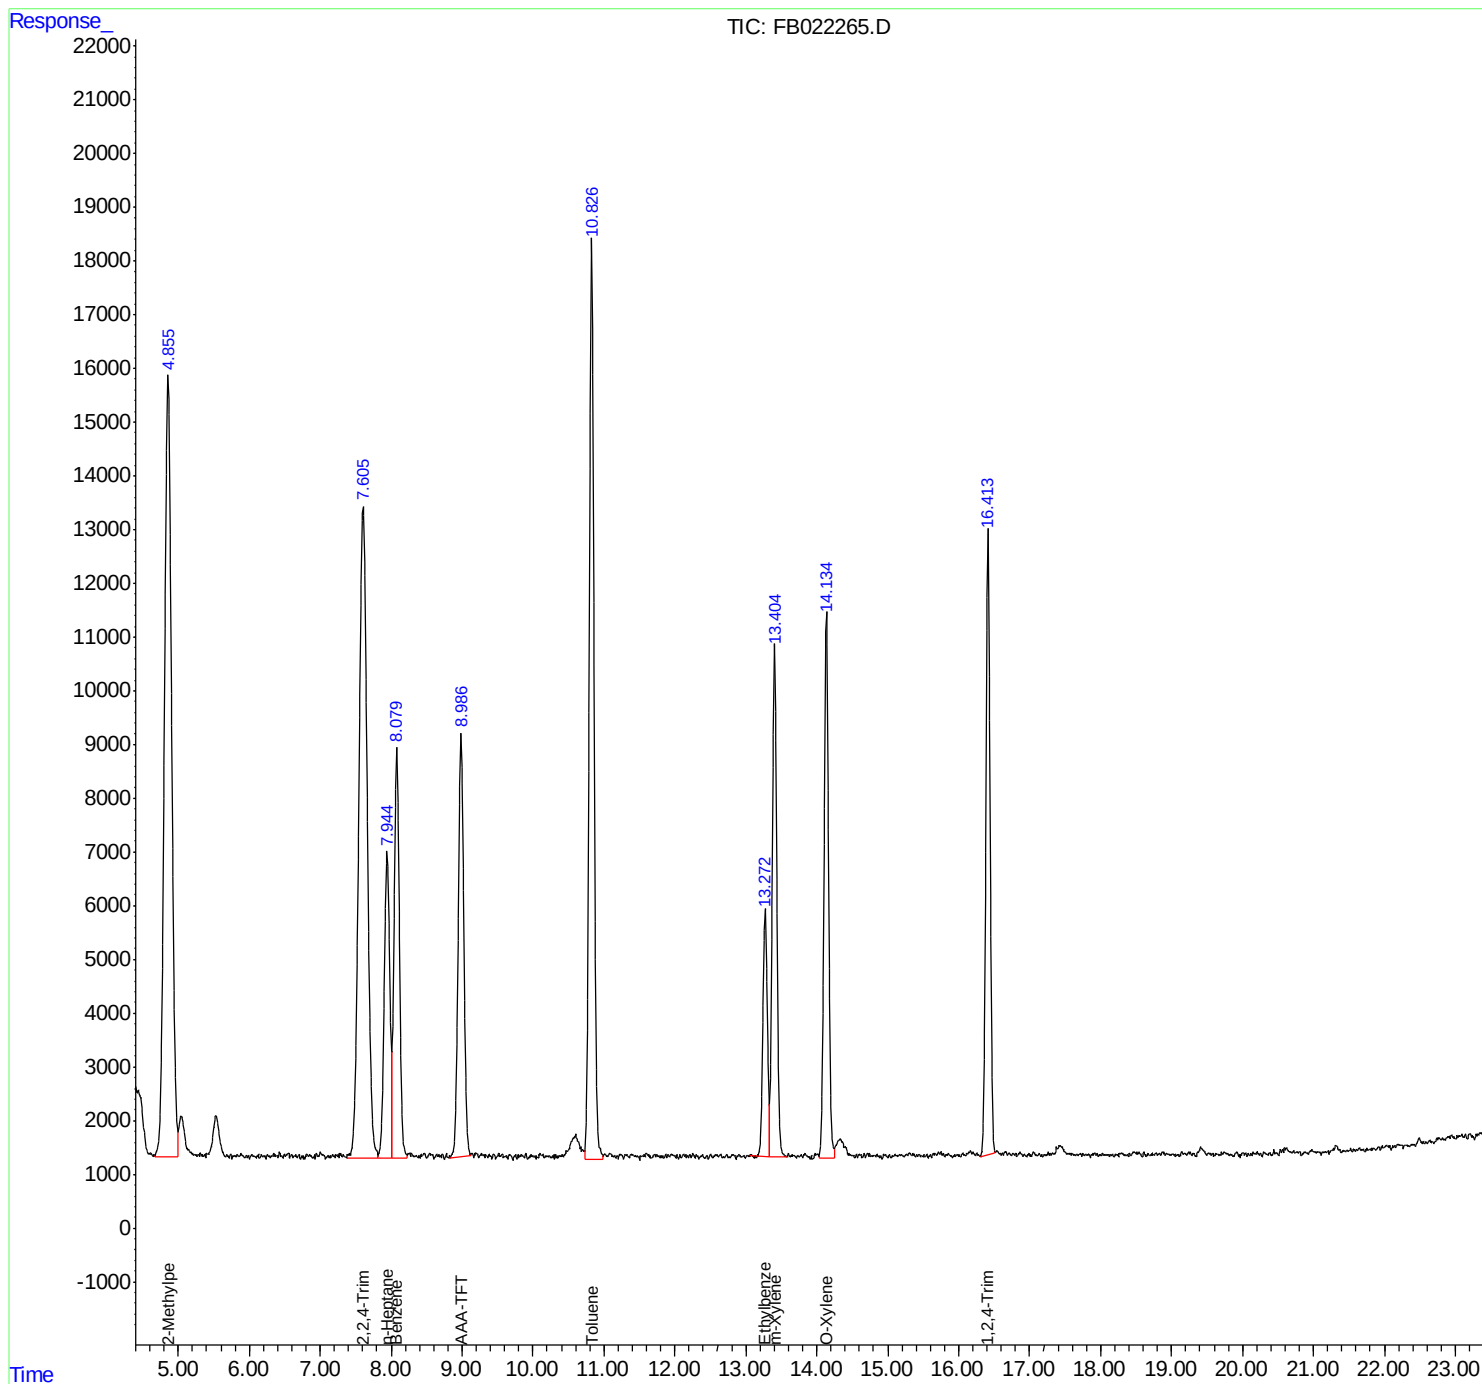


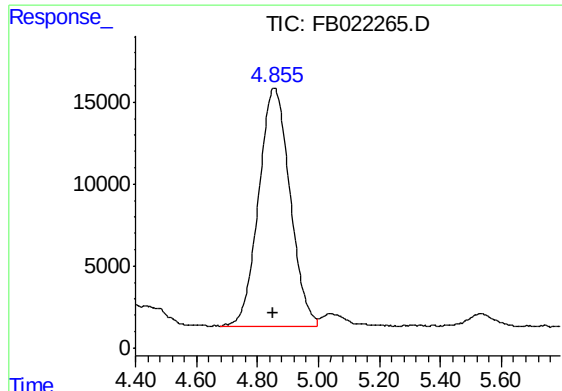

#1 2-Methylpentane


R.T.: 4.856 min
Delta R.T.: 0.004 min
Response: 1035780
Conc: 25.88 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-082919-1MS

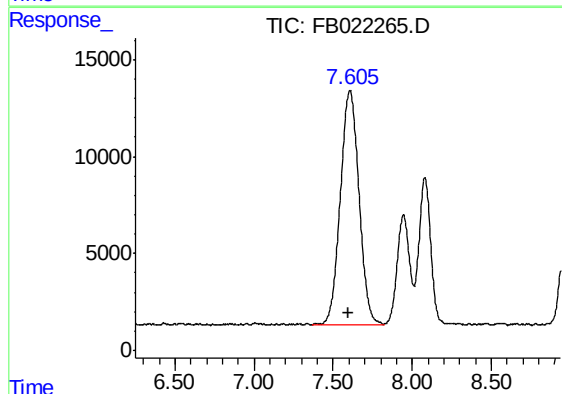


#2 2,2,4-Trimethylpentane

R.T.: 7.606 min
Delta R.T.: 0.006 min
Response: 996693
Conc: 24.75 ng/ml

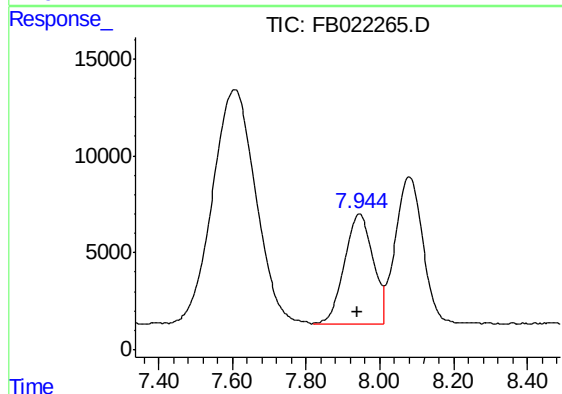


#3 n-Heptane

R.T.: 7.945 min
Delta R.T.: 0.003 min
Response: 310144
Conc: 8.12 ng/ml

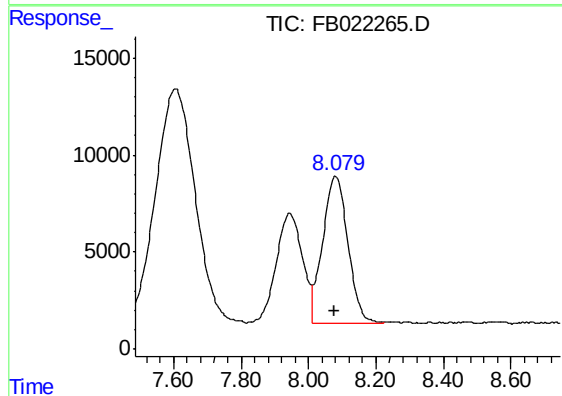

#4 Benzene


R.T.: 8.080 min
Delta R.T.: 0.004 min
Response: 398028
Conc: 8.87 ng/ml

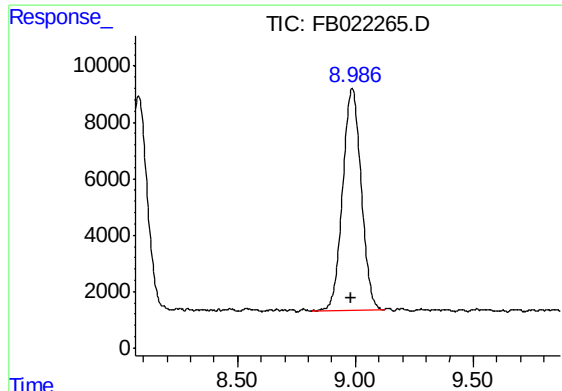

#5 AAA-TFT


R.T.: 8.987 min
Delta R.T.: 0.004 min
Response: 429911
Conc: 20.24 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-082919-1MS

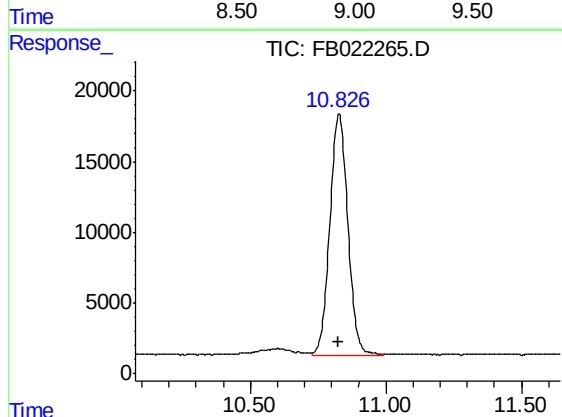


#6 Toluene

R.T.: 10.828 min
Delta R.T.: 0.005 min
Response: 789301
Conc: 25.67 ng/ml

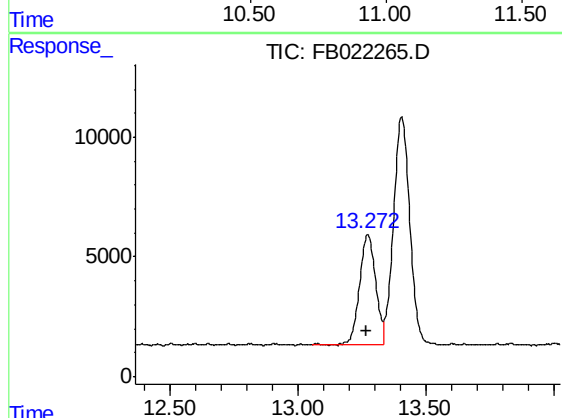


#7 Ethylbenzene

R.T.: 13.273 min
Delta R.T.: 0.004 min
Response: 198818
Conc: 9.74 ng/ml

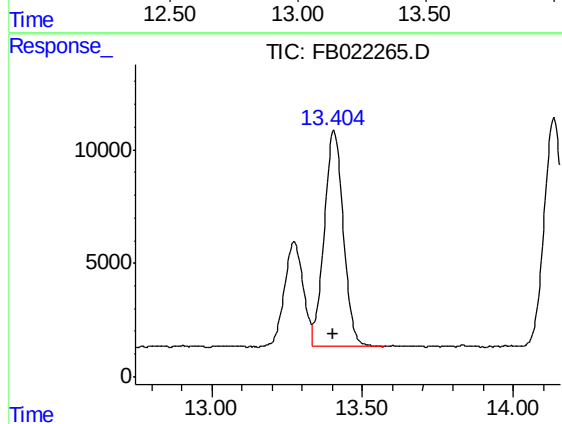

#8 m-Xylene


R.T.: 13.405 min
Delta R.T.: 0.004 min
Response: 422209
Conc: 20.05 ng/ml

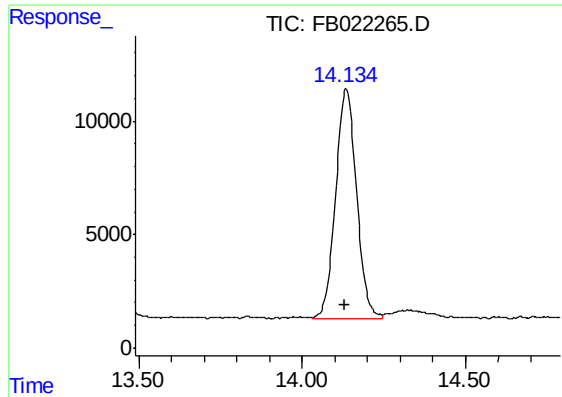

#9 O-Xylene

R.T.: 14.135 min
Delta R.T.: 0.004 min
Response: 449225
Conc: 20.09 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-082919-1MS

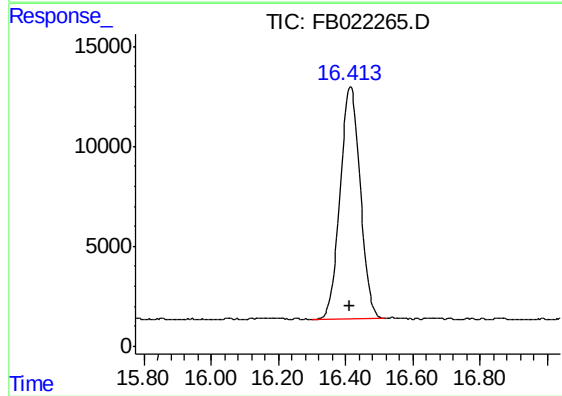

#10 1,2,4-Trimethylbenzene

R.T.: 16.415 min
Delta R.T.: 0.003 min
Response: 483065
Conc: 18.84 ng/ml