

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083019\
 Data File : FB022266.D
 Signal(s) : FID2B.CH
 Acq On : 30 Aug 2019 11:17
 Operator : DD/AJ
 Sample : K4090-18MSD
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OR-02-082919-1MSD

Integration File: Calibration.e
 Quant Time: Aug 30 14:03:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.988	442353	20.826 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.857	1123158	28.063 ng/ml
2) t 2,2,4-Trimethylpentane	7.607	1078588	26.779 ng/ml
3) t n-Heptane	7.946	335423	8.781 ng/ml
4) t Benzene	8.082	429121	9.559 ng/ml
6) t Toluene	10.829	843580	27.440 ng/ml
7) t Ethylbenzene	13.274	217903	10.678 ng/ml
8) t m-Xylene	13.407	463449	22.006 ng/ml
9) t O-Xylene	14.137	488961	21.863 ng/ml
10) t 1,2,4-Trimethylbenzene	16.416	519862	20.271 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083019\
Data File : FB022266.D
Signal(s) : FID2B.CH
Acq On : 30 Aug 2019 11:17
Operator : DD/AJ
Sample : K4090-18MSD
Misc : 5.01/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OR-02-082919-1MSD

Integration File: Calibration.e
Quant Time: Aug 30 14:03:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

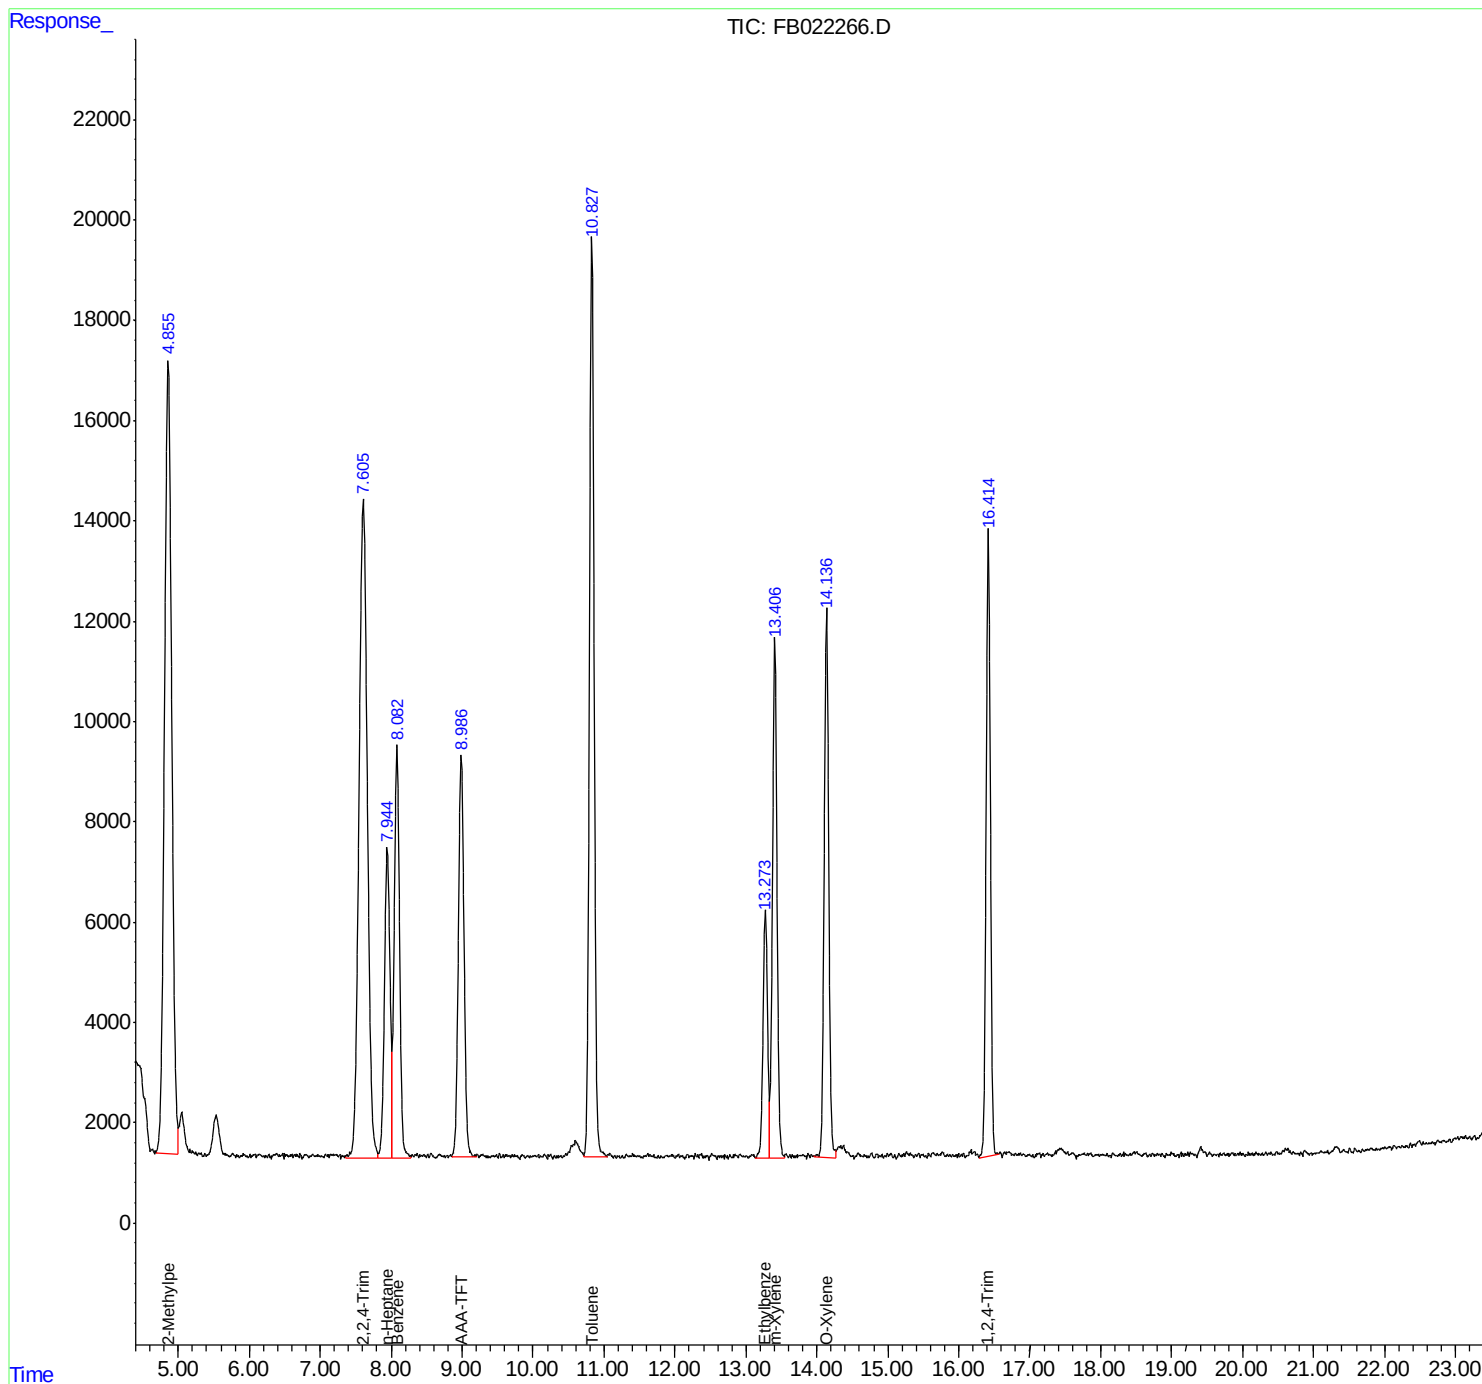


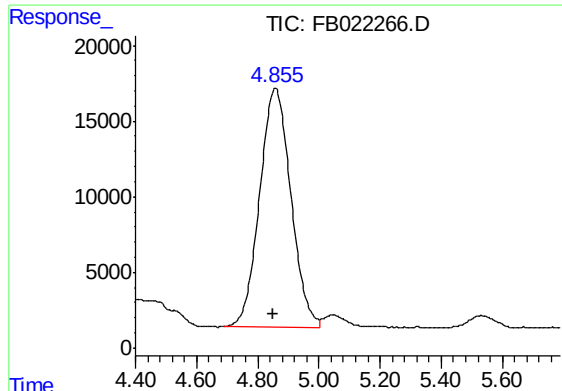

#1 2-Methylpentane


R.T.: 4.857 min
Delta R.T.: 0.005 min
Response: 1123158
Conc: 28.06 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-082919-1MSD

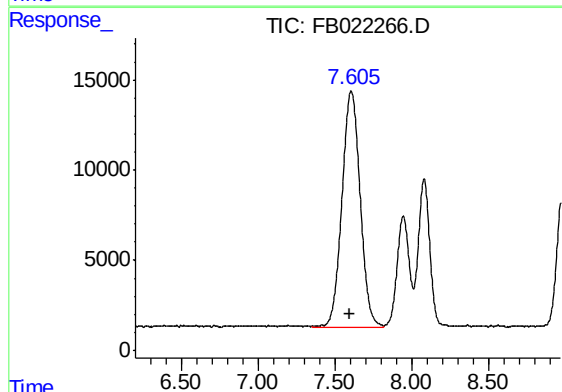


#2 2,2,4-Trimethylpentane

R.T.: 7.607 min
Delta R.T.: 0.007 min
Response: 1078588
Conc: 26.78 ng/ml

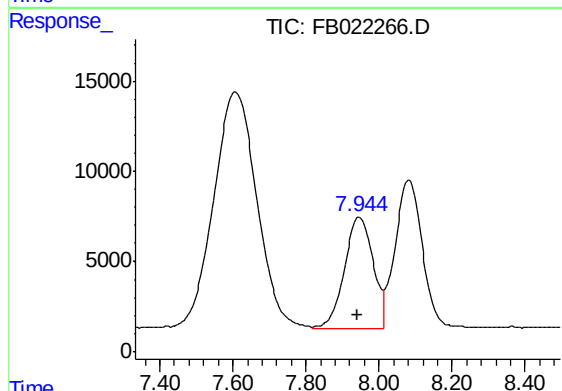


#3 n-Heptane

R.T.: 7.946 min
Delta R.T.: 0.005 min
Response: 335423
Conc: 8.78 ng/ml

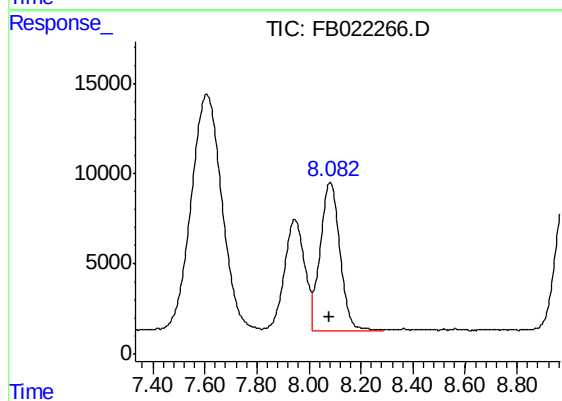

#4 Benzene


R.T.: 8.082 min
Delta R.T.: 0.006 min
Response: 429121
Conc: 9.56 ng/ml

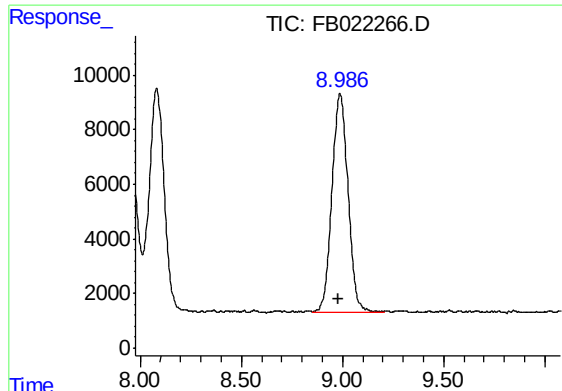

#5 AAA-TFT


R.T.: 8.988 min
Delta R.T.: 0.006 min
Response: 442353
Conc: 20.83 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-082919-1MSD

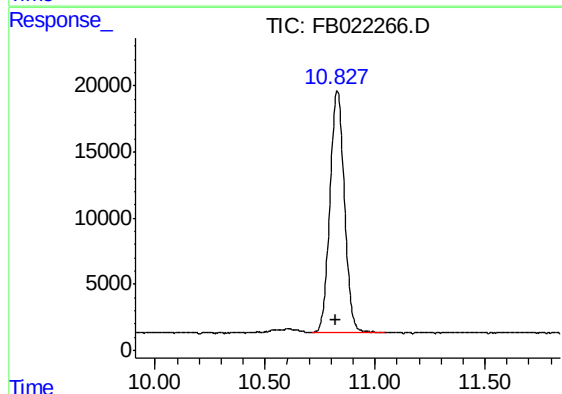


#6 Toluene

R.T.: 10.829 min
Delta R.T.: 0.006 min
Response: 843580
Conc: 27.44 ng/ml

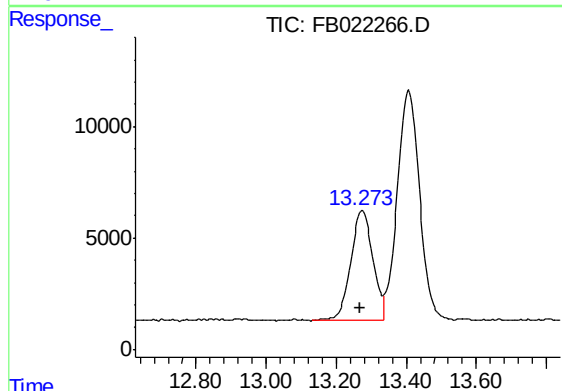


#7 Ethylbenzene

R.T.: 13.274 min
Delta R.T.: 0.005 min
Response: 217903
Conc: 10.68 ng/ml

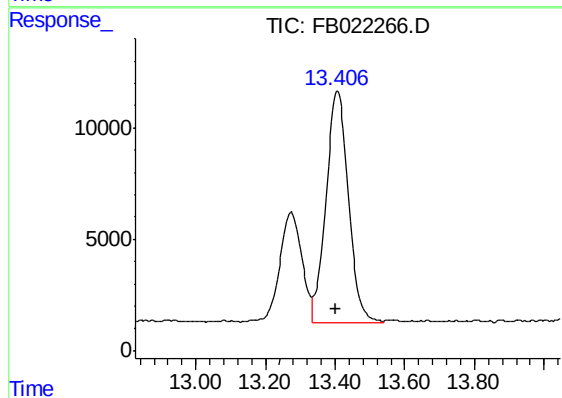

#8 m-Xylene


R.T.: 13.407 min
Delta R.T.: 0.005 min
Response: 463449
Conc: 22.01 ng/ml

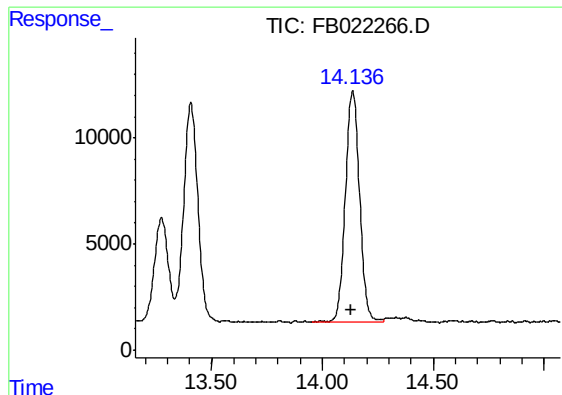

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: 0.005 min
Response: 488961
Conc: 21.86 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-02-082919-1MSD

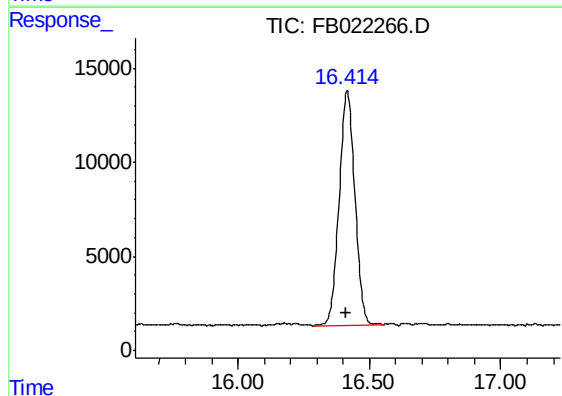

#10 1,2,4-Trimethylbenzene

R.T.: 16.416 min
Delta R.T.: 0.004 min
Response: 519862
Conc: 20.27 ng/ml