

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083022\
 Data File : FB028060.D
 Signal(s) : FID2B.CH
 Acq On : 30 Aug 2022 8:55
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 31 04:32:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	277273	23.925 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.714	565562	31.262 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	601325	30.664 ng/ml
3) t n-Heptane	7.755	181830	9.438 ng/ml
4) t Benzene	7.891	227499	9.784 ng/ml
6) t Toluene	10.625	637986	29.095 ng/ml
7) t Ethylbenzene	13.061	202057	9.805 ng/ml
8) t m-Xylene	13.194	401681	19.630 ng/ml
9) t O-Xylene	13.921	399129	20.149 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	412358	21.146 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083022\
Data File : FB028060.D
Signal(s) : FID2B.CH
Acq On : 30 Aug 2022 8:55
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 31 04:32:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

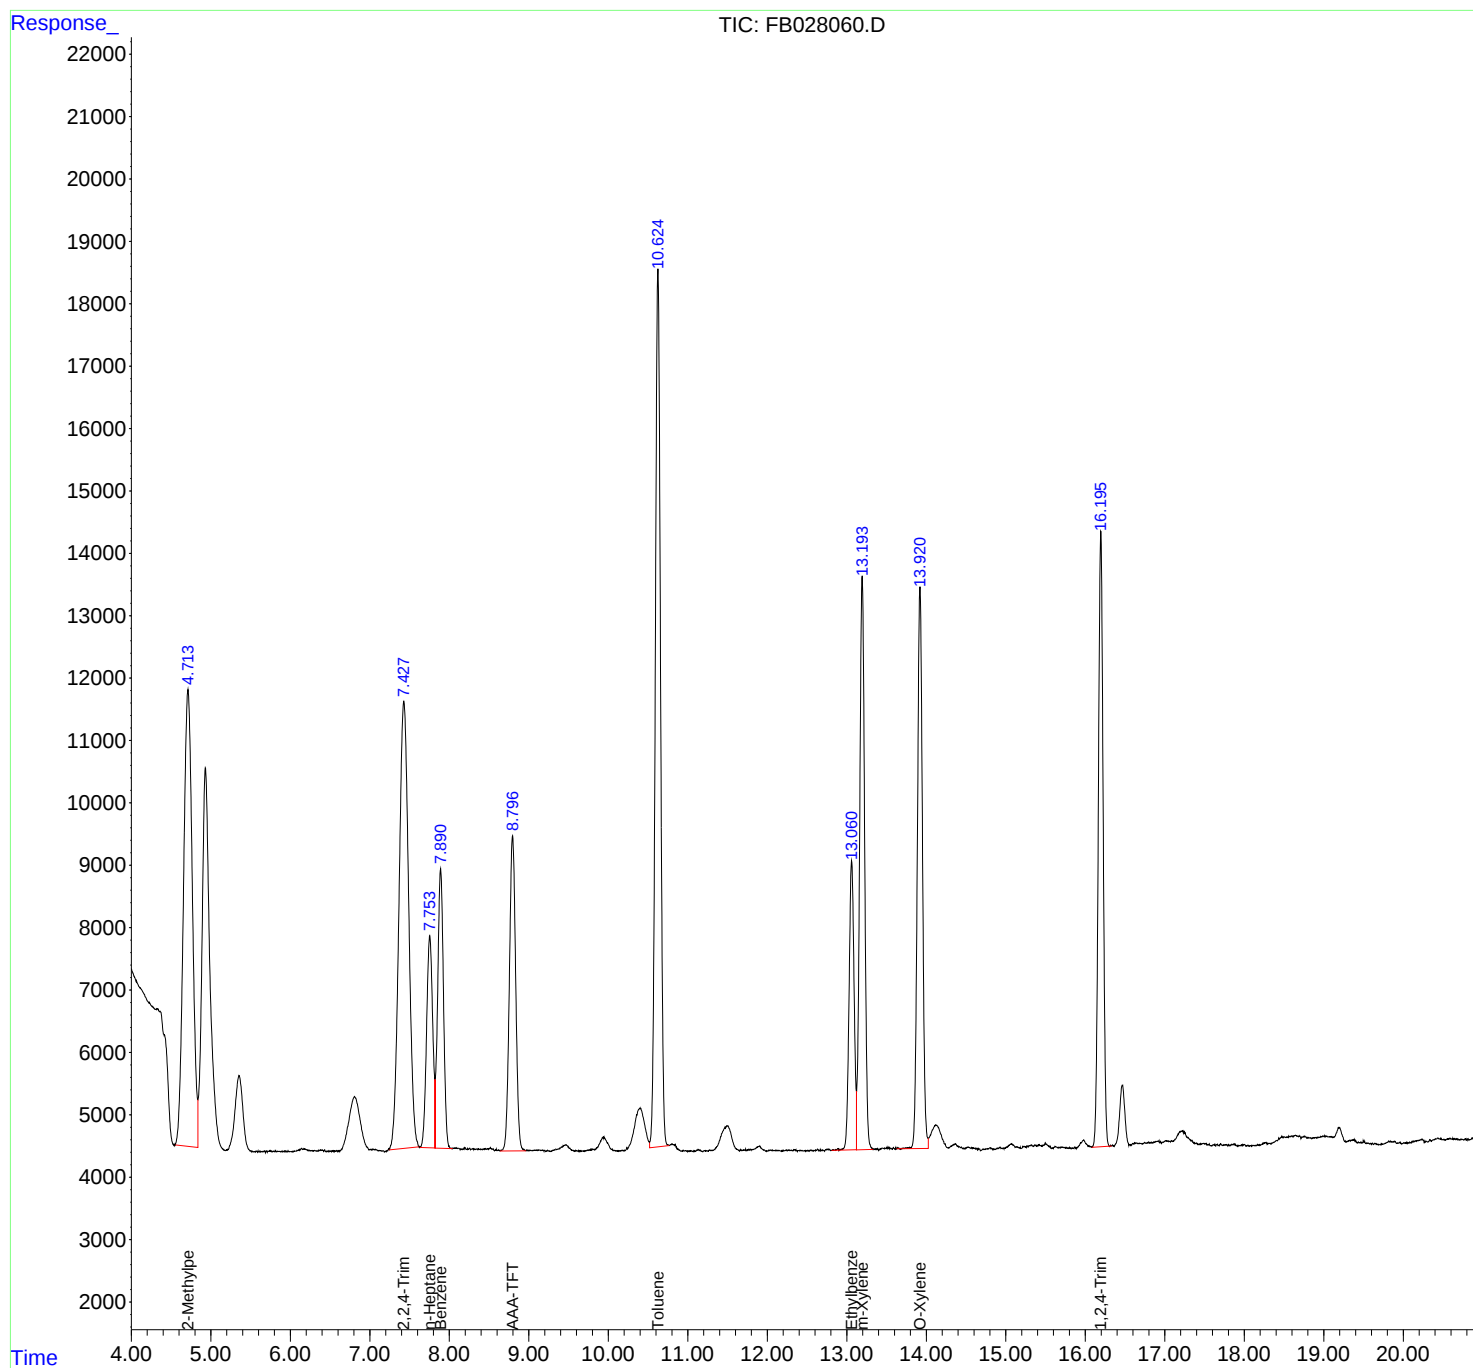


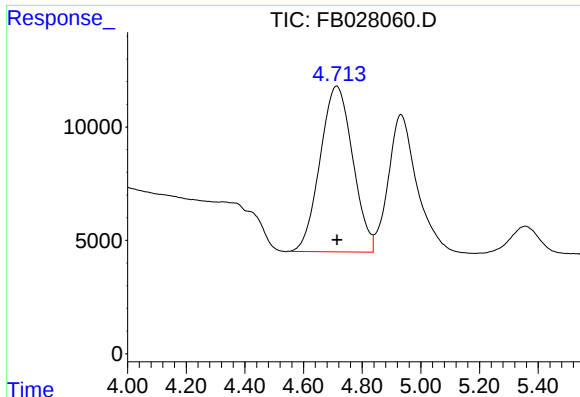

#1 2-Methylpentane


R.T.: 4.714 min
Delta R.T.: 0.000 min
Response: 565562
Conc: 31.26 ng/ml

Instrument :
FID_B
ClientSampleId :

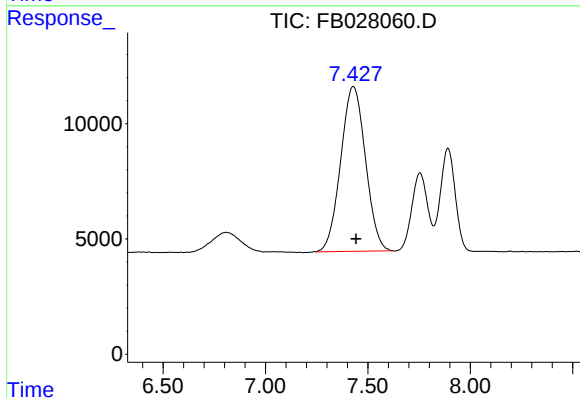


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: -0.014 min
Response: 601325
Conc: 30.66 ng/ml

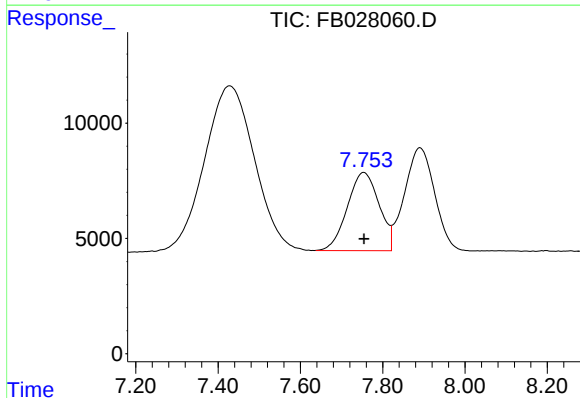


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 181830
Conc: 9.44 ng/ml

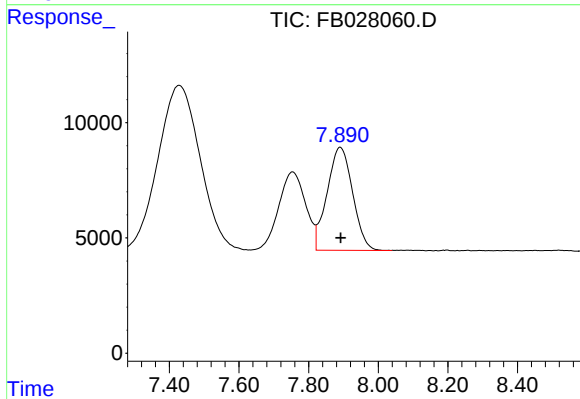

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.001 min
Response: 227499
Conc: 9.78 ng/ml

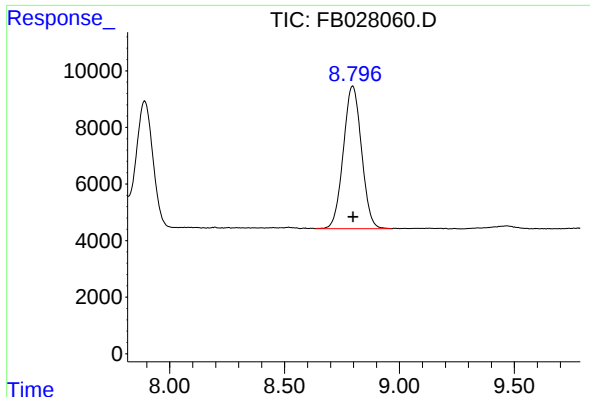

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.001 min
Response: 277273
Conc: 23.92 ng/ml

Instrument :
FID_B
ClientSampleId :

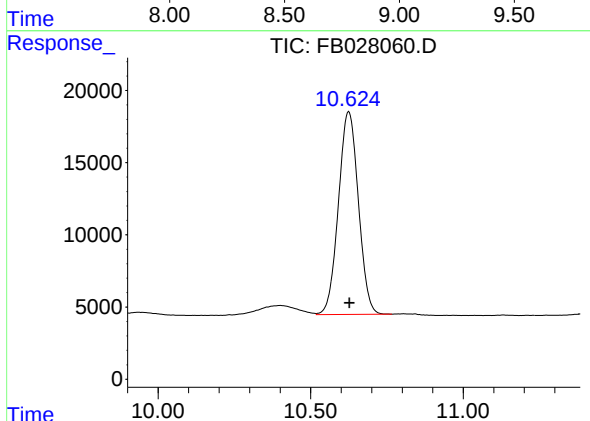


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.002 min
Response: 637986
Conc: 29.09 ng/ml

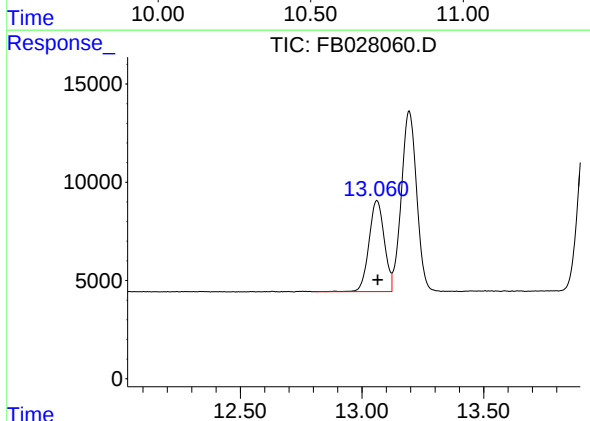


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: -0.003 min
Response: 202057
Conc: 9.81 ng/ml

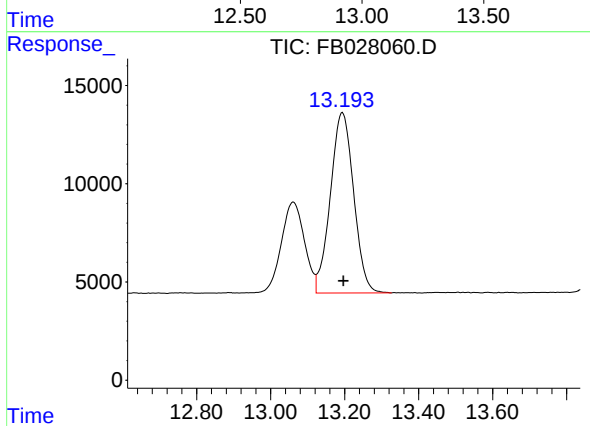

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: -0.003 min
Response: 401681
Conc: 19.63 ng/ml

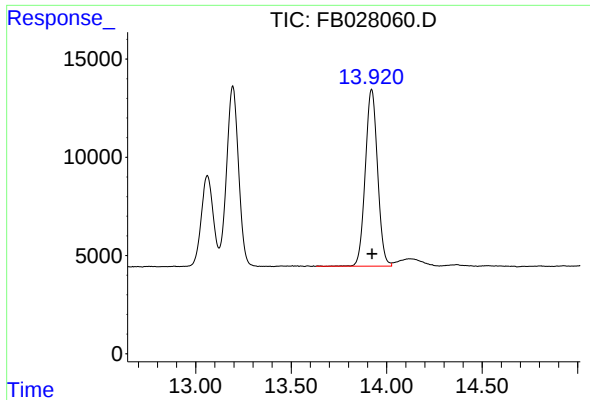

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: -0.003 min
Response: 399129
Conc: 20.15 ng/ml

Instrument :
FID_B
ClientSampleId :

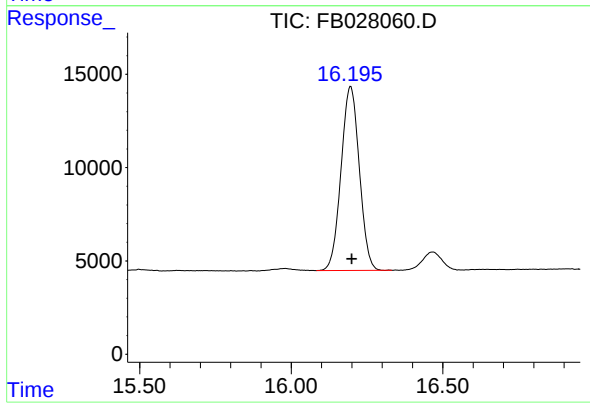

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: -0.003 min
Response: 412358
Conc: 21.15 ng/ml