

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083022\
 Data File : FB028063.D
 Signal(s) : FID2B.CH
 Acq On : 30 Aug 2022 11:02
 Operator : AJ/MA
 Sample : BSF0830S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0830S1

Integration File: SAMPLE.e
 Quant Time: Aug 31 04:32:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	253975	21.915 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	525422	29.044 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	553817	28.241 ng/ml
3) t n-Heptane	7.757	177270	9.202 ng/ml
4) t Benzene	7.895	212221	9.127 ng/ml
6) t Toluene	10.628	597687	27.257 ng/ml
7) t Ethylbenzene	13.065	189219	9.182 ng/ml
8) t m-Xylene	13.197	375006	18.326 ng/ml
9) t O-Xylene	13.924	364723	18.412 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	356853	18.299 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083022\
Data File : FB028063.D
Signal(s) : FID2B.CH
Acq On : 30 Aug 2022 11:02
Operator : AJ/MA
Sample : BSF0830S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0830S1

Integration File: SAMPLE.e
Quant Time: Aug 31 04:32:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

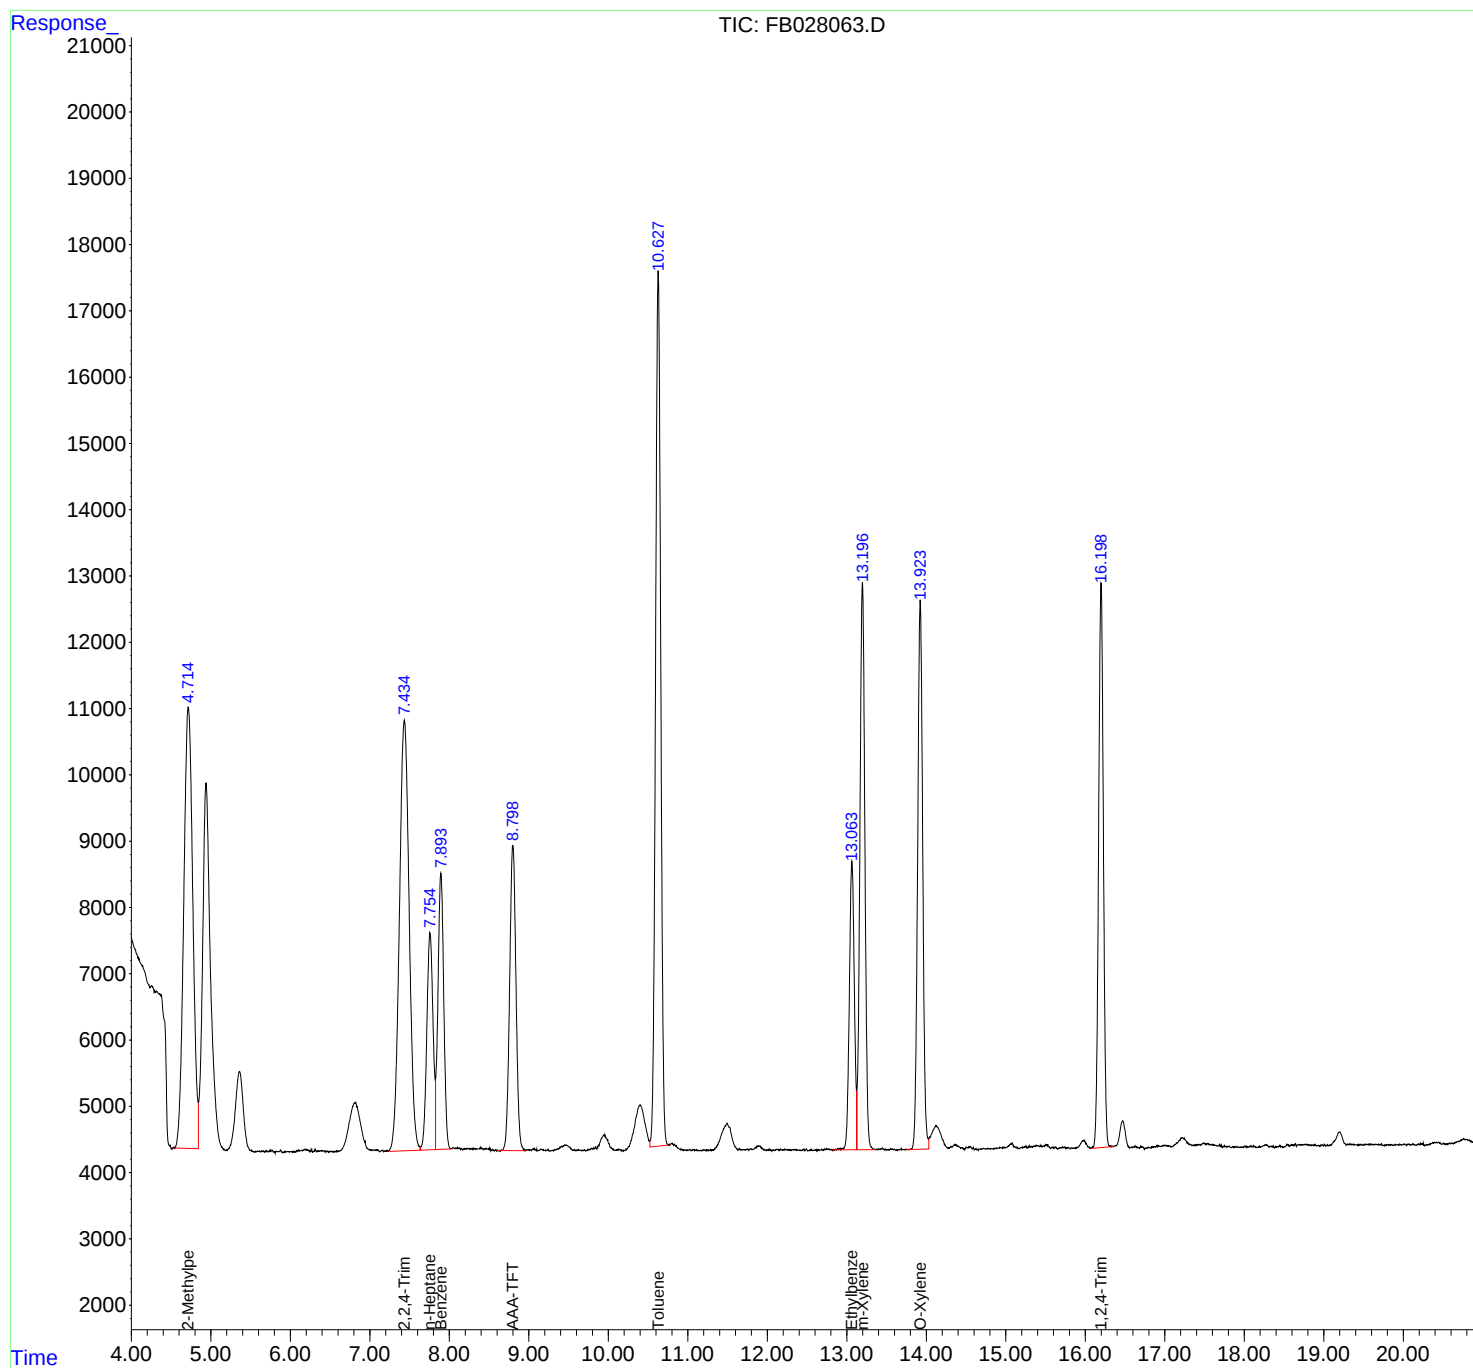


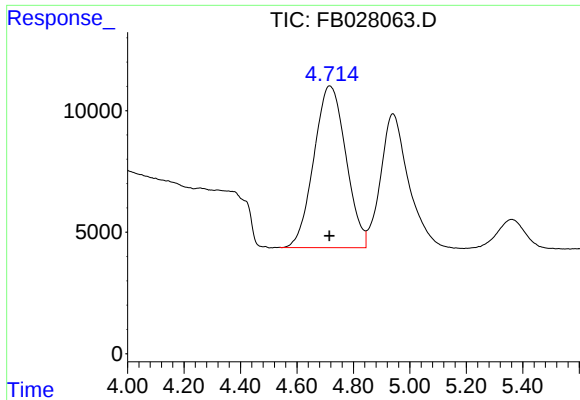

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: 0.001 min
Response: 525422
Conc: 29.04 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0830S1

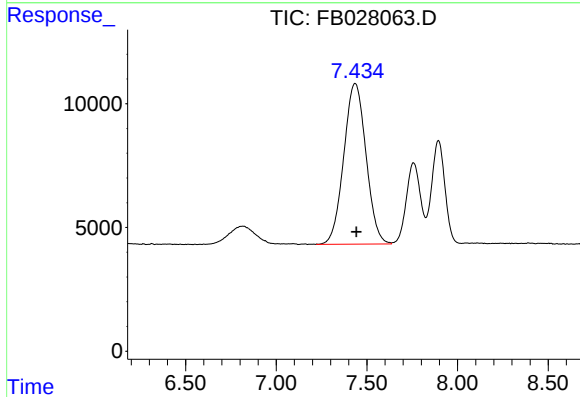


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: -0.008 min
Response: 553817
Conc: 28.24 ng/ml

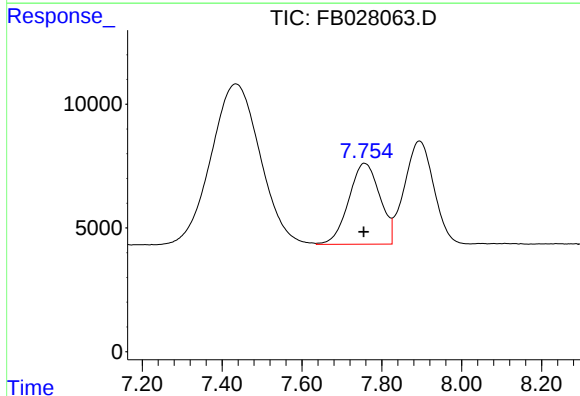


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.002 min
Response: 177270
Conc: 9.20 ng/ml

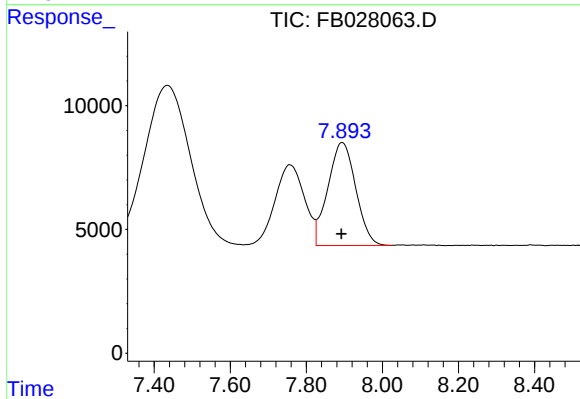

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.003 min
Response: 212221
Conc: 9.13 ng/ml

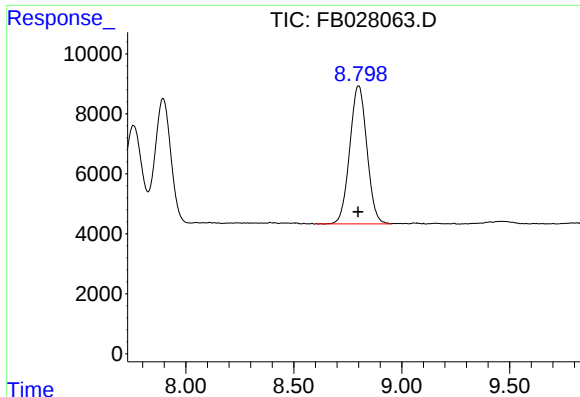

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.002 min
Response: 253975
Conc: 21.91 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0830S1

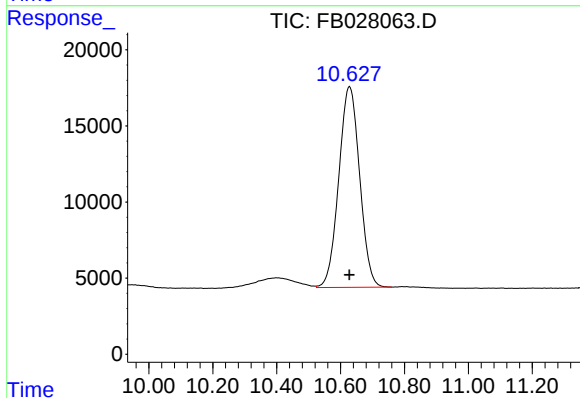


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.001 min
Response: 597687
Conc: 27.26 ng/ml

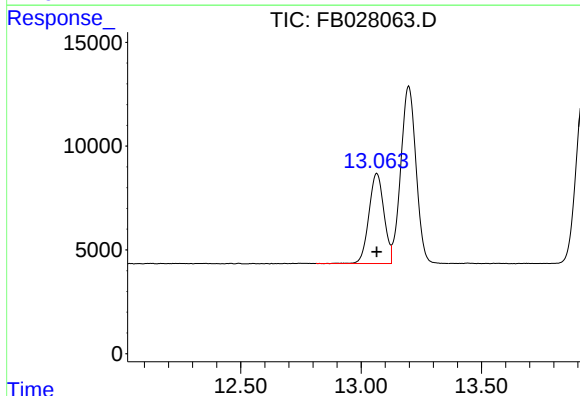


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: 0.000 min
Response: 189219
Conc: 9.18 ng/ml

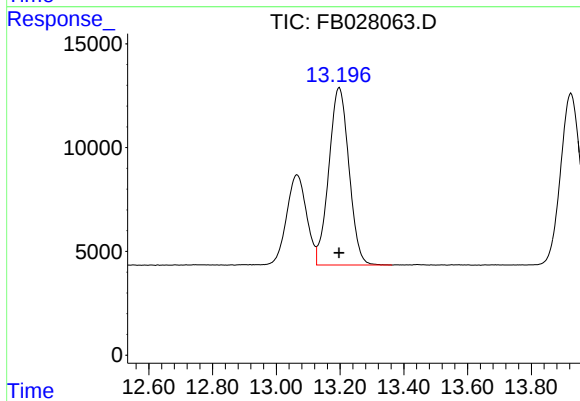

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.000 min
Response: 375006
Conc: 18.33 ng/ml

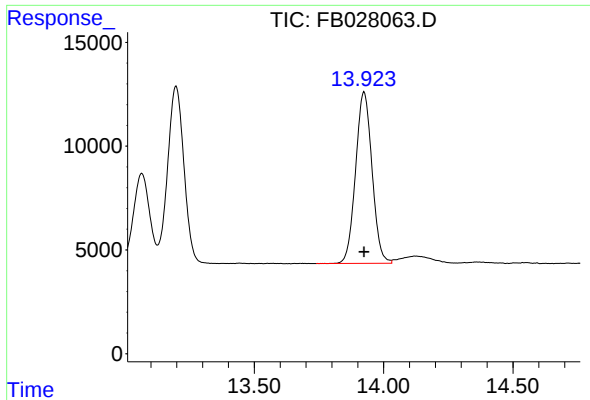

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.000 min
Response: 364723
Conc: 18.41 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0830S1

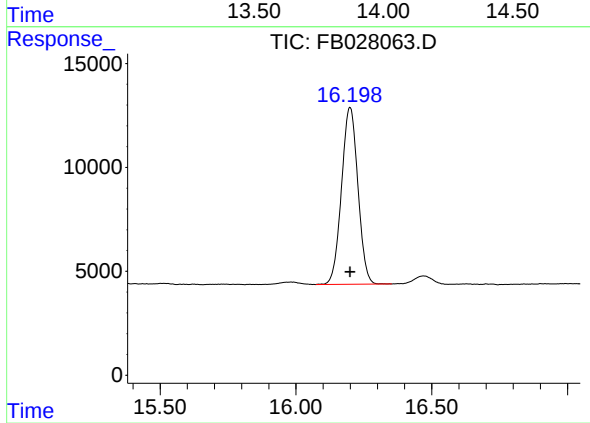

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.000 min
Response: 356853
Conc: 18.30 ng/ml