

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083022\
 Data File : FB028065.D
 Signal(s) : FID2B.CH
 Acq On : 30 Aug 2022 12:18
 Operator : AJ/MA
 Sample : BSF0830S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0830S2

Integration File: SAMPLE.e
 Quant Time: Aug 31 04:32:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	231938	20.013 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	564907	31.226 ng/ml
2) t 2,2,4-Trimethylpentane	7.436	594168	30.299 ng/ml
3) t n-Heptane	7.759	184176	9.560 ng/ml
4) t Benzene	7.897	219584	9.444 ng/ml
6) t Toluene	10.630	632793	28.858 ng/ml
7) t Ethylbenzene	13.066	198924	9.653 ng/ml
8) t m-Xylene	13.199	395425	19.324 ng/ml
9) t O-Xylene	13.926	404491	20.419 ng/ml
10) t 1,2,4-Trimethylbenzene	16.200	423885	21.737 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083022\
Data File : FB028065.D
Signal(s) : FID2B.CH
Acq On : 30 Aug 2022 12:18
Operator : AJ/MA
Sample : BSF0830S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0830S2

Integration File: SAMPLE.e
Quant Time: Aug 31 04:32:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

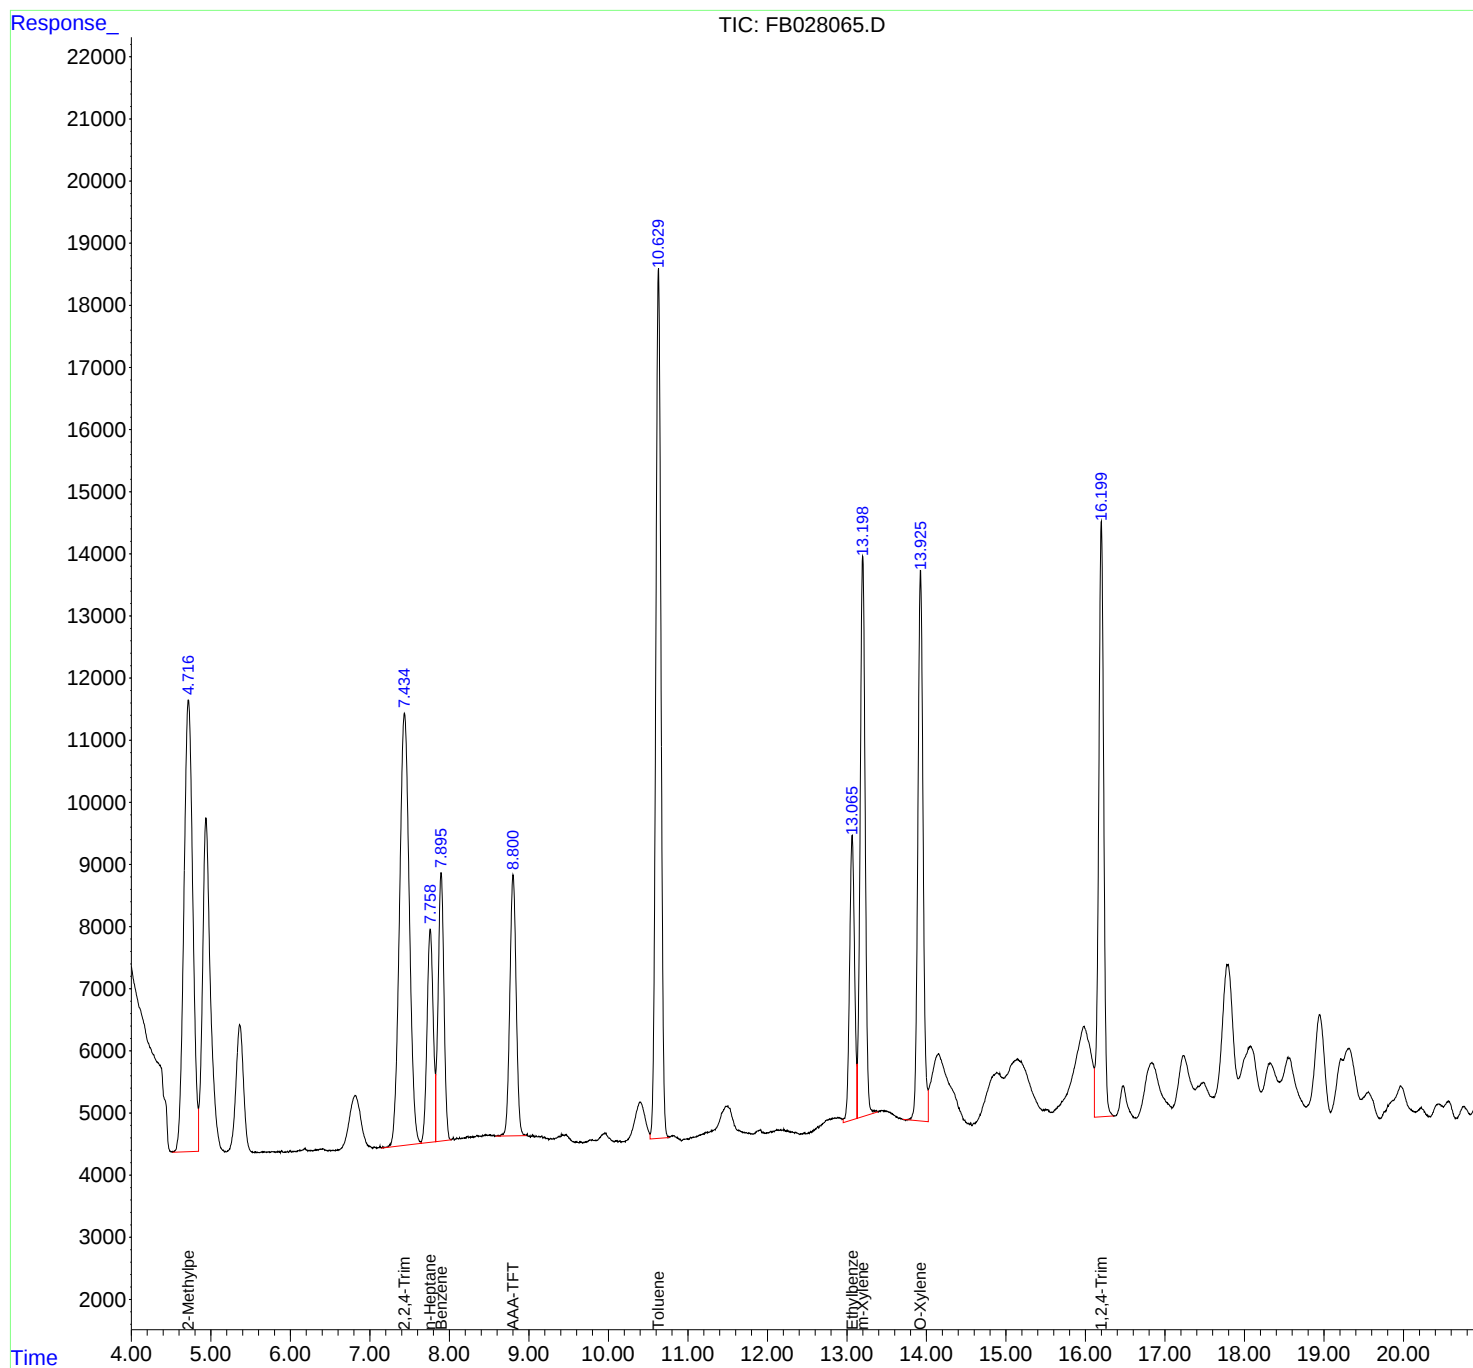


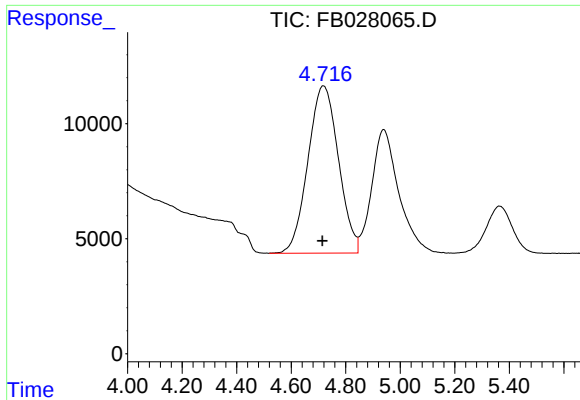

#1 2-Methylpentane


R.T.: 4.718 min
Delta R.T.: 0.003 min
Response: 564907
Conc: 31.23 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0830S2

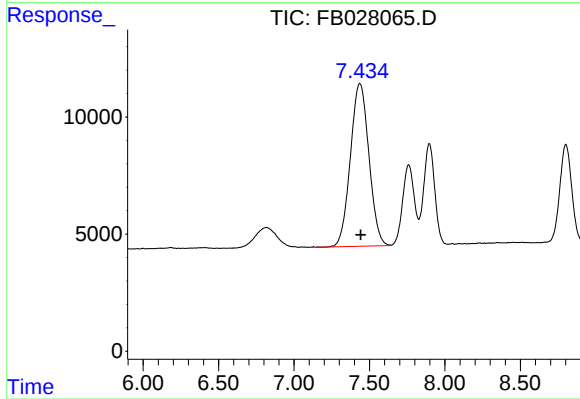


#2 2,2,4-Trimethylpentane

R.T.: 7.436 min
Delta R.T.: -0.007 min
Response: 594168
Conc: 30.30 ng/ml

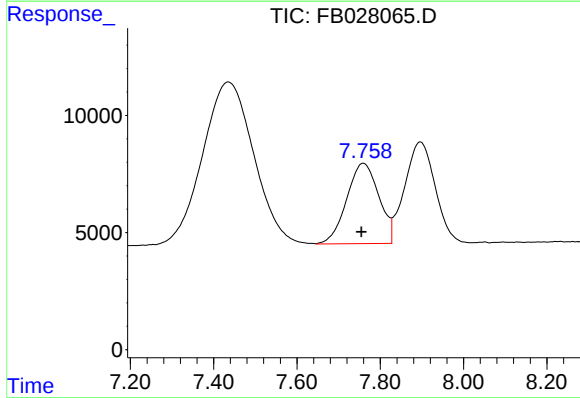


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.004 min
Response: 184176
Conc: 9.56 ng/ml

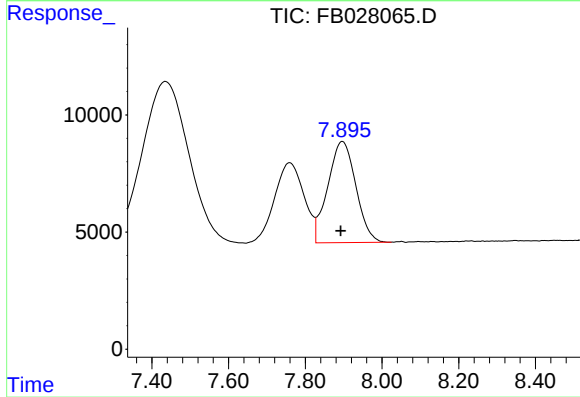

#4 Benzene


R.T.: 7.897 min
Delta R.T.: 0.005 min
Response: 219584
Conc: 9.44 ng/ml

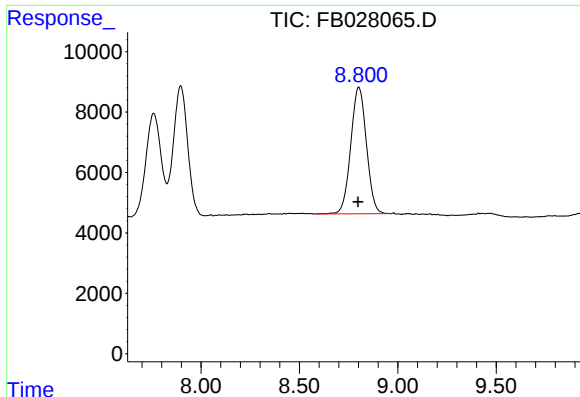

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.004 min
Response: 231938
Conc: 20.01 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0830S2

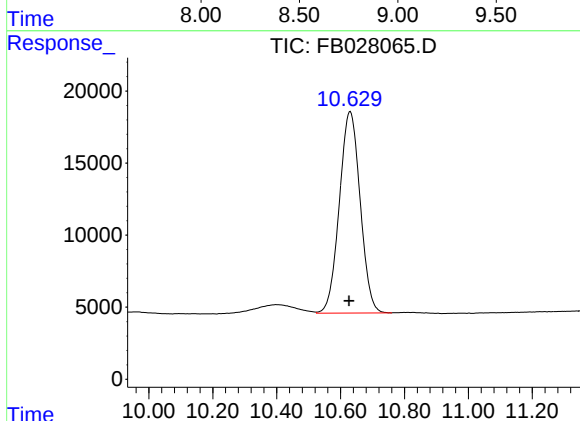


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.003 min
Response: 632793
Conc: 28.86 ng/ml

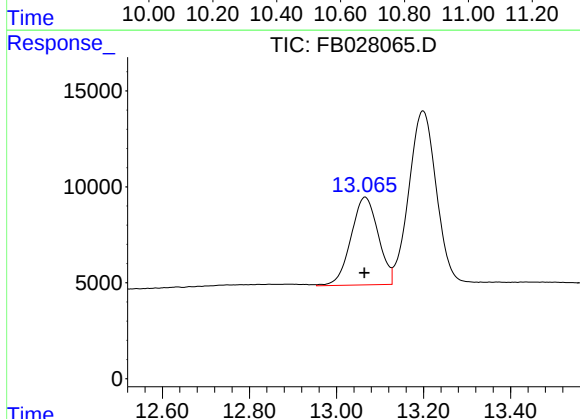


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: 0.002 min
Response: 198924
Conc: 9.65 ng/ml

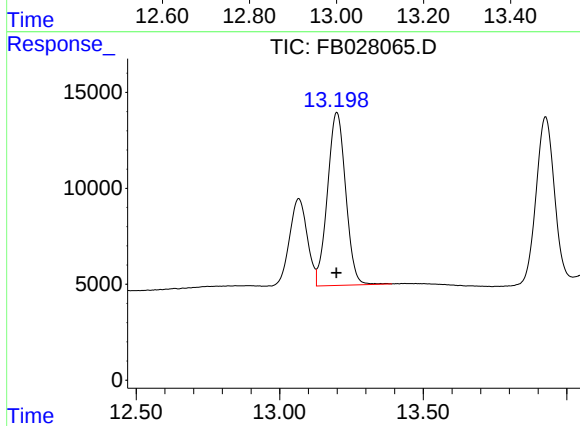

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: 0.002 min
Response: 395425
Conc: 19.32 ng/ml

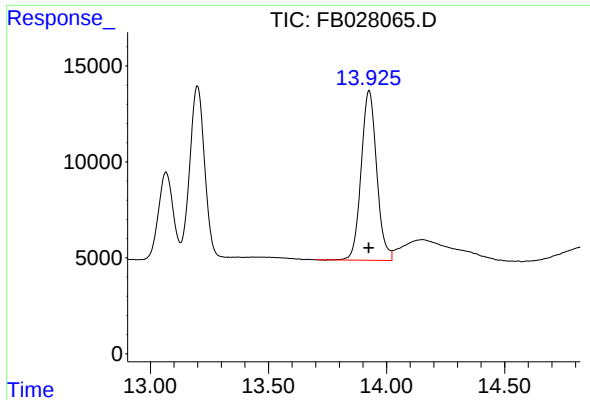

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.002 min
Response: 404491
Conc: 20.42 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0830S2

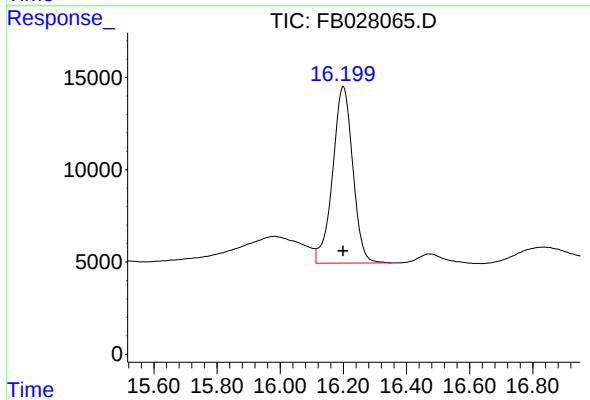

#10 1,2,4-Trimethylbenzene

R.T.: 16.200 min
Delta R.T.: 0.000 min
Response: 423885
Conc: 21.74 ng/ml