

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083023\
 Data File : FB030301.D
 Signal(s) : FID2B.CH
 Acq On : 30 Aug 2023 11:22
 Operator : YP/AJ
 Sample : BSF0830S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0830S1

Integration File: Calibration.e
 Quant Time: Aug 31 00:42:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082223.M
 Quant Title :
 QLast Update : Tue Aug 22 18:06:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	297639	25.009 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	625895	34.414 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	669037	33.908 ng/ml
3) t n-Heptane	7.753	236224	11.081 ng/ml
4) t Benzene	7.889	284722	11.462 ng/ml
6) t Toluene	10.622	803589	33.511 ng/ml
7) t Ethylbenzene	13.058	242039	10.797 ng/ml
8) t m-Xylene	13.191	480927	21.570 ng/ml
9) t O-Xylene	13.918	467118	21.901 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	423213	19.972 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083023\
Data File : FB030301.D
Signal(s) : FID2B.CH
Acq On : 30 Aug 2023 11:22
Operator : YP/AJ
Sample : BSF0830S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0830S1

Integration File: Calibration.e
Quant Time: Aug 31 00:42:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082223.M
Quant Title :
QLast Update : Tue Aug 22 18:06:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

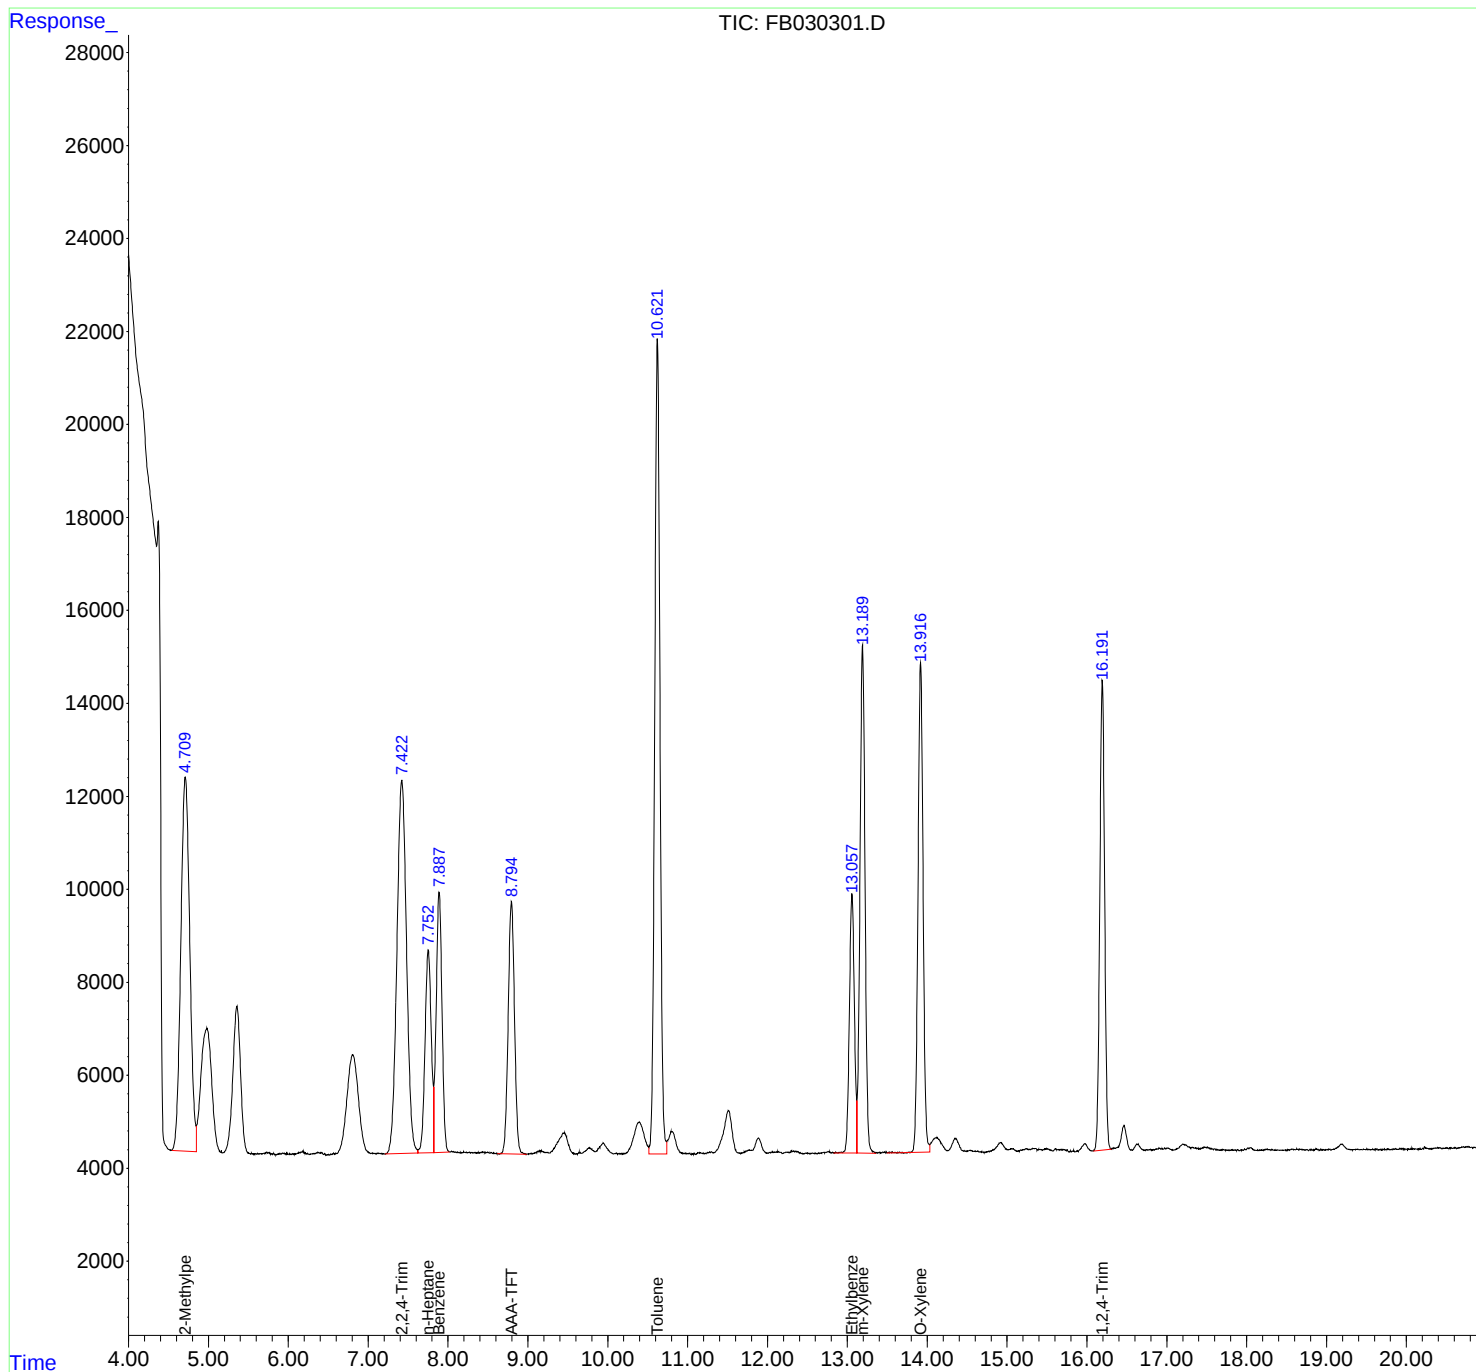


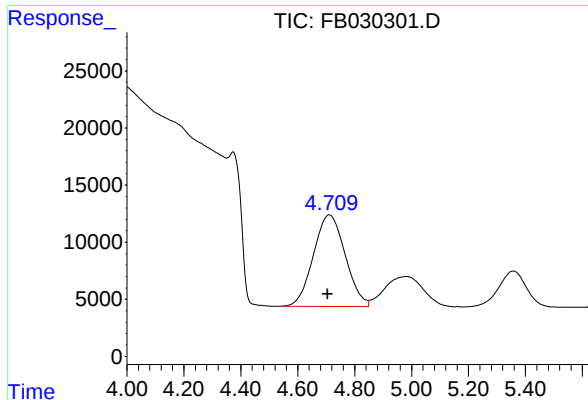

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.005 min
Response: 625895
Conc: 34.41 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0830S1

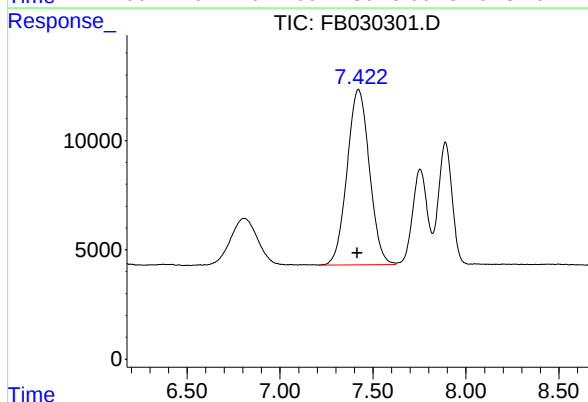


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: 0.007 min
Response: 669037
Conc: 33.91 ng/ml

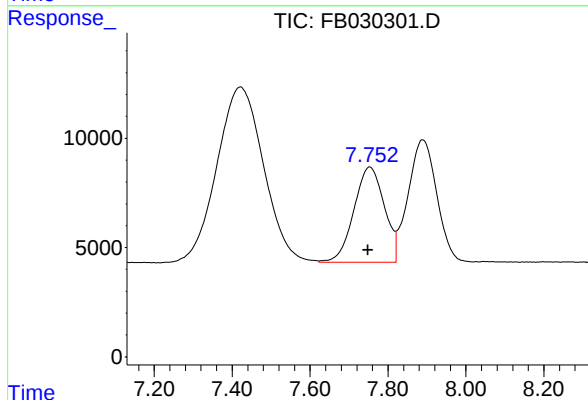


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.005 min
Response: 236224
Conc: 11.08 ng/ml

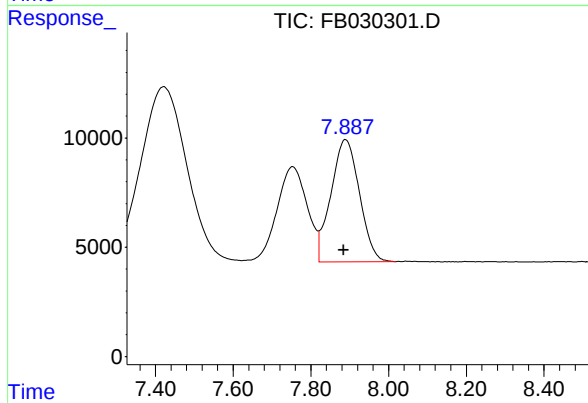

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.005 min
Response: 284722
Conc: 11.46 ng/ml

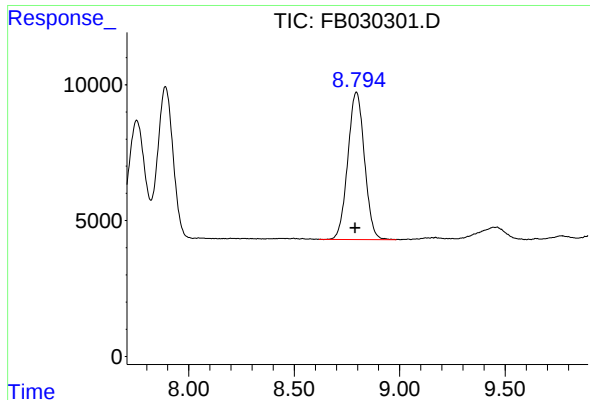

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.006 min
Response: 297639
Conc: 25.01 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0830S1

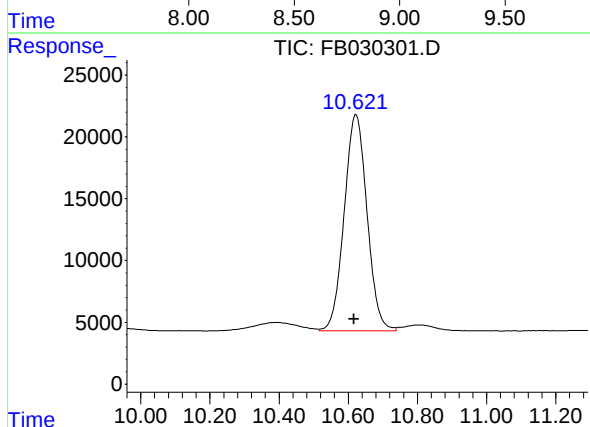


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.006 min
Response: 803589
Conc: 33.51 ng/ml

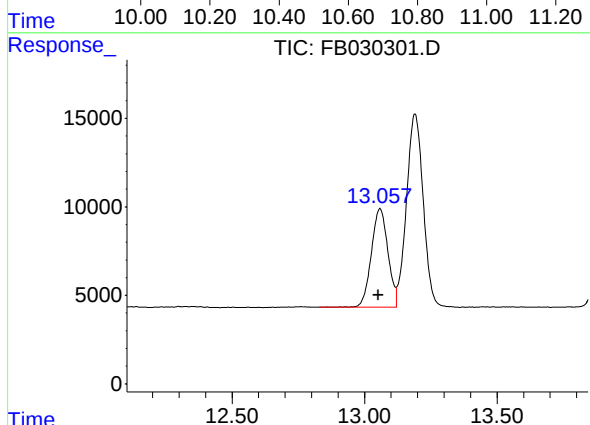


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.007 min
Response: 242039
Conc: 10.80 ng/ml

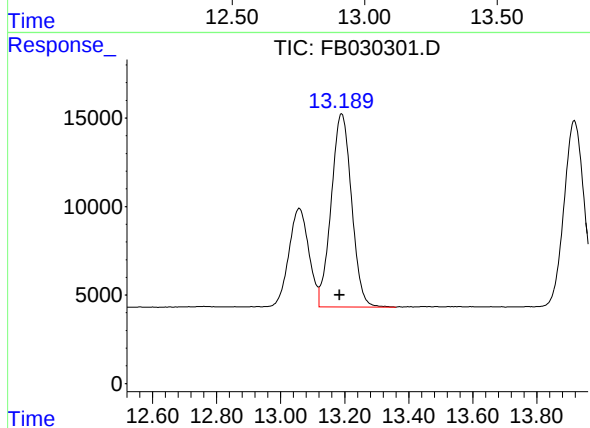

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.006 min
Response: 480927
Conc: 21.57 ng/ml

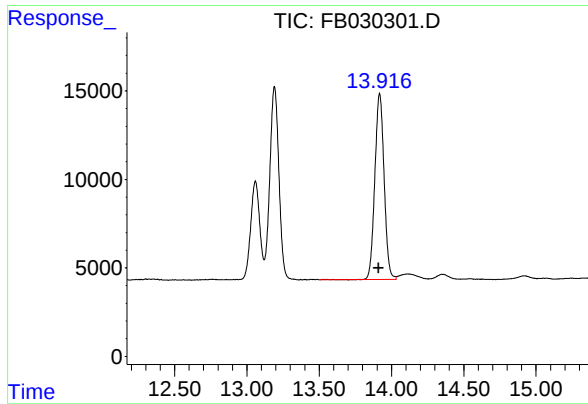

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.007 min
Response: 467118
Conc: 21.90 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0830S1

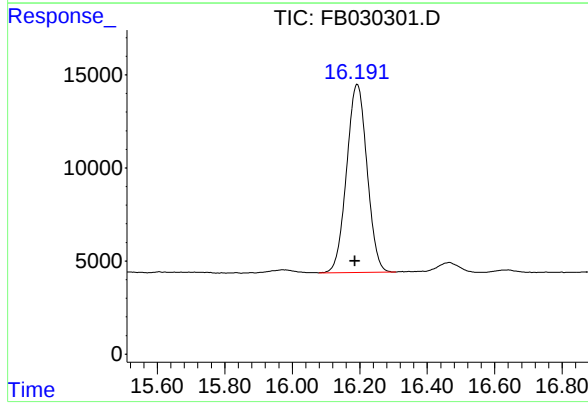

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.007 min
Response: 423213
Conc: 19.97 ng/ml