

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083023\
 Data File : FB030310.D
 Signal(s) : FID2B.CH
 Acq On : 30 Aug 2023 17:20
 Operator : YP/AJ
 Sample : BSF0830S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0830S3

Integration File: Calibration.e
 Quant Time: Aug 31 00:42:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082223.M
 Quant Title :
 QLast Update : Tue Aug 22 18:06:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	261051	21.934 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	626135	34.427 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	663997	33.653 ng/ml
3) t n-Heptane	7.757	237271	11.130 ng/ml
4) t Benzene	7.893	282757	11.383 ng/ml
6) t Toluene	10.626	835390	34.837 ng/ml
7) t Ethylbenzene	13.063	254752	11.364 ng/ml
8) t m-Xylene	13.195	504638	22.634 ng/ml
9) t O-Xylene	13.922	483605	22.674 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	438451	20.691 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083023\
Data File : FB030310.D
Signal(s) : FID2B.CH
Acq On : 30 Aug 2023 17:20
Operator : YP/AJ
Sample : BSF0830S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0830S3

Integration File: Calibration.e
Quant Time: Aug 31 00:42:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082223.M
Quant Title :
QLast Update : Tue Aug 22 18:06:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

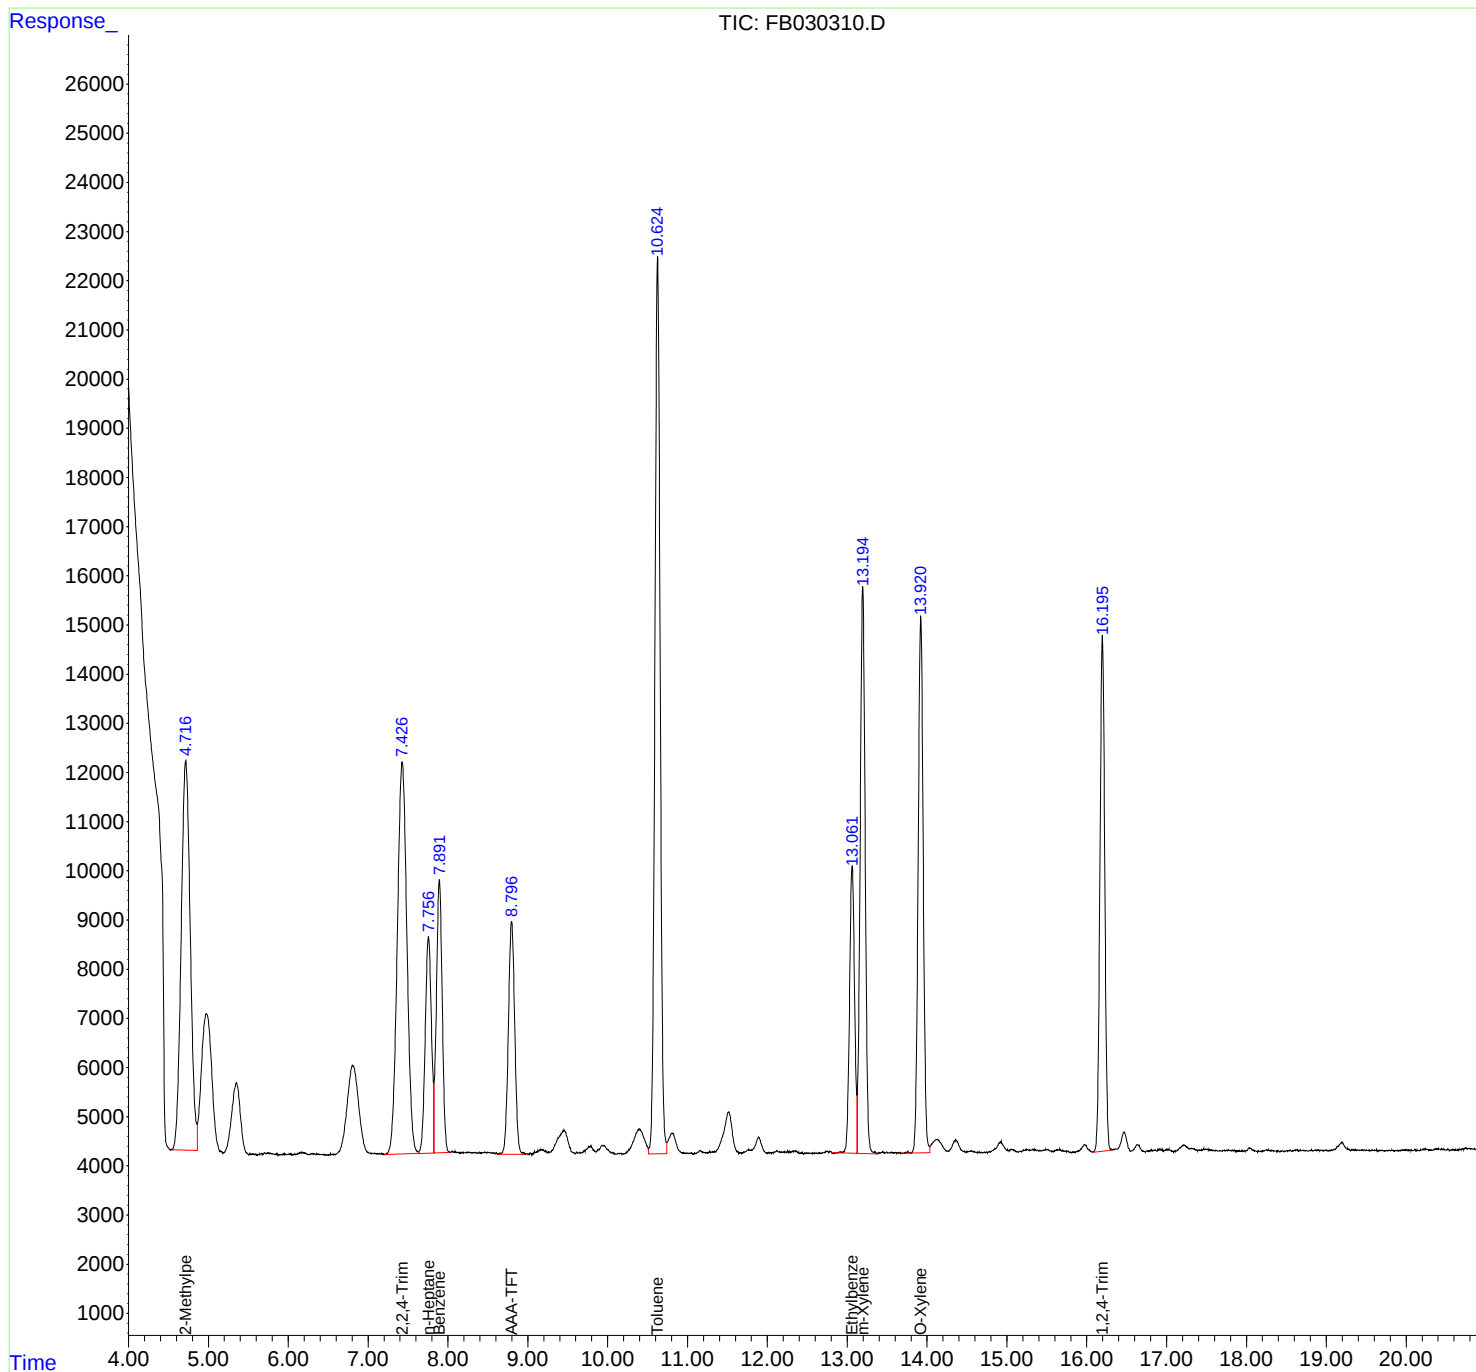


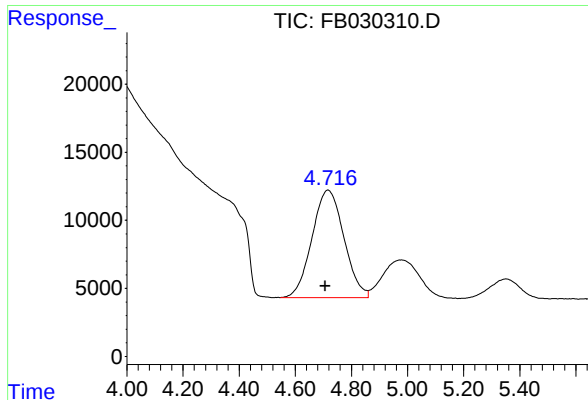

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: 0.011 min
Response: 626135
Conc: 34.43 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0830S3

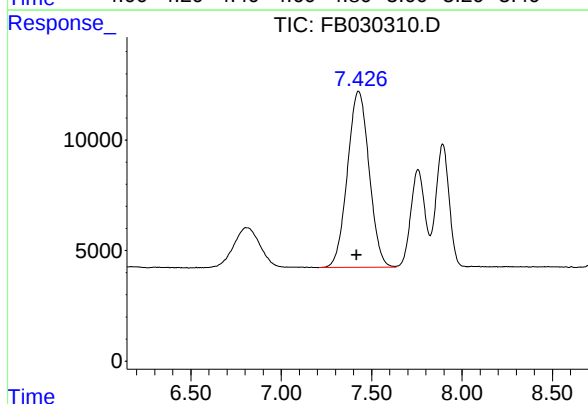


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.011 min
Response: 663997
Conc: 33.65 ng/ml

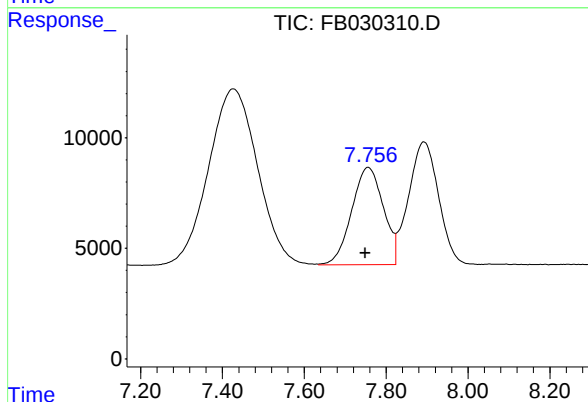


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.008 min
Response: 237271
Conc: 11.13 ng/ml

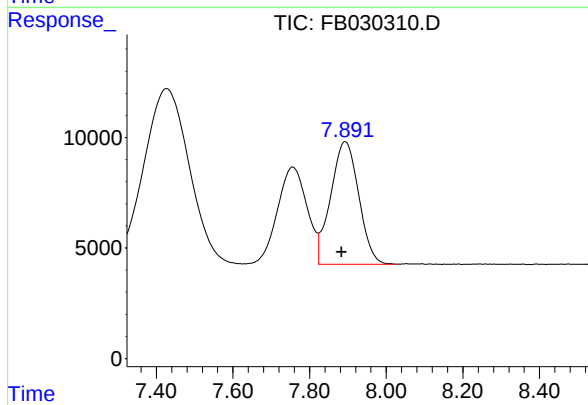

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.008 min
Response: 282757
Conc: 11.38 ng/ml

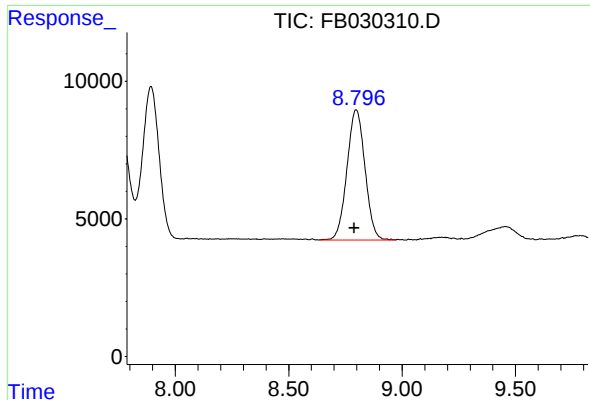

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.009 min
Response: 261051
Conc: 21.93 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0830S3

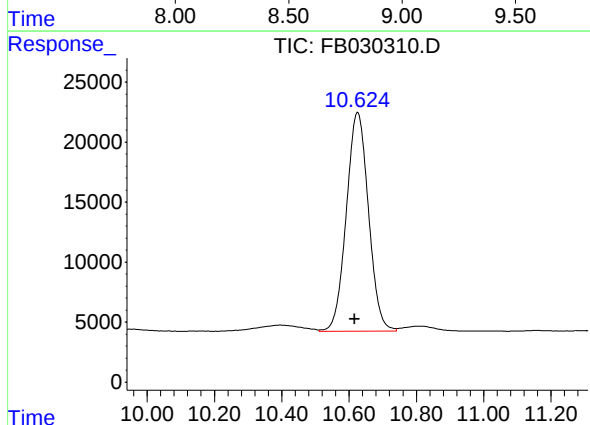


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.010 min
Response: 835390
Conc: 34.84 ng/ml

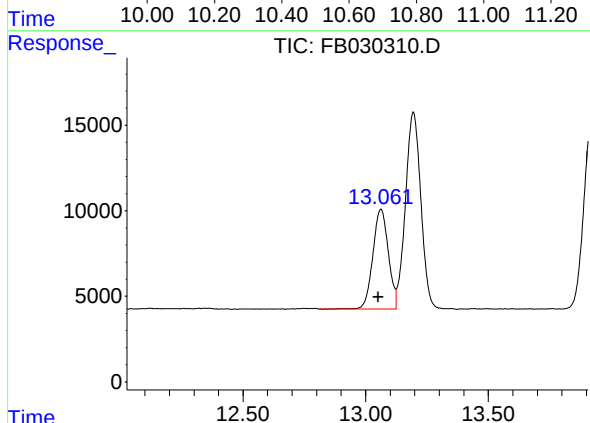


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.011 min
Response: 254752
Conc: 11.36 ng/ml

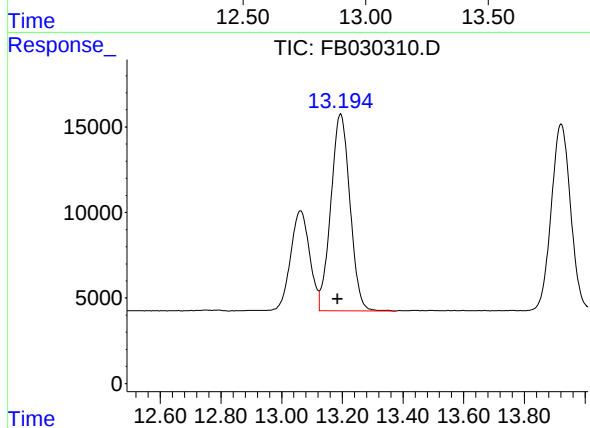

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: 0.010 min
Response: 504638
Conc: 22.63 ng/ml

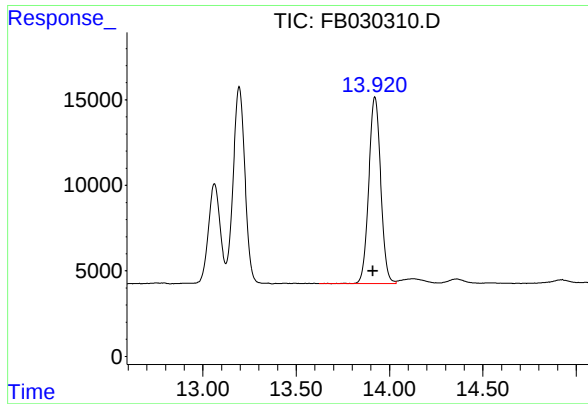

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.011 min
Response: 483605
Conc: 22.67 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0830S3

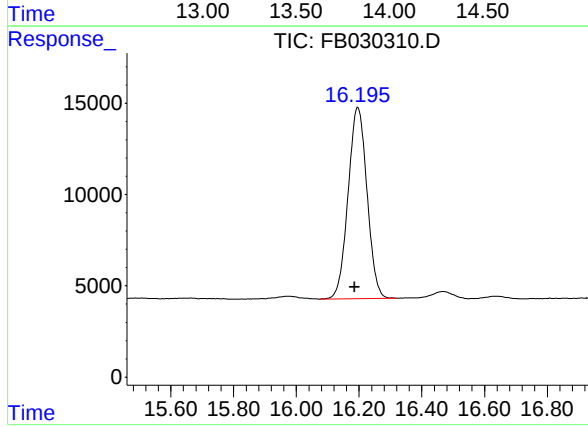

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.010 min
Response: 438451
Conc: 20.69 ng/ml