

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083118\
 Data File : FB017594.D
 Signal(s) : FID2B.CH
 Acq On : 31 Aug 2018 7:52
 Operator : MJ/SJ
 Sample : 20 PPB GRO STD
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 31 08:18:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
 Quant Title :
 QLast Update : Mon Aug 20 13:42:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.106	177262	21.500 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.957	393546	28.086 ng/ml
2) t 2,2,4-Trimethylpentane	7.722	413559	29.347 ng/ml
3) t n-Heptane	8.061	131509	9.542 ng/ml
4) t Benzene	8.200	179676	10.191 ng/ml
6) t Toluene	10.955	433841	30.157 ng/ml
7) t Ethylbenzene	13.404	148964	10.101 ng/ml
8) t m-Xylene	13.537	315564	20.300 ng/ml
9) t O-Xylene	14.269	363862	22.166 ng/ml
10) t 1,2,4-Trimethylbenzene	16.551	398096	20.440 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083118\
Data File : FB017594.D
Signal(s) : FID2B.CH
Acq On : 31 Aug 2018 7:52
Operator : MJ/SJ
Sample : 20 PPB GRO STD
Misc : 5.00g/5.00mL DI Water
ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 31 08:18:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

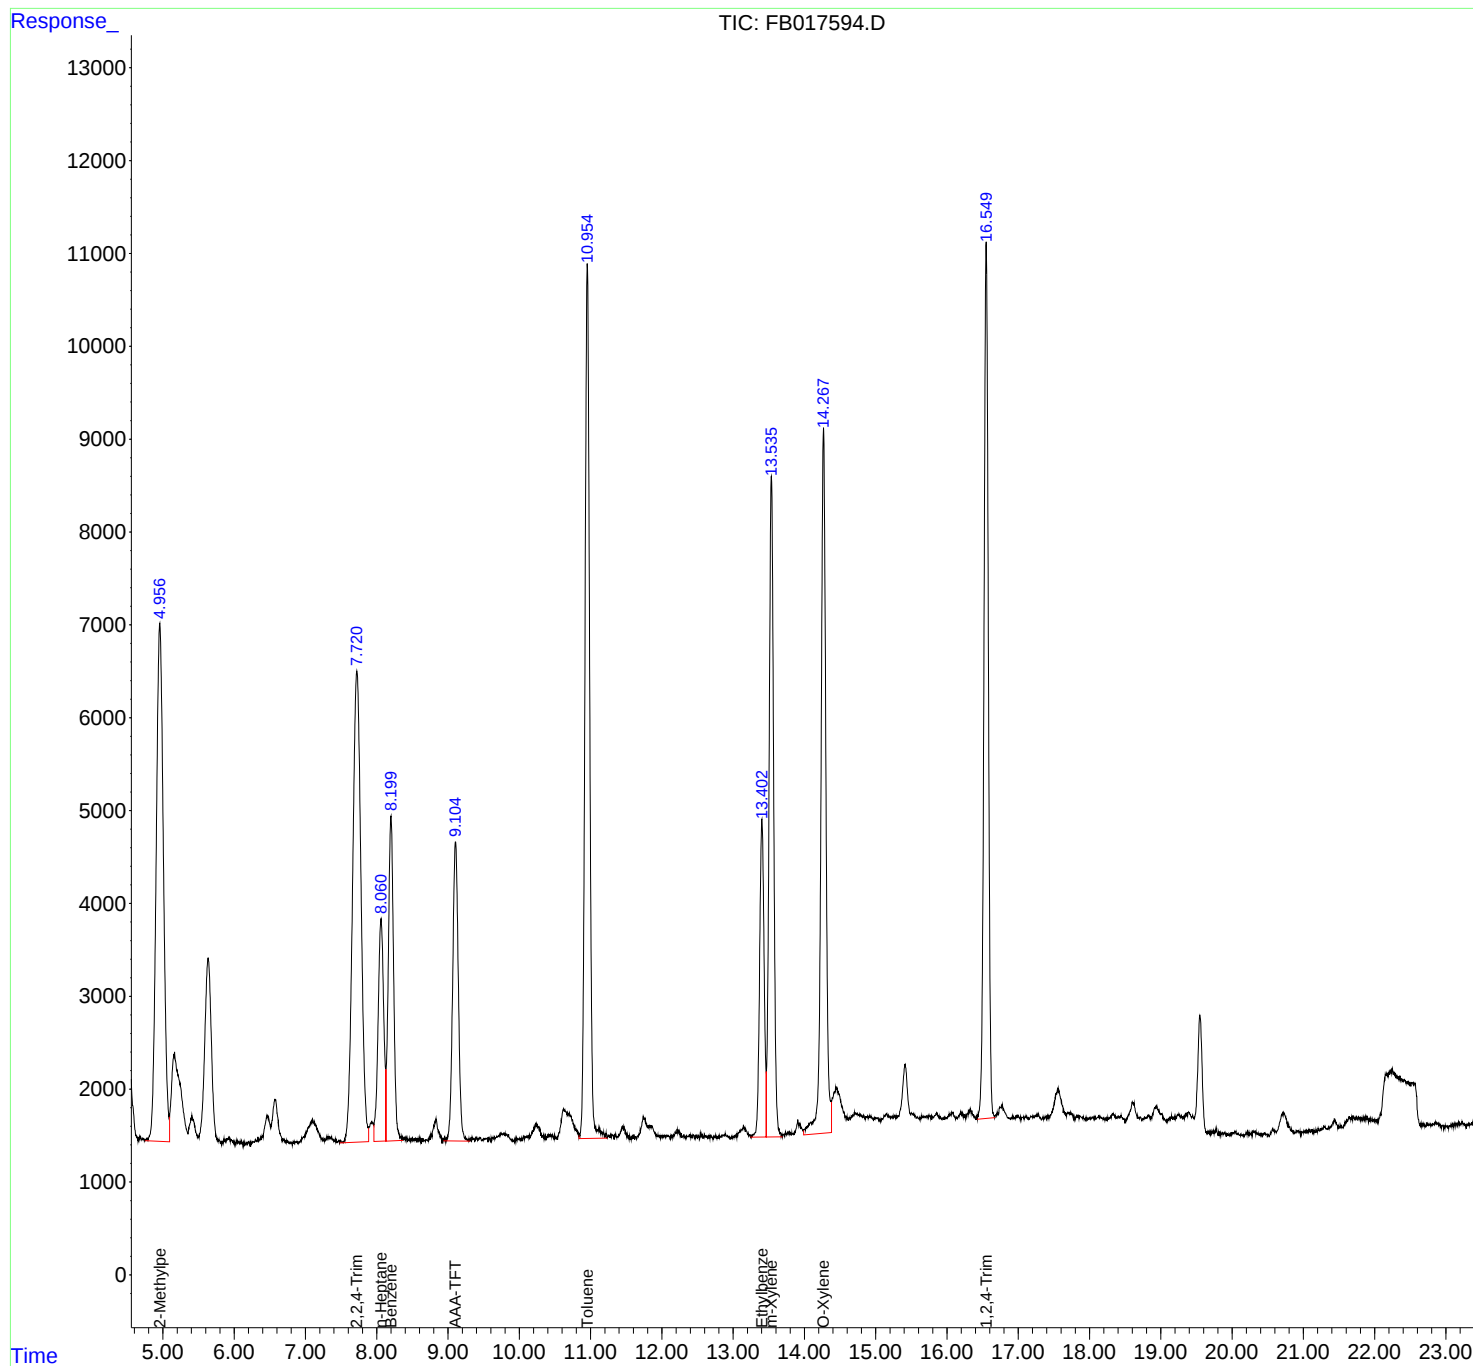

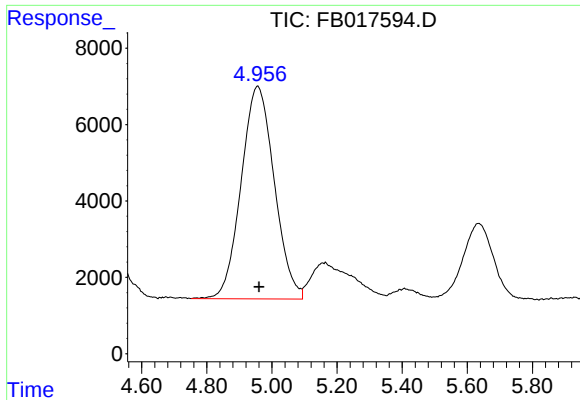


#1 2-Methylpentane

R.T.: 4.957 min
Delta R.T.: -0.004 min
Response: 393546
Conc: 28.09 ng/ml

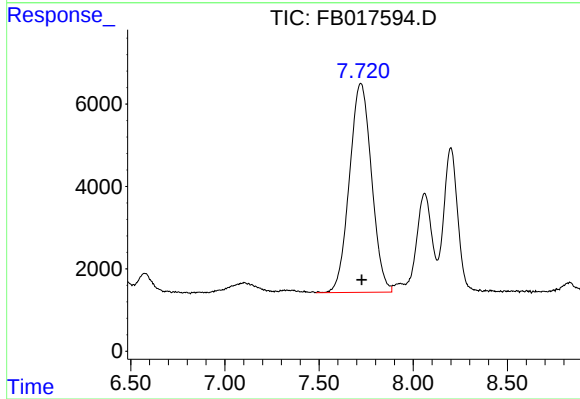


#2 2,2,4-Trimethylpentane

R.T.: 7.722 min
Delta R.T.: -0.005 min
Response: 413559
Conc: 29.35 ng/ml

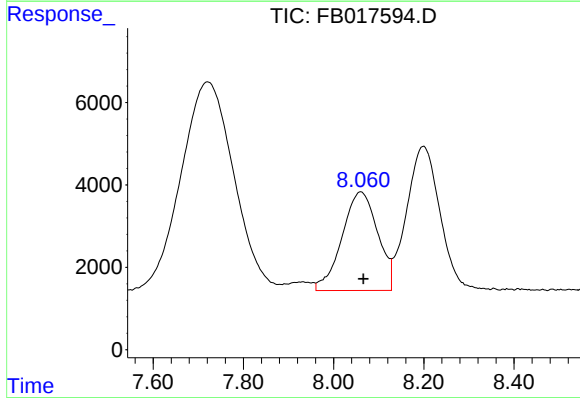


#3 n-Heptane

R.T.: 8.061 min
Delta R.T.: -0.005 min
Response: 131509
Conc: 9.54 ng/ml

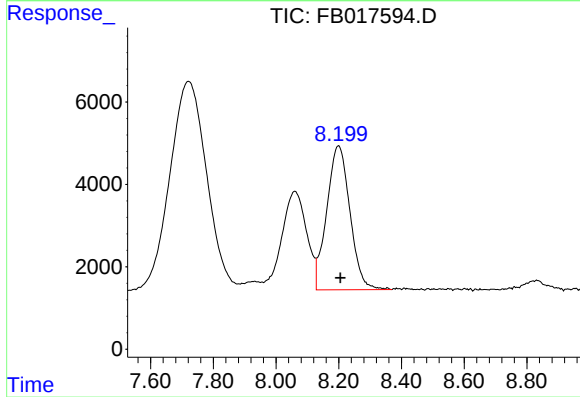


#4 Benzene

R.T.: 8.200 min
Delta R.T.: -0.006 min
Response: 179676
Conc: 10.19 ng/ml

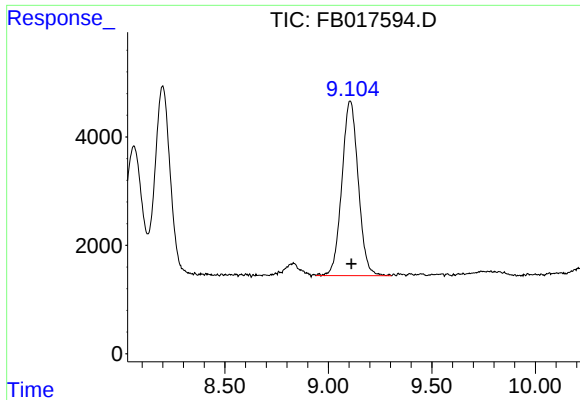


#5 AAA-TFT

R.T.: 9.106 min
Delta R.T.: -0.005 min
Response: 177262
Conc: 21.50 ng/ml

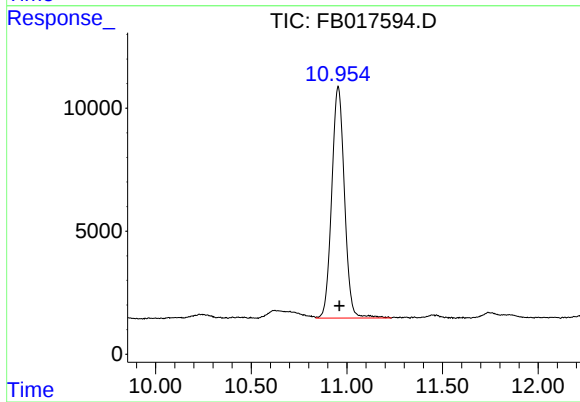


#6 Toluene

R.T.: 10.955 min
Delta R.T.: -0.006 min
Response: 433841
Conc: 30.16 ng/ml

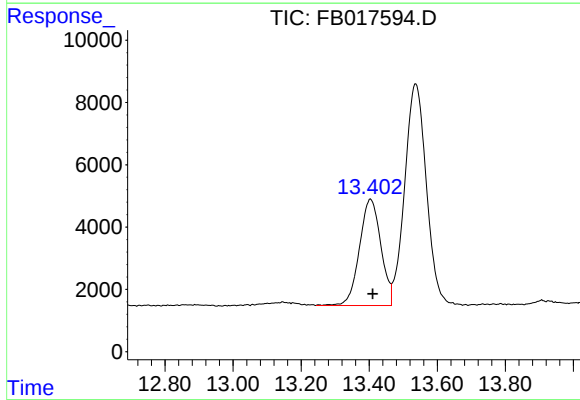


#7 Ethylbenzene

R.T.: 13.404 min
Delta R.T.: -0.006 min
Response: 148964
Conc: 10.10 ng/ml

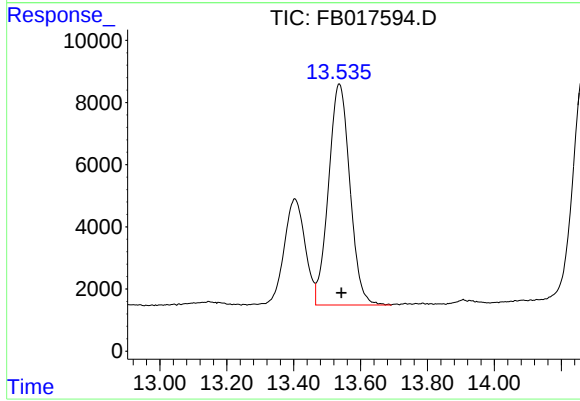


#8 m-Xylene

R.T.: 13.537 min
Delta R.T.: -0.006 min
Response: 315564
Conc: 20.30 ng/ml

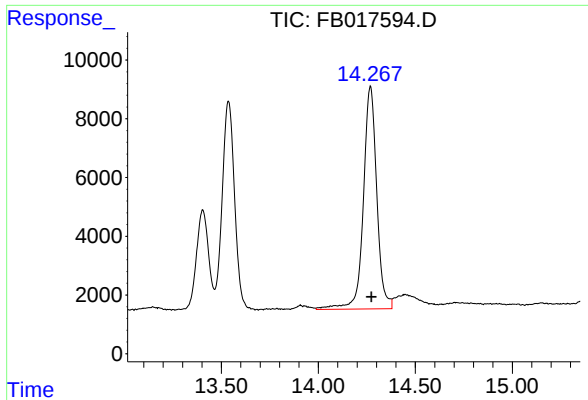

#9 O-Xylene

R.T.: 14.269 min
Delta R.T.: -0.005 min
Response: 363862
Conc: 22.17 ng/ml

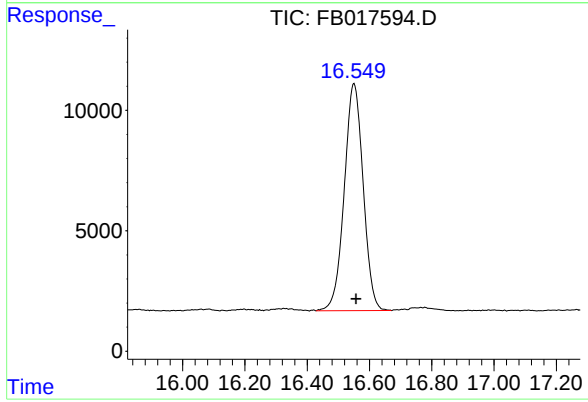

#10 1,2,4-Trimethylbenzene

R.T.: 16.551 min
Delta R.T.: -0.007 min
Response: 398096
Conc: 20.44 ng/ml