

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083118\
 Data File : FB017596.D
 Signal(s) : FID2B.CH
 Acq On : 31 Aug 2018 9:05
 Operator : MJ/SJ
 Sample : BSF0831S1
 Misc : 5.04g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 31 09:26:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
 Quant Title :
 QLast Update : Mon Aug 20 13:42:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.109	160132	19.422 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.960	377144	26.915 ng/ml
2) t 2,2,4-Trimethylpentane	7.725	390404	27.704 ng/ml
3) t n-Heptane	8.067	115761	8.400 ng/ml
4) t Benzene	8.204	166260	9.430 ng/ml
6) t Toluene	10.958	422643	29.379 ng/ml
7) t Ethylbenzene	13.408	143403	9.724 ng/ml
8) t m-Xylene	13.540	304587	19.594 ng/ml
9) t O-Xylene	14.272	324279	19.754 ng/ml
10) t 1,2,4-Trimethylbenzene	16.554	382783	19.654 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB083118\
Data File : FB017596.D
Signal(s) : FID2B.CH
Acq On : 31 Aug 2018 9:05
Operator : MJ/SJ
Sample : BSF0831S1
Misc : 5.04g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 31 09:26:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

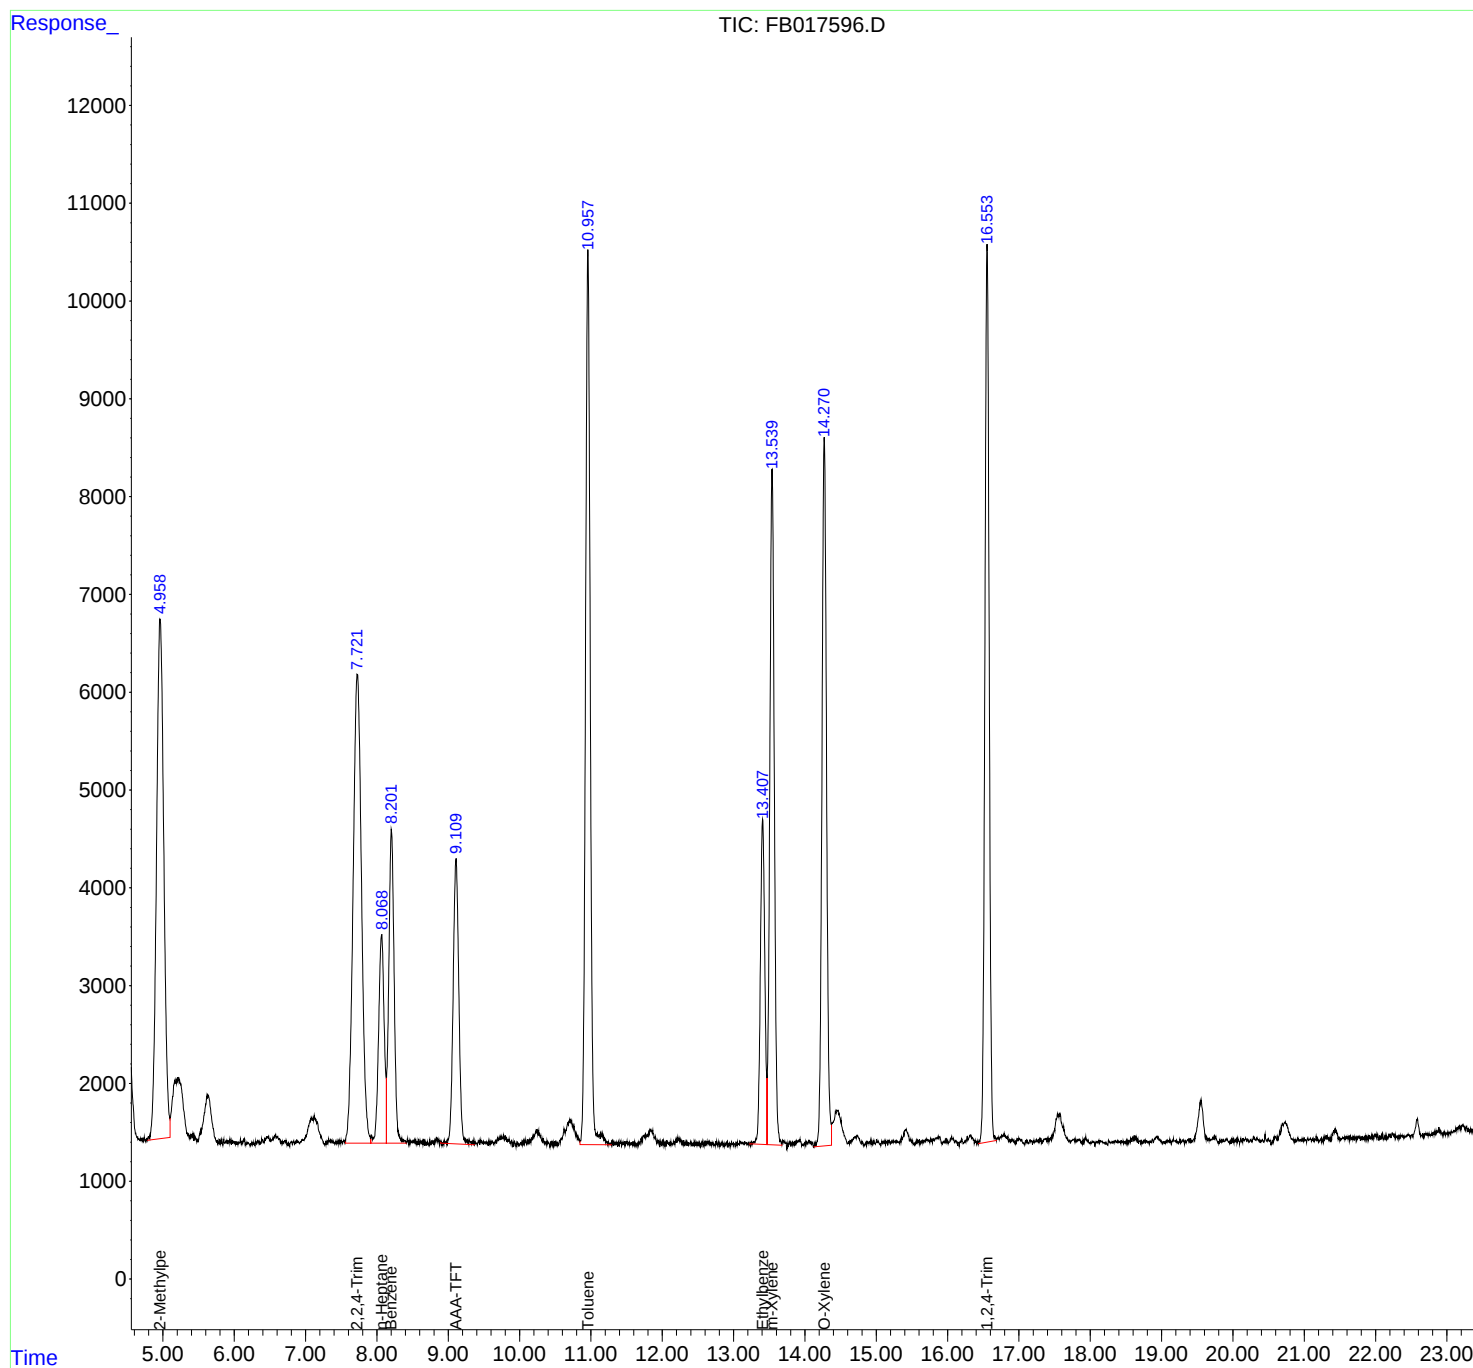

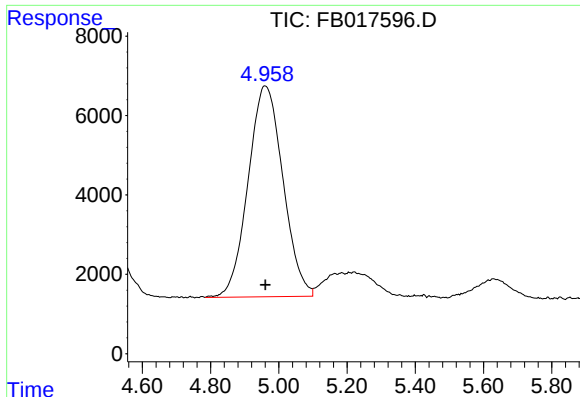


#1 2-Methylpentane

R.T.: 4.960 min
Delta R.T.: 0.000 min
Response: 377144
Conc: 26.92 ng/ml

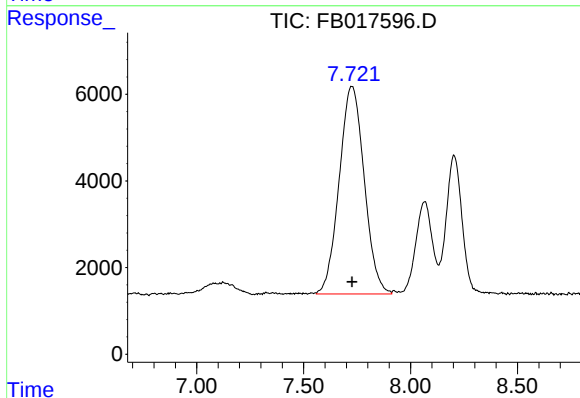


#2 2,2,4-Trimethylpentane

R.T.: 7.725 min
Delta R.T.: -0.002 min
Response: 390404
Conc: 27.70 ng/ml

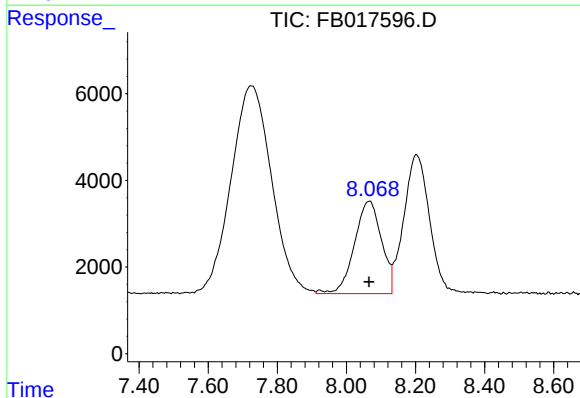


#3 n-Heptane

R.T.: 8.067 min
Delta R.T.: 0.000 min
Response: 115761
Conc: 8.40 ng/ml

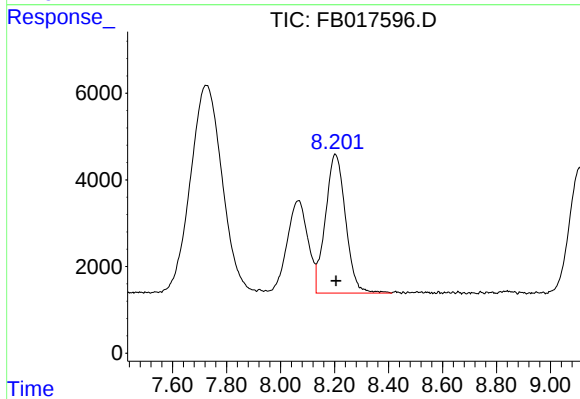


#4 Benzene

R.T.: 8.204 min
Delta R.T.: -0.002 min
Response: 166260
Conc: 9.43 ng/ml

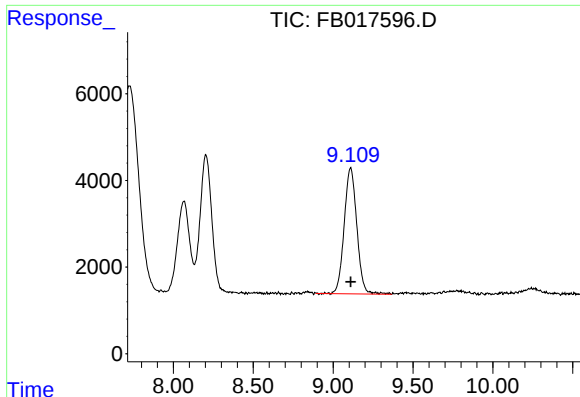


#5 AAA-TFT

R.T.: 9.109 min
Delta R.T.: -0.002 min
Response: 160132
Conc: 19.42 ng/ml

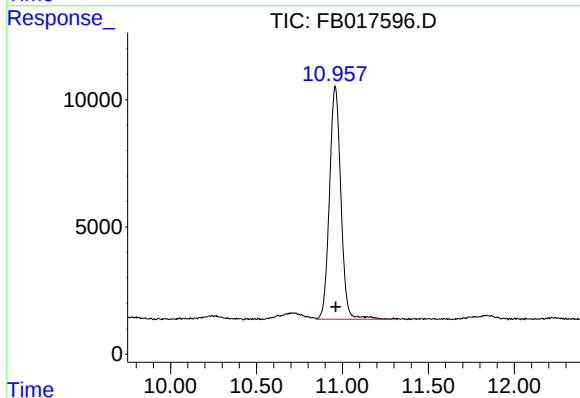


#6 Toluene

R.T.: 10.958 min
Delta R.T.: -0.002 min
Response: 422643
Conc: 29.38 ng/ml

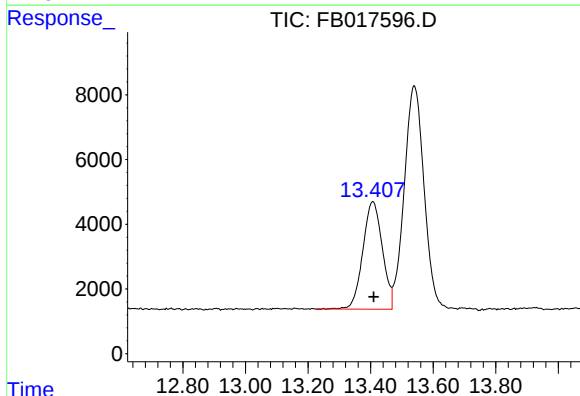


#7 Ethylbenzene

R.T.: 13.408 min
Delta R.T.: -0.003 min
Response: 143403
Conc: 9.72 ng/ml

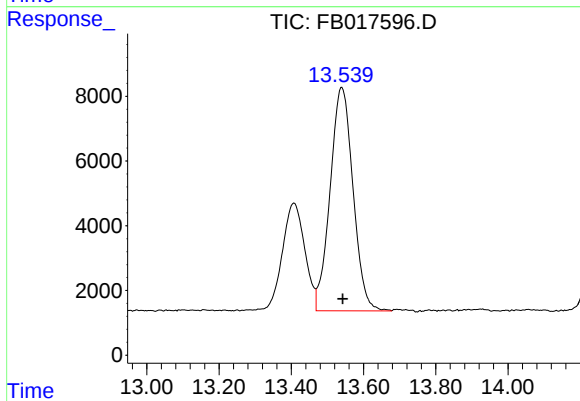


#8 m-Xylene

R.T.: 13.540 min
Delta R.T.: -0.002 min
Response: 304587
Conc: 19.59 ng/ml

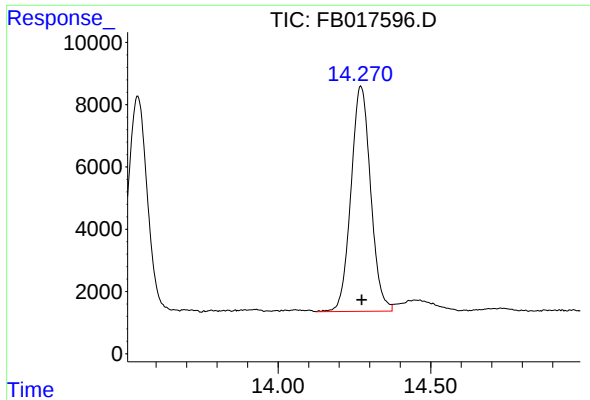

#9 O-Xylene

R.T.: 14.272 min
Delta R.T.: -0.002 min
Response: 324279
Conc: 19.75 ng/ml

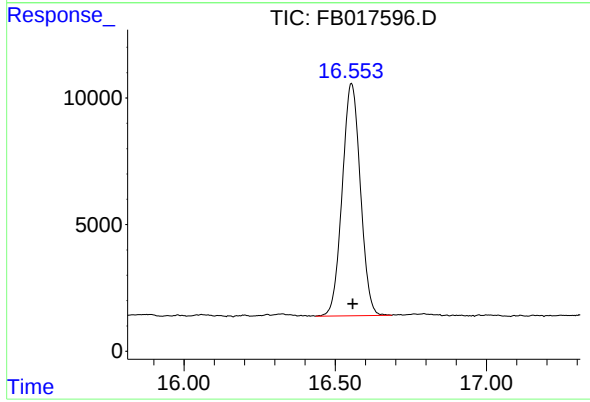

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: -0.003 min
Response: 382783
Conc: 19.65 ng/ml