

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090122\
 Data File : FB028067.D
 Signal(s) : FID2B.CH
 Acq On : 1 Sep 2022 9:08
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 02 03:22:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	277242	23.922 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	525492	29.047 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	562644	28.691 ng/ml
3) t n-Heptane	7.748	184960	9.601 ng/ml
4) t Benzene	7.886	221687	9.534 ng/ml
6) t Toluene	10.619	621457	28.341 ng/ml
7) t Ethylbenzene	13.056	200055	9.708 ng/ml
8) t m-Xylene	13.188	388664	18.994 ng/ml
9) t O-Xylene	13.915	380097	19.188 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	390251	20.012 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090122\
Data File : FB028067.D
Signal(s) : FID2B.CH
Acq On : 1 Sep 2022 9:08
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 02 03:22:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

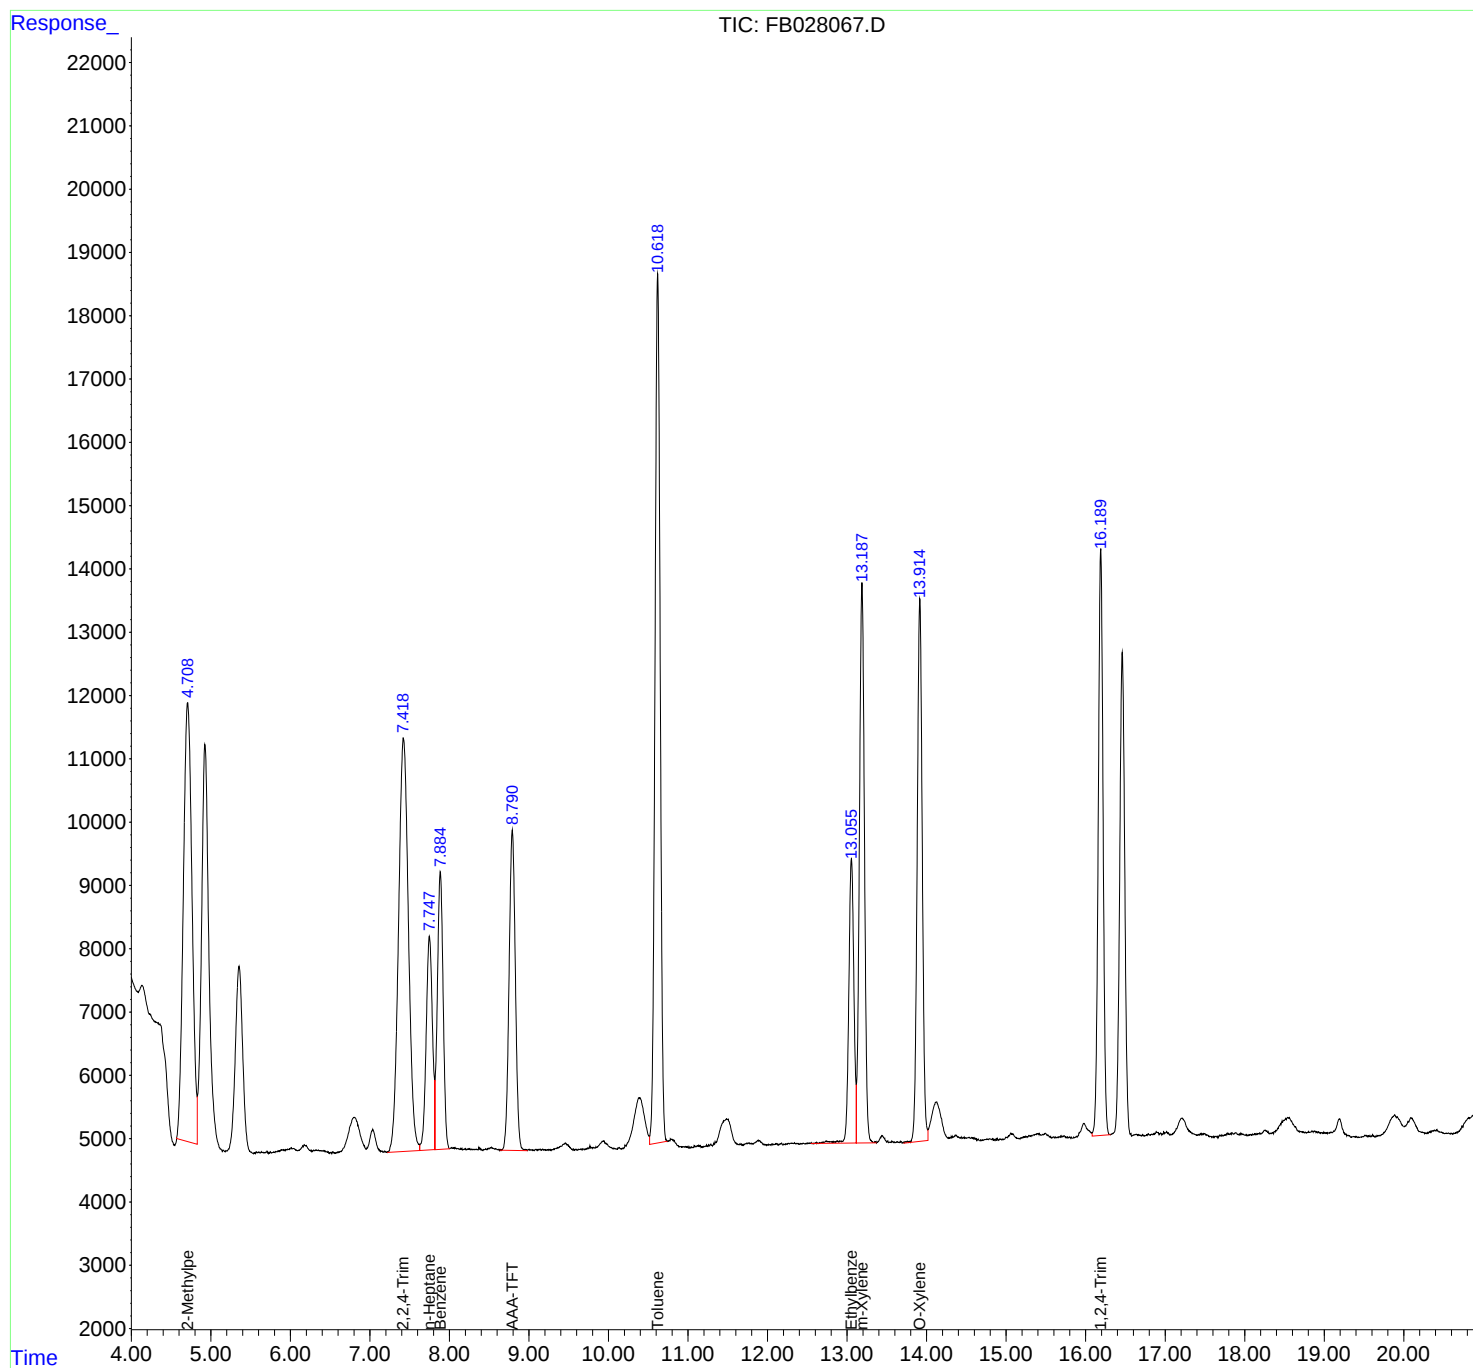


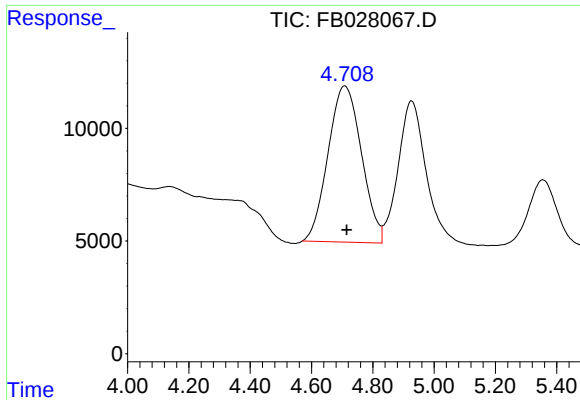

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: -0.006 min
Response: 525492
Conc: 29.05 ng/ml

Instrument :
FID_B
ClientSampleId :

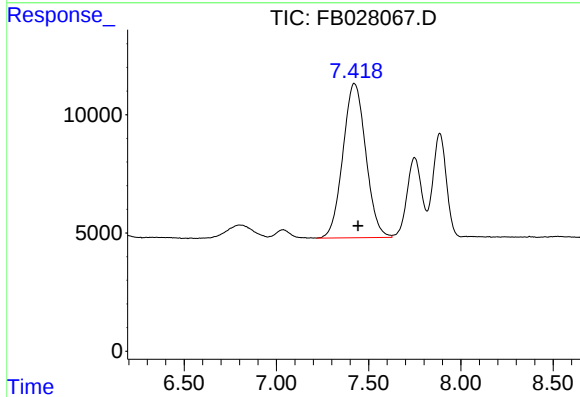


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: -0.022 min
Response: 562644
Conc: 28.69 ng/ml

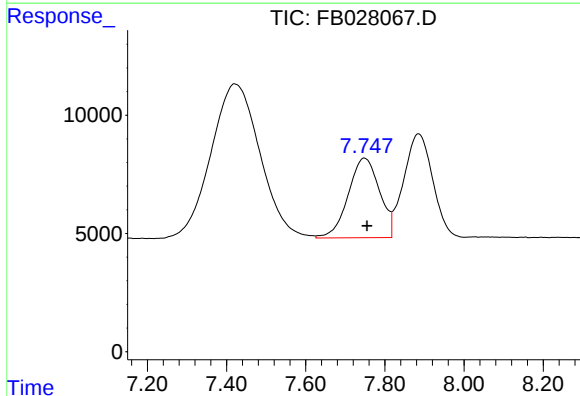


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.007 min
Response: 184960
Conc: 9.60 ng/ml

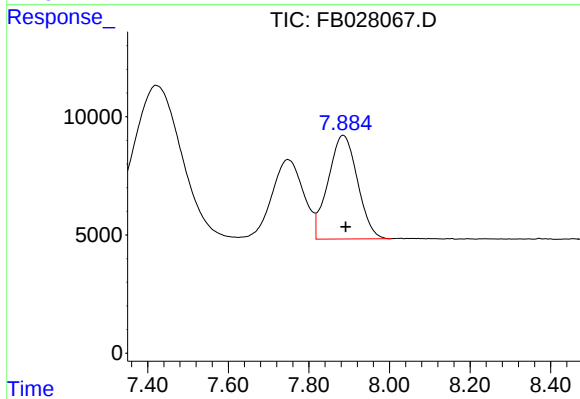

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.006 min
Response: 221687
Conc: 9.53 ng/ml

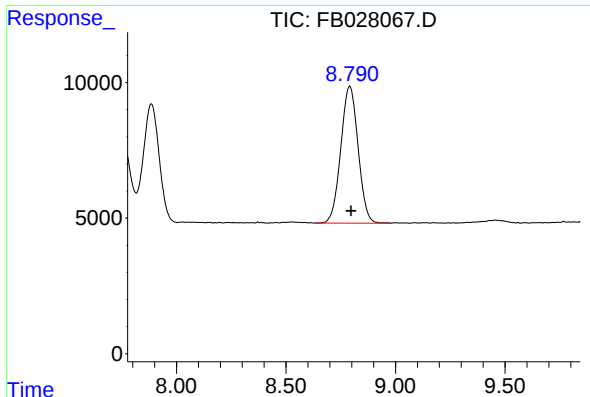

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.007 min
Response: 277242
Conc: 23.92 ng/ml

Instrument :
FID_B
ClientSampleId :

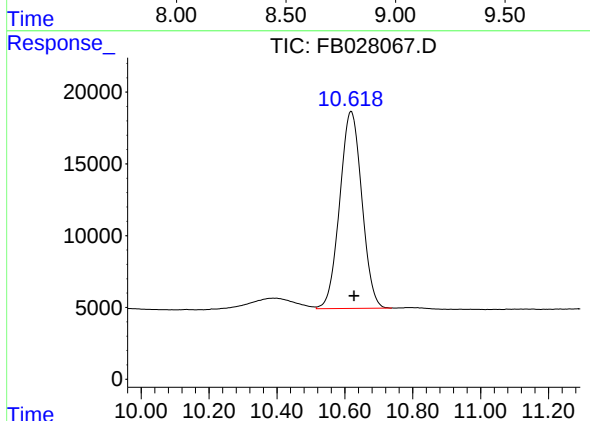


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.008 min
Response: 621457
Conc: 28.34 ng/ml

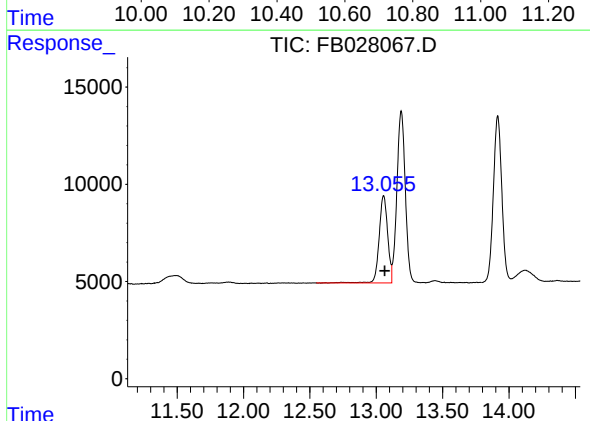


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.009 min
Response: 200055
Conc: 9.71 ng/ml

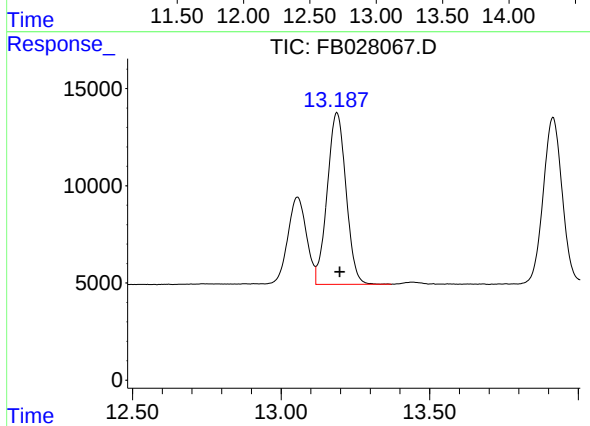

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.009 min
Response: 388664
Conc: 18.99 ng/ml

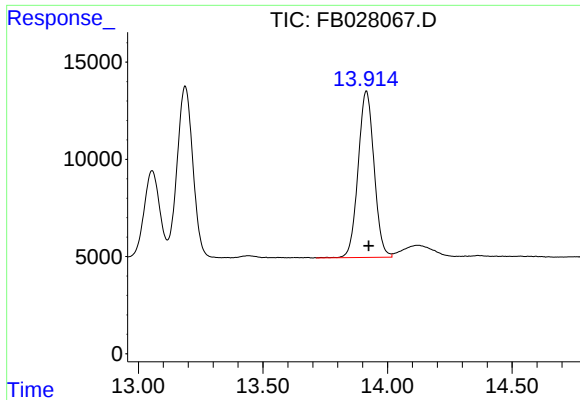

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.009 min
Response: 380097
Conc: 19.19 ng/ml

Instrument :
FID_B
ClientSampleId :

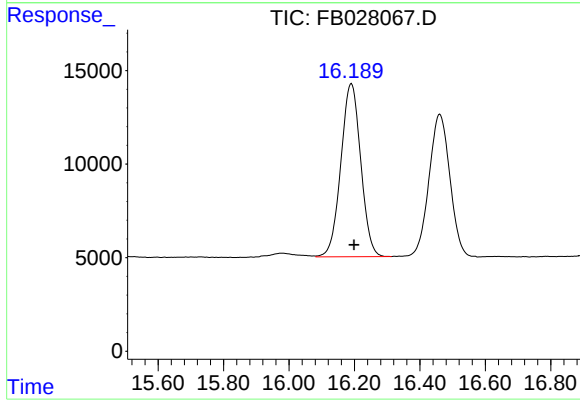

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.009 min
Response: 390251
Conc: 20.01 ng/ml