

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090122\
 Data File : FB028070.D
 Signal(s) : FID2B.CH
 Acq On : 1 Sep 2022 11:00
 Operator : AJ/MA
 Sample : BSF0901S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 02 03:22:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	218363	18.842 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	513357	28.377 ng/ml
2) t 2,2,4-Trimethylpentane	7.431	576251	29.385 ng/ml
3) t n-Heptane	7.754	175463	9.108 ng/ml
4) t Benzene	7.891	214679	9.233 ng/ml
6) t Toluene	10.624	621215	28.330 ng/ml
7) t Ethylbenzene	13.061	194413	9.434 ng/ml
8) t m-Xylene	13.193	384810	18.805 ng/ml
9) t O-Xylene	13.920	377144	19.039 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	382305	19.604 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090122\
Data File : FB028070.D
Signal(s) : FID2B.CH
Acq On : 1 Sep 2022 11:00
Operator : AJ/MA
Sample : BSF0901S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 02 03:22:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

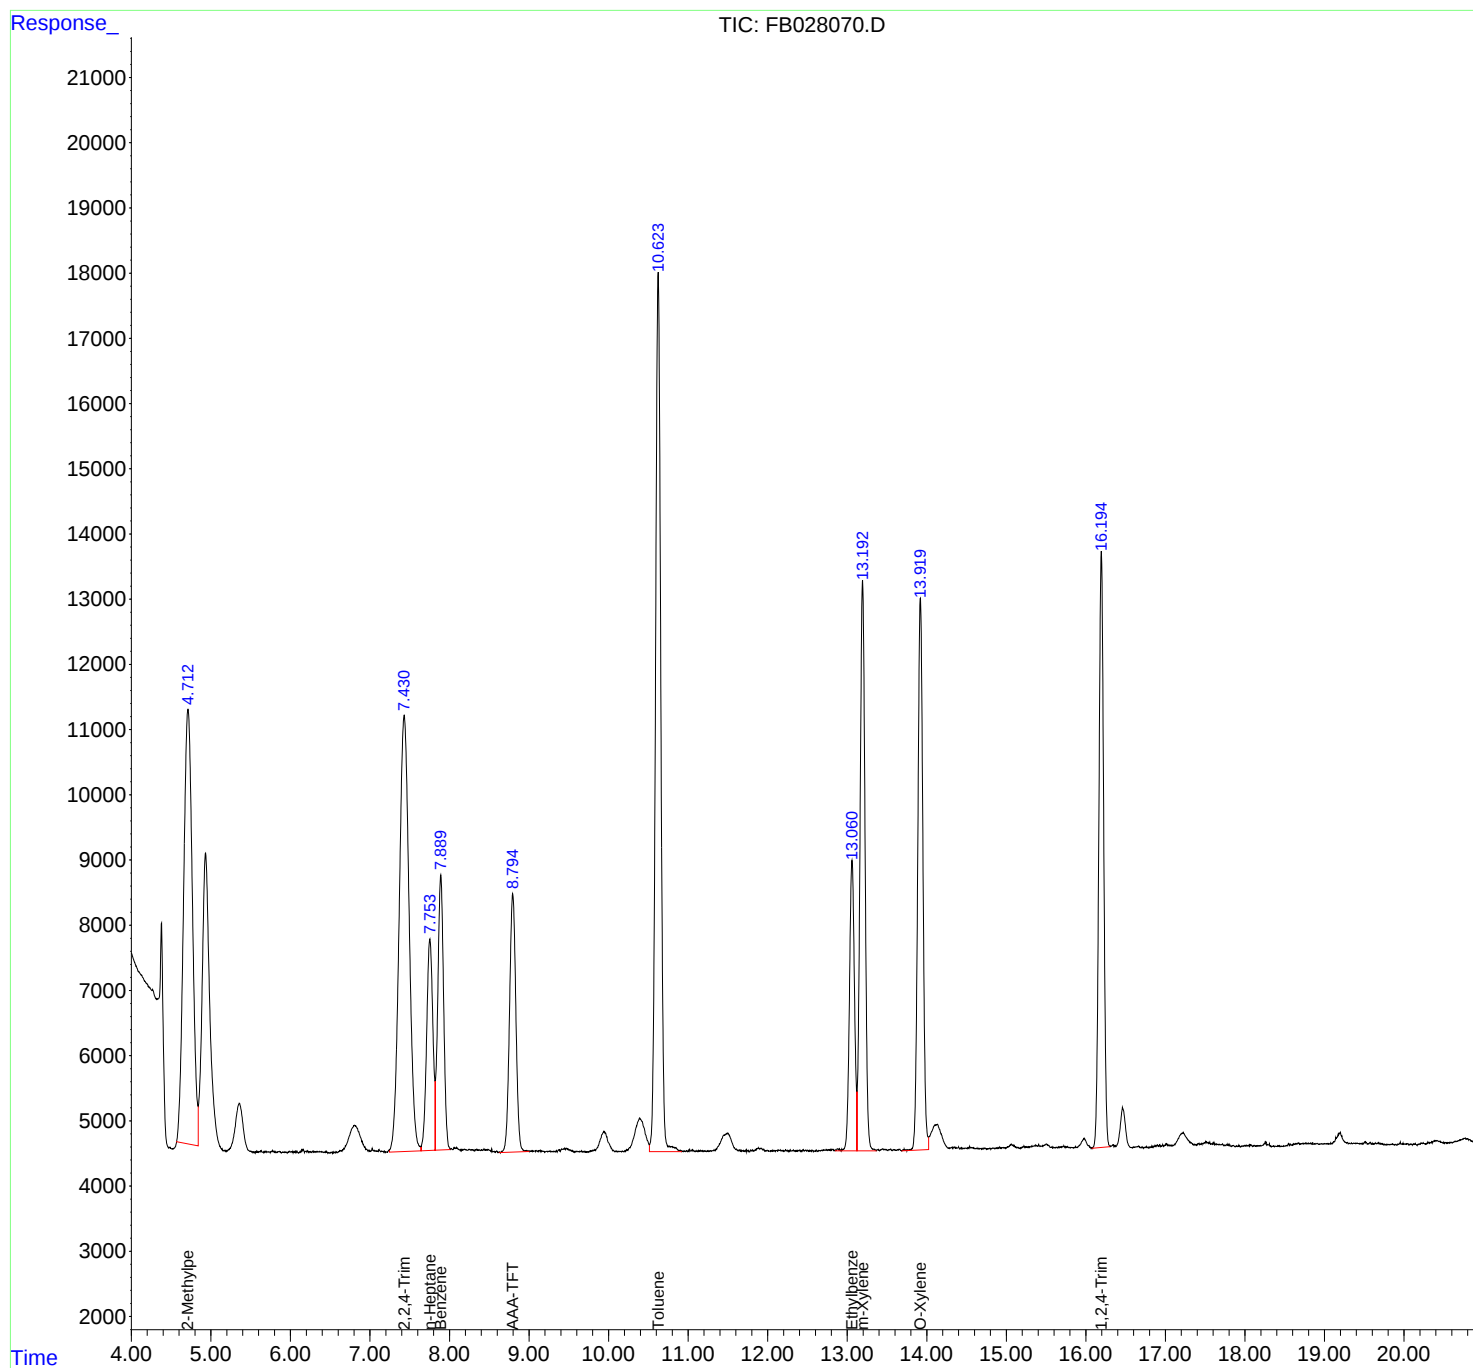


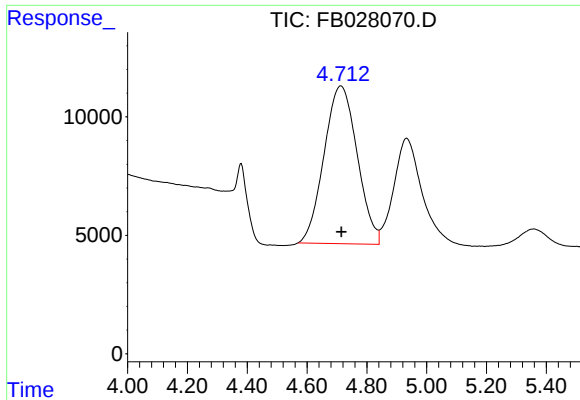

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: -0.002 min
Response: 513357
Conc: 28.38 ng/ml

Instrument :
FID_B
ClientSampleId :

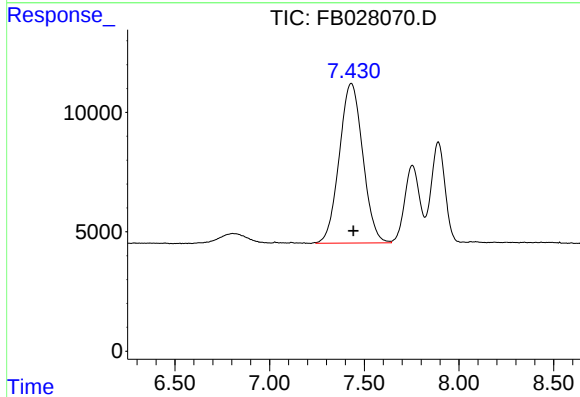


#2 2,2,4-Trimethylpentane

R.T.: 7.431 min
Delta R.T.: -0.012 min
Response: 576251
Conc: 29.39 ng/ml

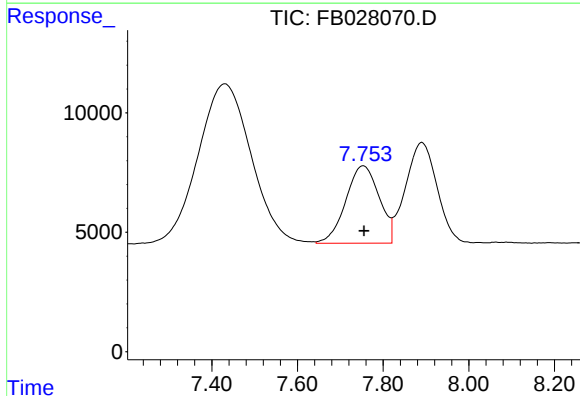


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.001 min
Response: 175463
Conc: 9.11 ng/ml

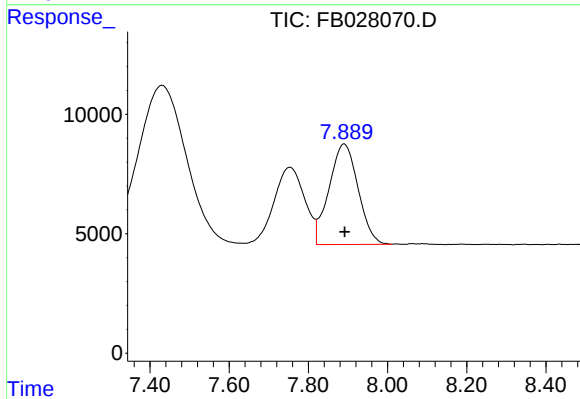

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.001 min
Response: 214679
Conc: 9.23 ng/ml

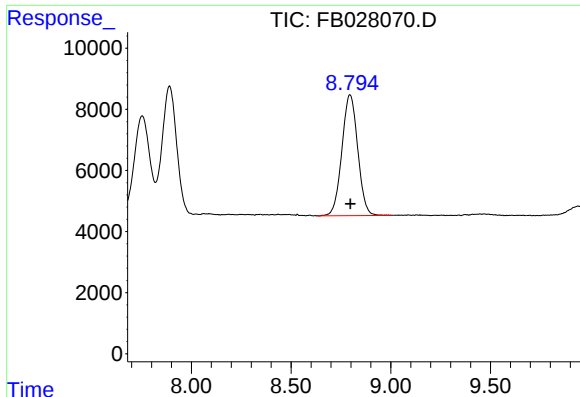

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.002 min
Response: 218363
Conc: 18.84 ng/ml

Instrument :
FID_B
ClientSampleId :

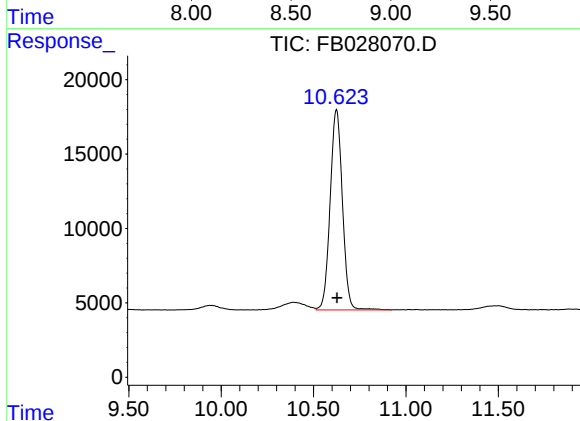


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.003 min
Response: 621215
Conc: 28.33 ng/ml

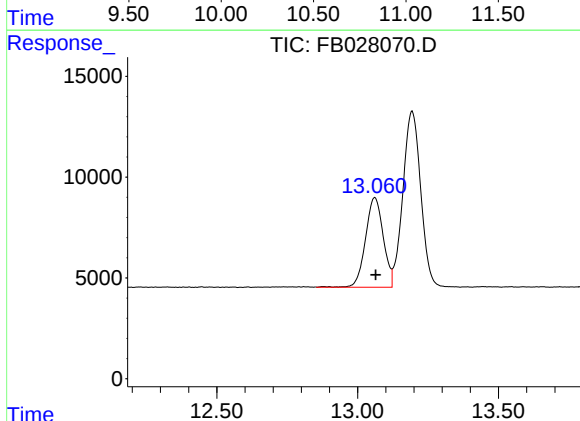


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: -0.003 min
Response: 194413
Conc: 9.43 ng/ml

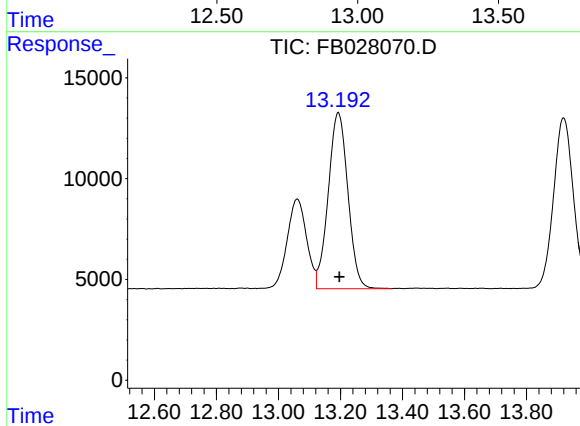

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: -0.004 min
Response: 384810
Conc: 18.81 ng/ml

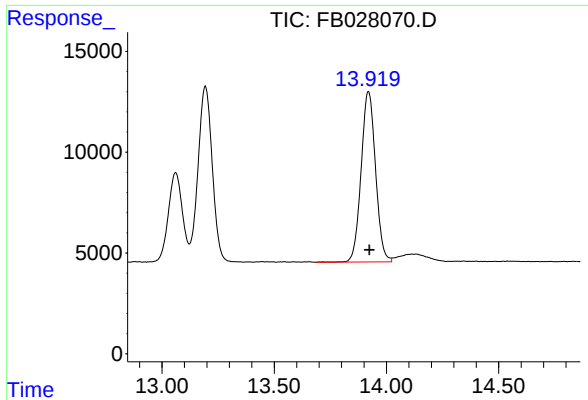

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: -0.004 min
Response: 377144
Conc: 19.04 ng/ml

Instrument :
FID_B
ClientSampleId :

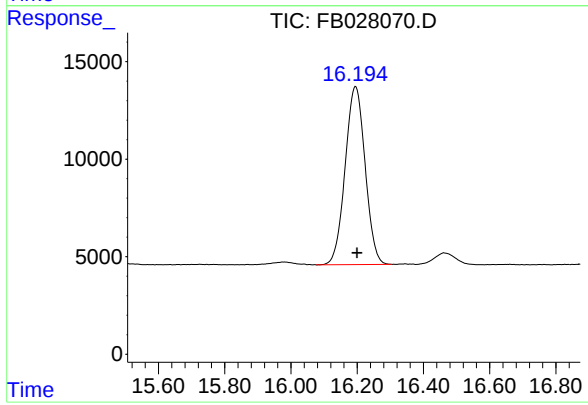

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.004 min
Response: 382305
Conc: 19.60 ng/ml