

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090220\
 Data File : FB024823.D
 Signal(s) : FID2B.CH
 Acq On : 2 Sep 2020 12:30
 Operator : DD/AJ
 Sample : L3866-02
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 03 02:42:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
 Quant Title :
 QLast Update : Mon Aug 10 12:11:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.802	315067	15.258 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.689	3950	0.164 ng/ml
2) t	2,2,4-Trimethylpentane	7.415	588	0.021 ng/ml
3) t	n-Heptane	7.782	866	0.032 ng/ml
4) t	Benzene	7.894	15545	0.443 ng/ml
6) t	Toluene	10.629	15621	0.453 ng/ml
7) t	Ethylbenzene	13.064	4295	0.134 ng/ml
8) t	m-Xylene	13.208	9492	0.304 ng/ml
9) t	O-Xylene	13.926	6175	0.204 ng/ml
10) t	1,2,4-Trimethylbenzene	16.202	2913	0.119 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090220\
Data File : FB024823.D
Signal(s) : FID2B.CH
Acq On : 2 Sep 2020 12:30
Operator : DD/AJ
Sample : L3866-02
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 03 02:42:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
Quant Title :
QLast Update : Mon Aug 10 12:11:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

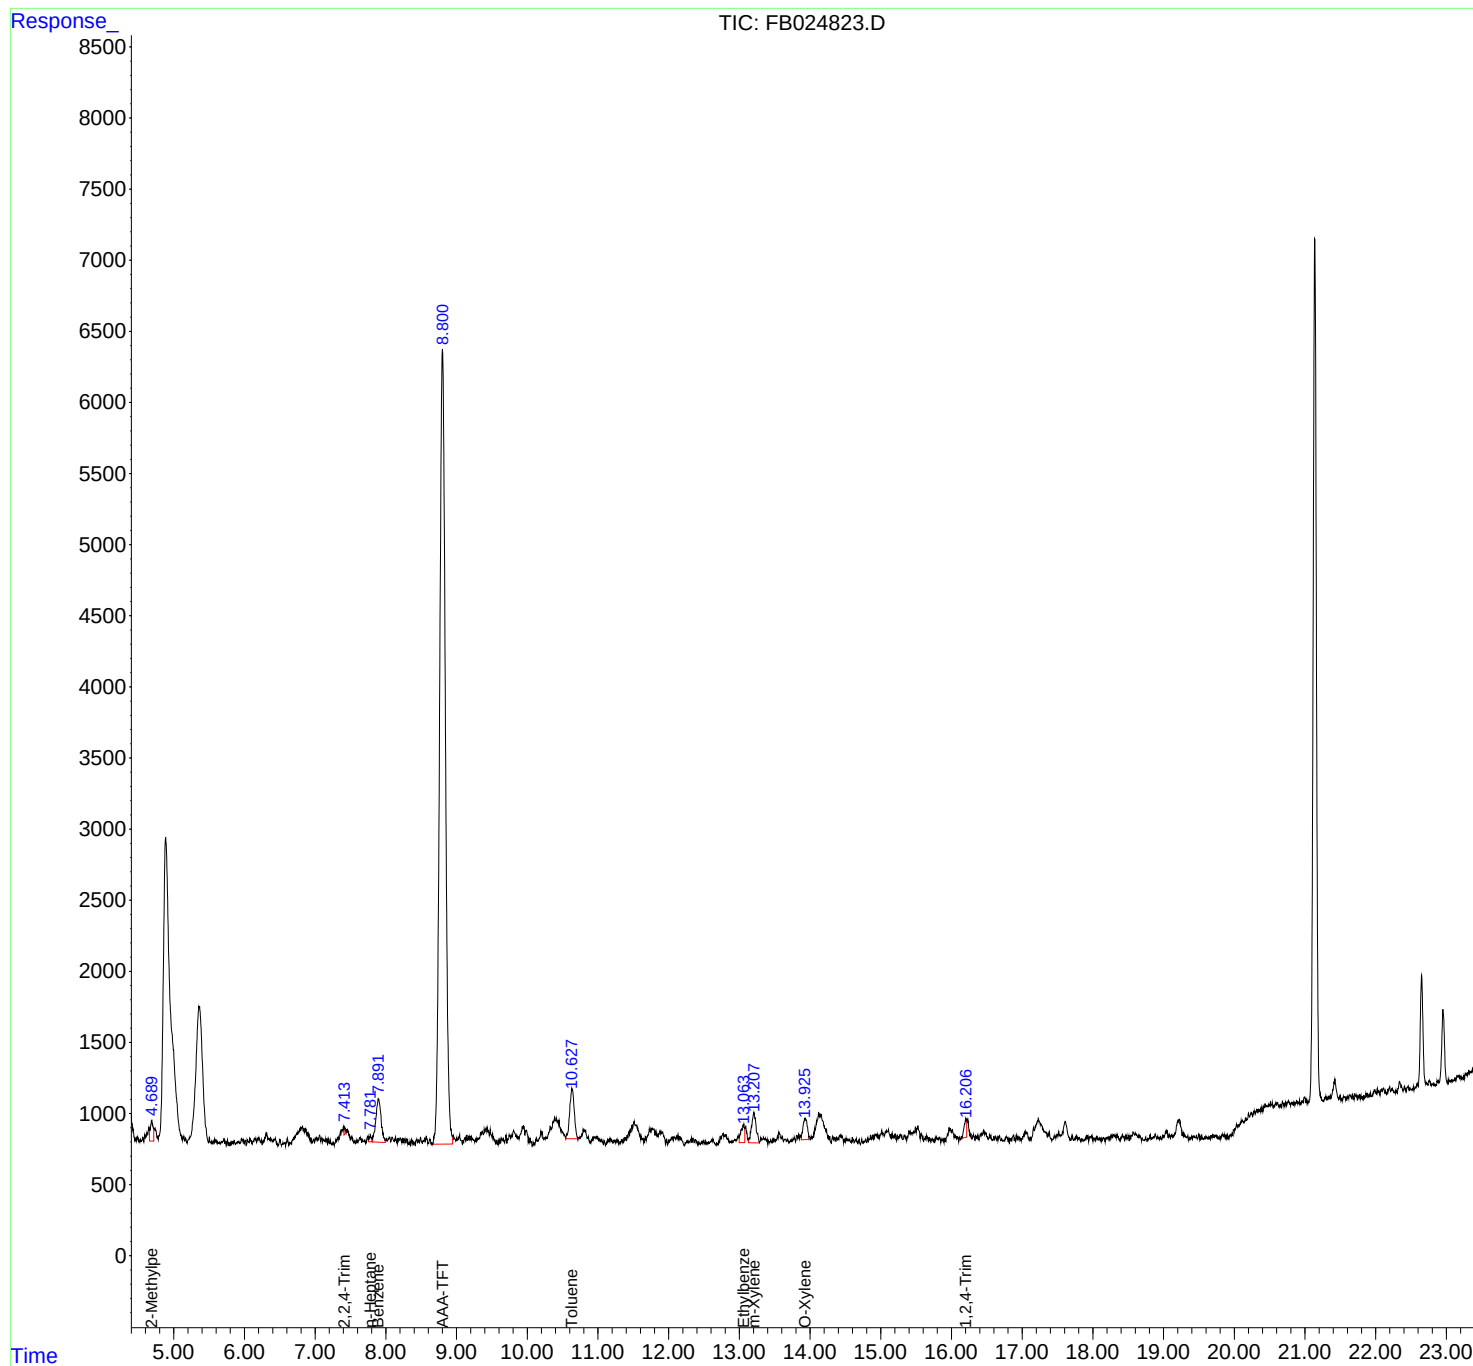

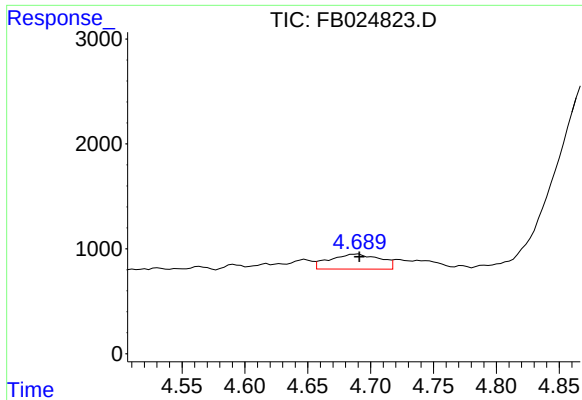


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.002 min
Response: 3950
Conc: 0.16 ng/ml

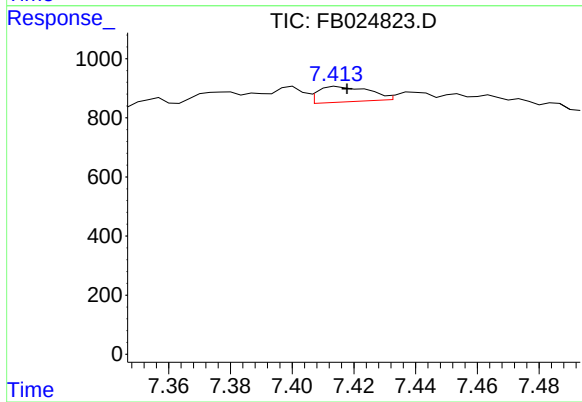


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 588
Conc: 0.02 ng/ml

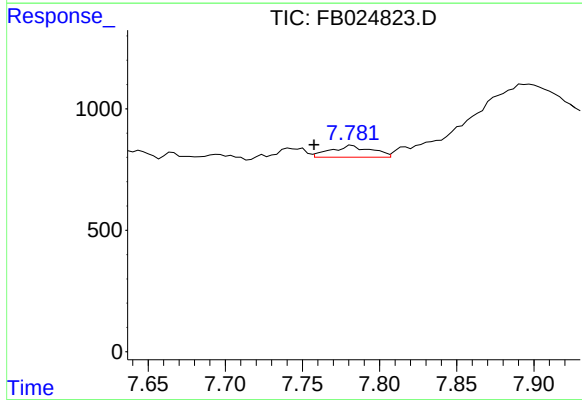


#3 n-Heptane

R.T.: 7.782 min
Delta R.T.: 0.025 min
Response: 866
Conc: 0.03 ng/ml

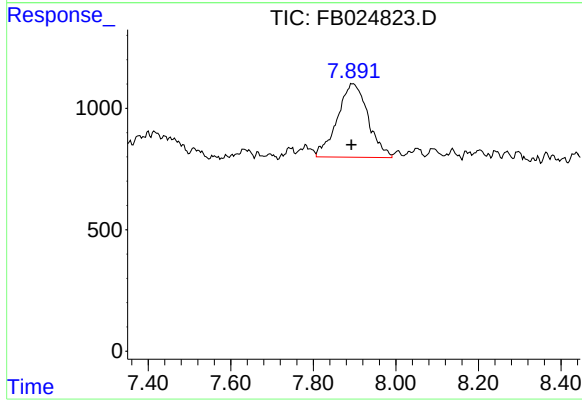


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.002 min
Response: 15545
Conc: 0.44 ng/ml

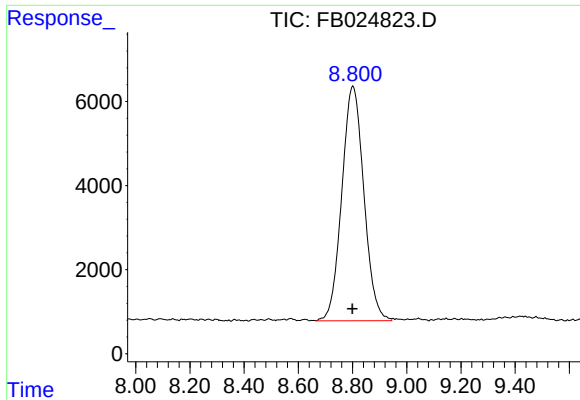


#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.003 min
Response: 315067
Conc: 15.26 ng/ml

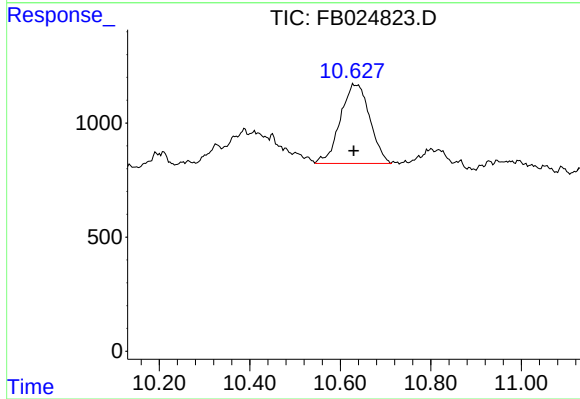


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.000 min
Response: 15621
Conc: 0.45 ng/ml

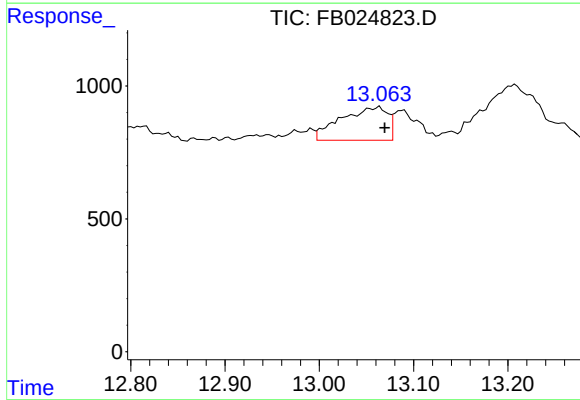


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: -0.005 min
Response: 4295
Conc: 0.13 ng/ml

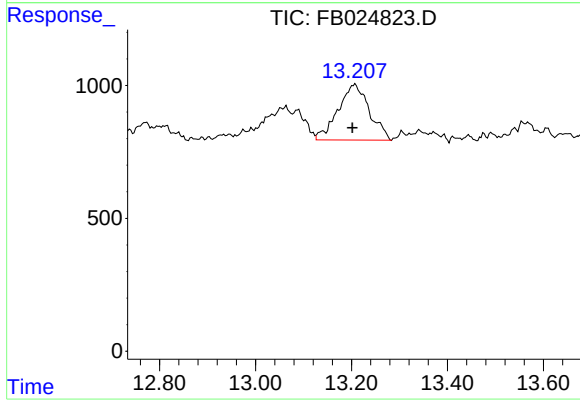


#8 m-Xylene

R.T.: 13.208 min
Delta R.T.: 0.007 min
Response: 9492
Conc: 0.30 ng/ml

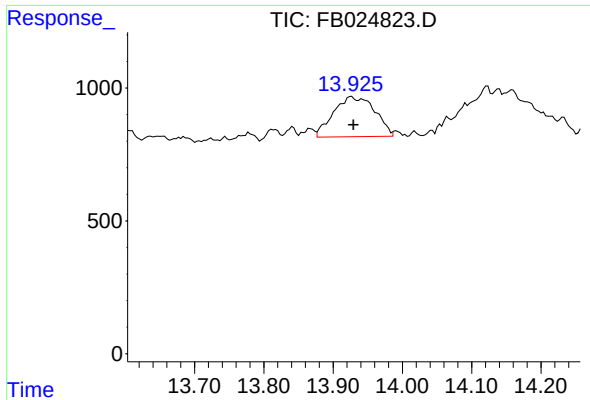

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.003 min
Response: 6175
Conc: 0.20 ng/ml

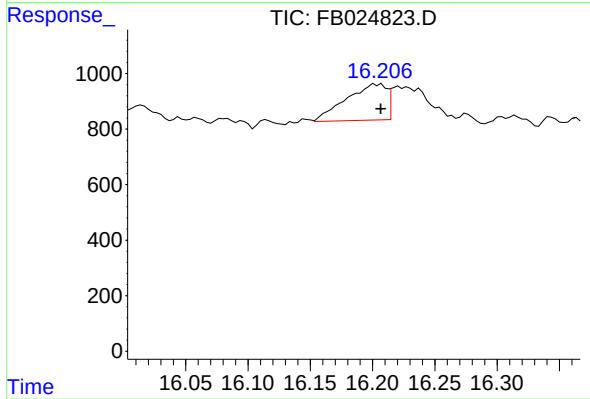

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: -0.005 min
Response: 2913
Conc: 0.12 ng/ml