

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090222\
 Data File : FB028098.D
 Signal(s) : FID2B.CH
 Acq On : 2 Sep 2022 17:29
 Operator : AJ/MA
 Sample : I.BLK
 Misc : 5.05G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 05 02:32:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	282143	24.345 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	298	0.016 ng/ml
6) t Toluene	10.644	3306	0.151 ng/ml
7) t Ethylbenzene	13.056	11564	0.561 ng/ml
8) t m-Xylene	13.262	81002	3.959 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090222\
Data File : FB028098.D
Signal(s) : FID2B.CH
Acq On : 2 Sep 2022 17:29
Operator : AJ/MA
Sample : I.BLK
Misc : 5.05G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 05 02:32:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

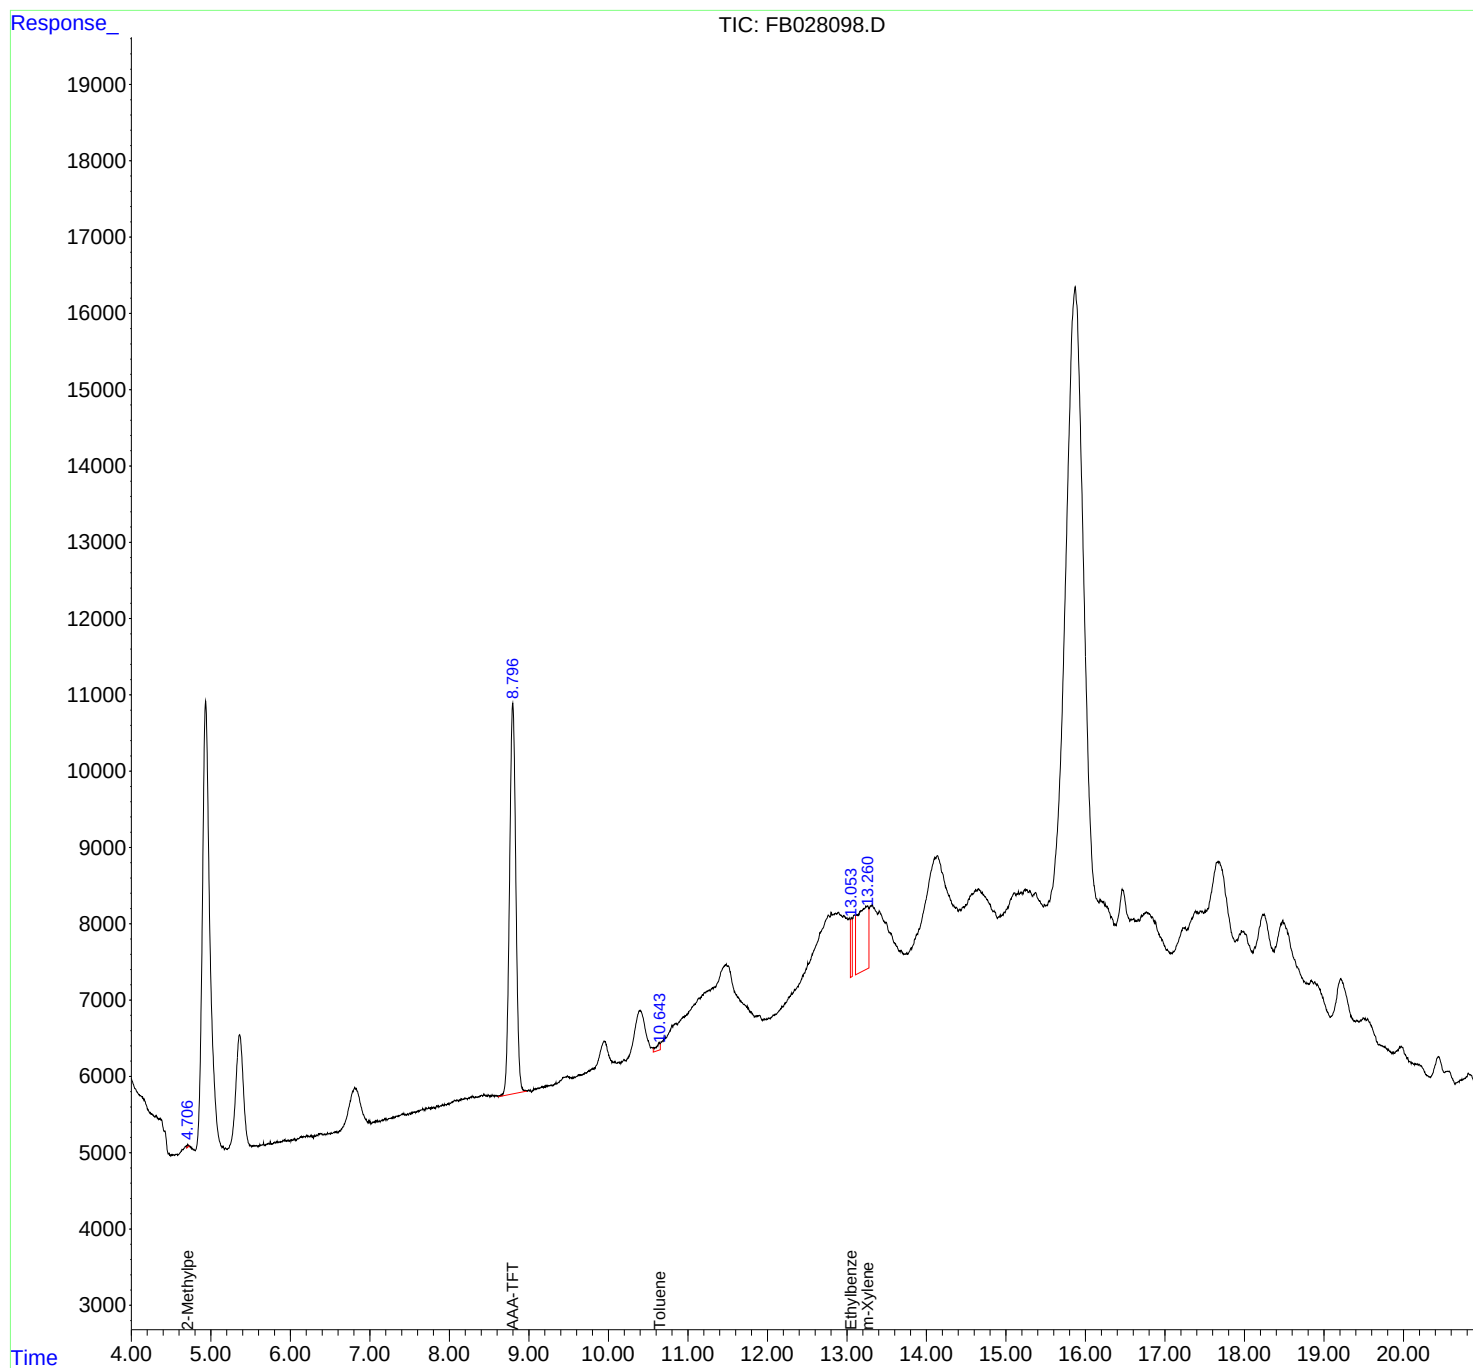


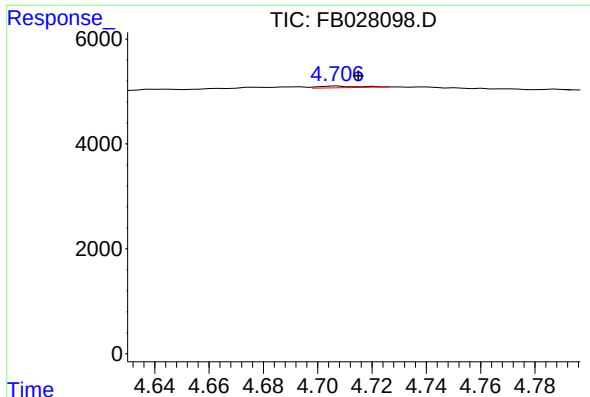

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: -0.008 min
Response: 298
Conc: 0.02 ng/ml

Instrument :
FID_B
ClientSampleId :

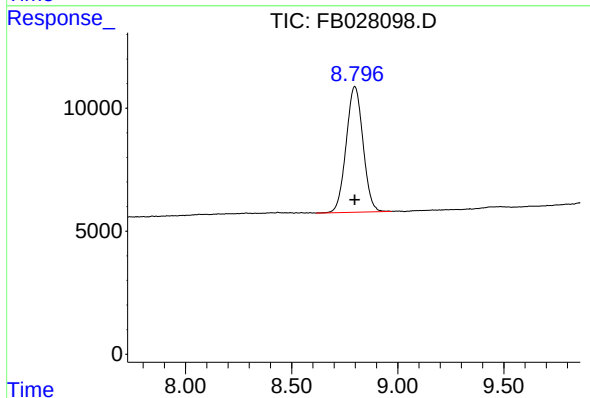


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 282143
Conc: 24.34 ng/ml

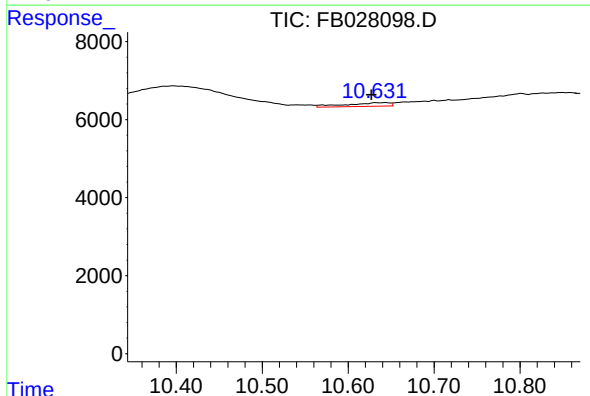


#6 Toluene

R.T.: 10.644 min
Delta R.T.: 0.017 min
Response: 3306
Conc: 0.15 ng/ml

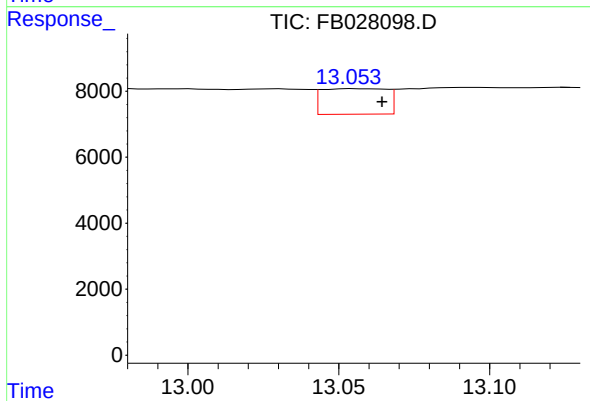

#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.009 min
Response: 11564
Conc: 0.56 ng/ml

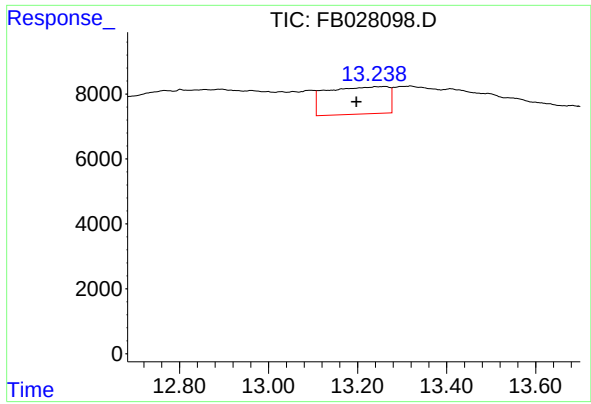

#8 m-Xylene

R.T.: 13.262 min
Delta R.T.: 0.065 min
Response: 81002
Conc: 3.96 ng/ml

Instrument :
FID_B
ClientSampleId :