

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090222\
 Data File : FB028101.D
 Signal(s) : FID2B.CH
 Acq On : 2 Sep 2022 23:03
 Operator : AJ/MA
 Sample : N4490-04MSD
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 06 06:34:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	82728	7.138 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	283291	15.659 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	228529	11.654 ng/ml
3) t n-Heptane	7.755	72190	3.747 ng/ml
4) t Benzene	7.891	126463	5.439 ng/ml
6) t Toluene	10.624	273585	12.476 ng/ml
7) t Ethylbenzene	13.047	241642	11.726 ng/ml
8) t m-Xylene	13.190	128658	6.287 ng/ml
9) t O-Xylene	13.921	162225	8.189 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	80780	4.142 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090222\
Data File : FB028101.D
Signal(s) : FID2B.CH
Acq On : 2 Sep 2022 23:03
Operator : AJ/MA
Sample : N4490-04MSD
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 06 06:34:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

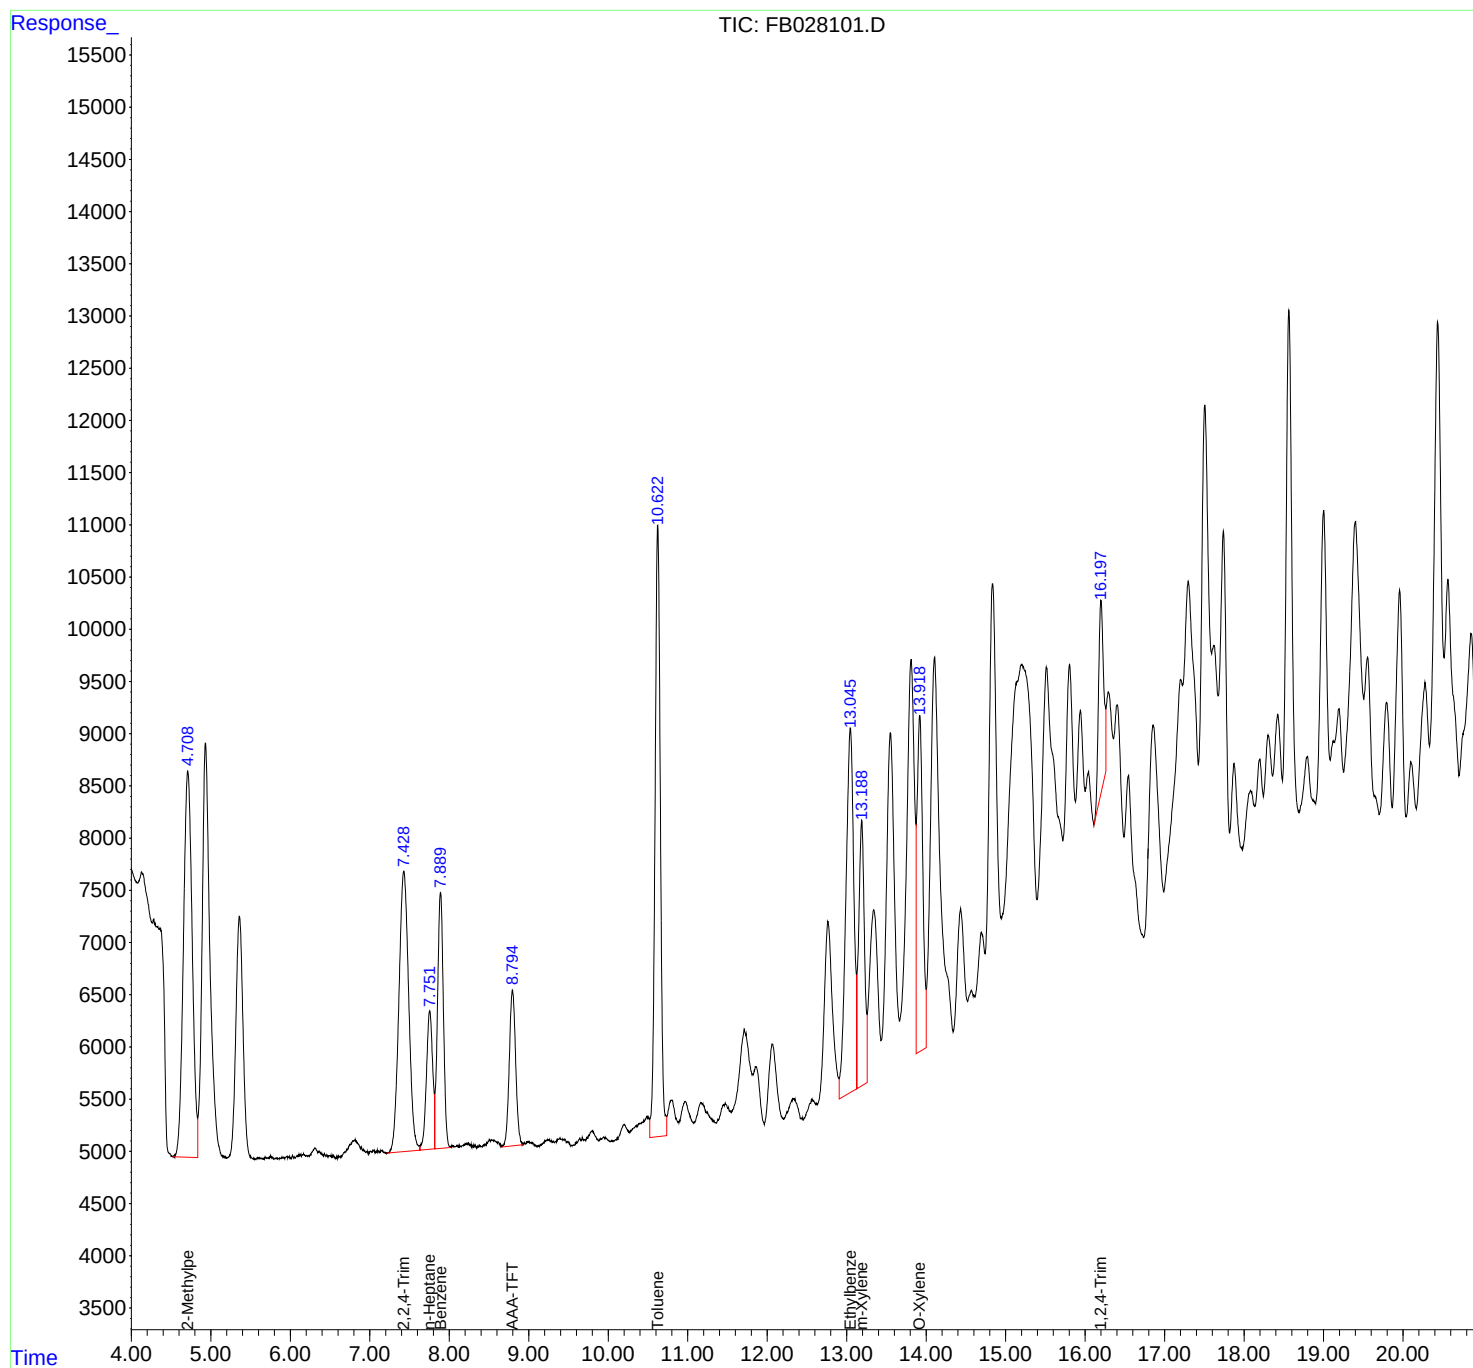


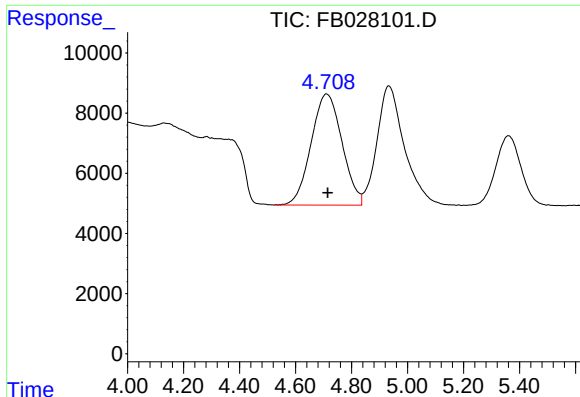

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: -0.005 min
Response: 283291
Conc: 15.66 ng/ml

Instrument :
FID_B
ClientSampleId :

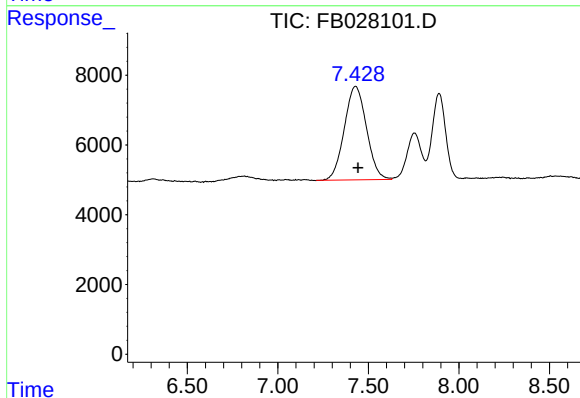


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: -0.013 min
Response: 228529
Conc: 11.65 ng/ml

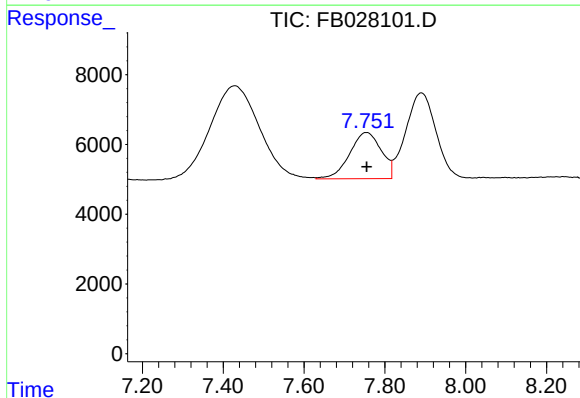


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 72190
Conc: 3.75 ng/ml

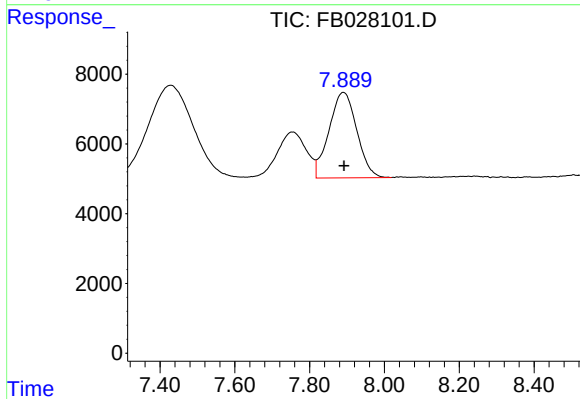

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.001 min
Response: 126463
Conc: 5.44 ng/ml

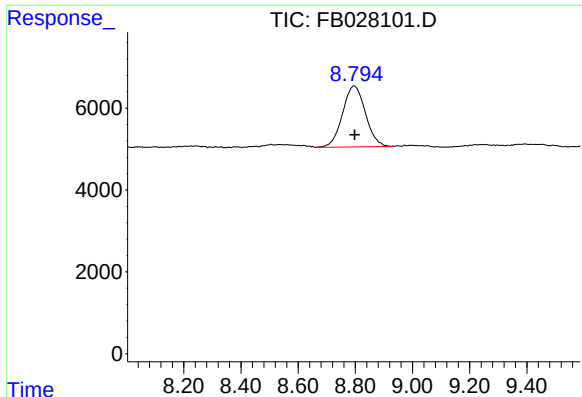

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.002 min
Response: 82728
Conc: 7.14 ng/ml

Instrument :
FID_B
ClientSampleId :

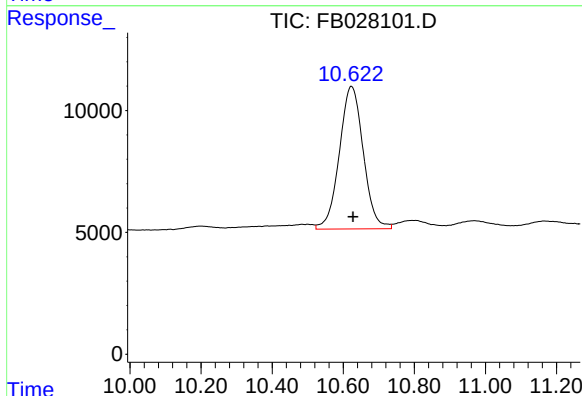


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.003 min
Response: 273585
Conc: 12.48 ng/ml

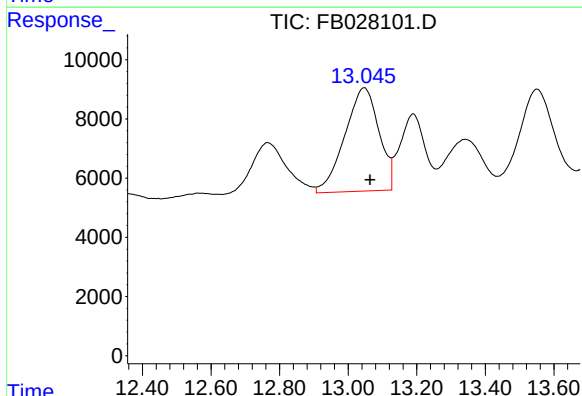


#7 Ethylbenzene

R.T.: 13.047 min
Delta R.T.: -0.017 min
Response: 241642
Conc: 11.73 ng/ml

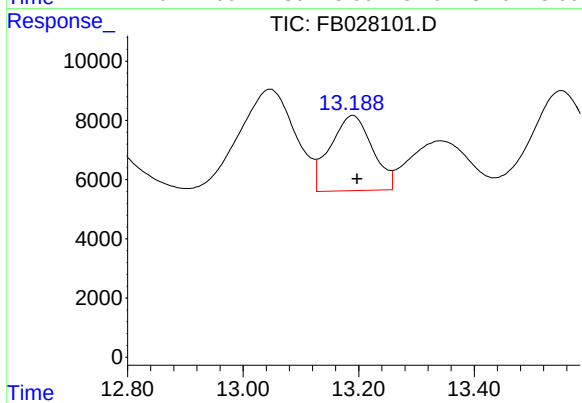

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: -0.007 min
Response: 128658
Conc: 6.29 ng/ml

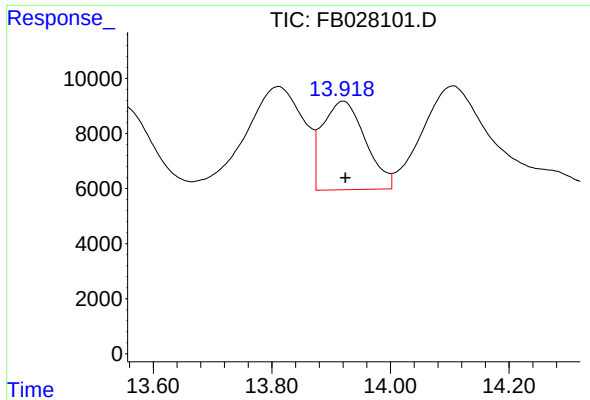

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: -0.004 min
Response: 162225
Conc: 8.19 ng/ml

Instrument :
FID_B
ClientSampleId :

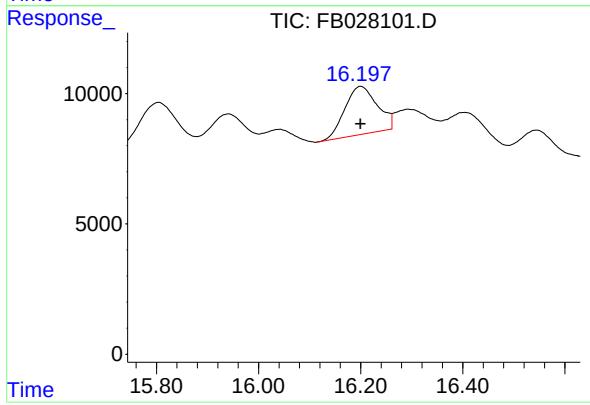

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: 0.001 min
Response: 80780
Conc: 4.14 ng/ml