

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090222\
 Data File : FB028099.D
 Signal(s) : FID2B.CH
 Acq On : 2 Sep 2022 20:35
 Operator : AJ/MA
 Sample : 20 PPB GRO CCC
 Misc : 5.05G/5.00 ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Integration File: Calibration.e
 Quant Time: Sep 06 06:31:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	263287	22.718 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	535974	29.627 ng/ml
2) t 2,2,4-Trimethylpentane	7.432	574434	29.293 ng/ml
3) t n-Heptane	7.755	185012	9.603 ng/ml
4) t Benzene	7.892	227613	9.789 ng/ml
6) t Toluene	10.626	649393	29.615 ng/ml
7) t Ethylbenzene	13.062	204163	9.907 ng/ml
8) t m-Xylene	13.195	402036	19.647 ng/ml
9) t O-Xylene	13.922	388456	19.610 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	371694	19.060 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090222\
Data File : FB028099.D
Signal(s) : FID2B.CH
Acq On : 2 Sep 2022 20:35
Operator : AJ/MA
Sample : 20 PPB GRO CCC
Misc : 5.05G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Integration File: Calibration.e
Quant Time: Sep 06 06:31:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

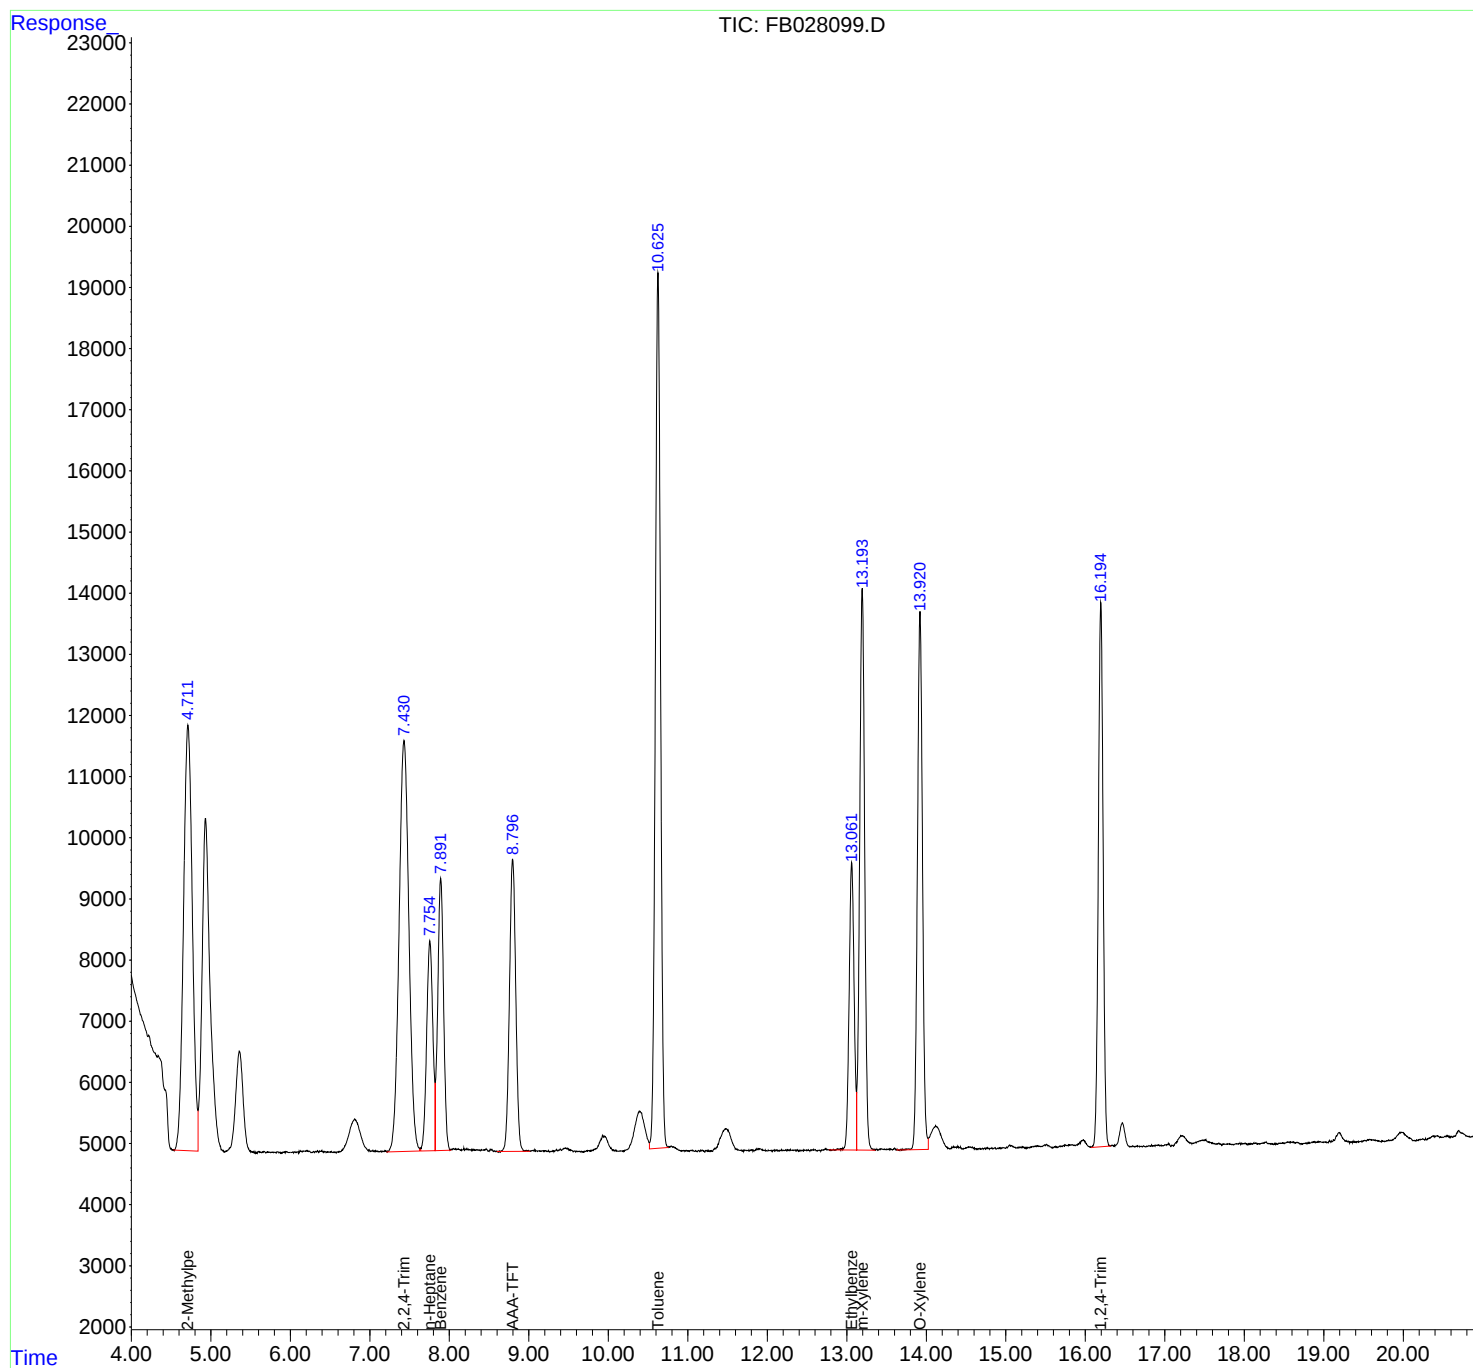


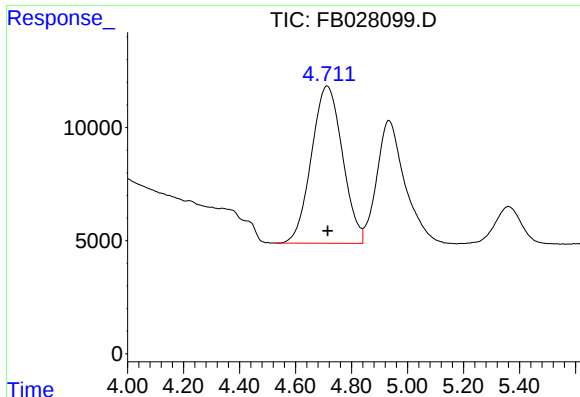

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: -0.002 min
Response: 535974
Conc: 29.63 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

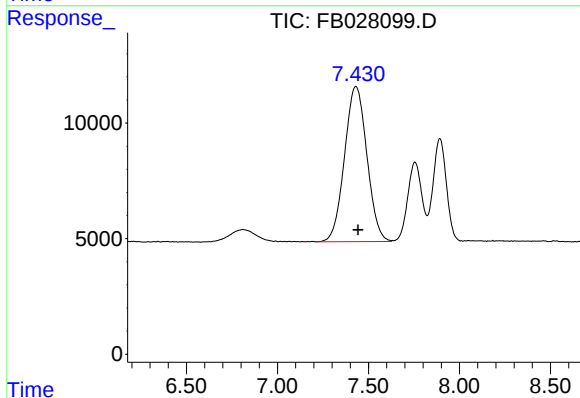


#2 2,2,4-Trimethylpentane

R.T.: 7.432 min
Delta R.T.: -0.011 min
Response: 574434
Conc: 29.29 ng/ml

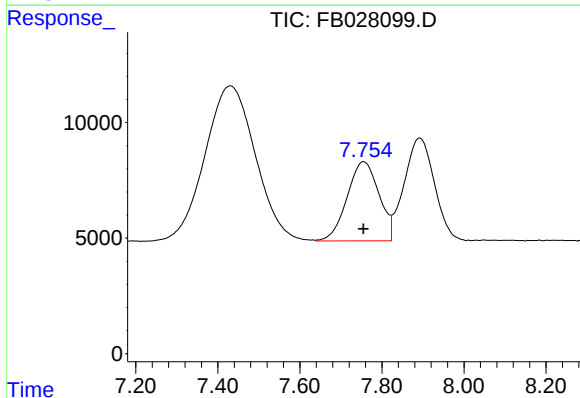


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 185012
Conc: 9.60 ng/ml

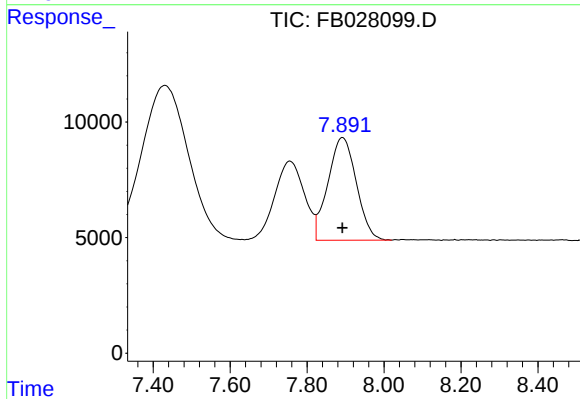

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 227613
Conc: 9.79 ng/ml

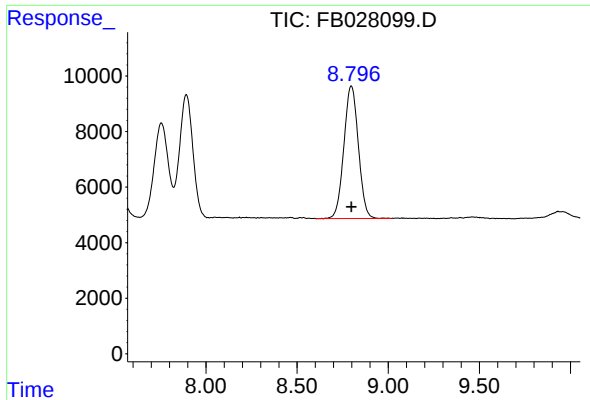

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 263287
Conc: 22.72 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

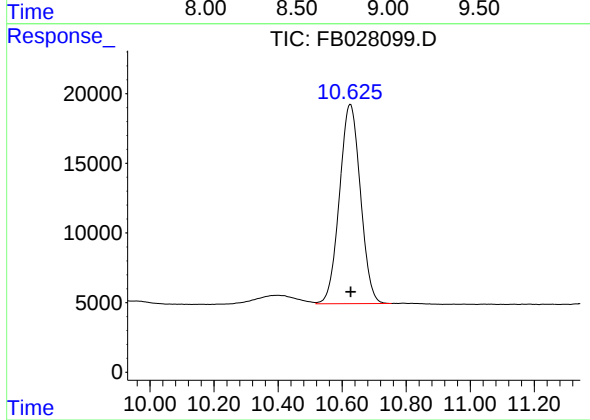


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.002 min
Response: 649393
Conc: 29.61 ng/ml

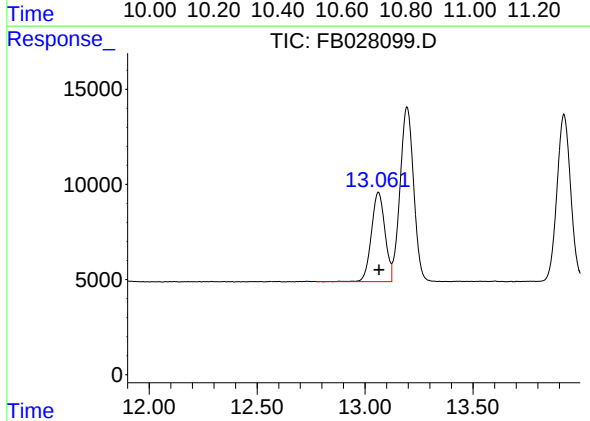


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: -0.002 min
Response: 204163
Conc: 9.91 ng/ml

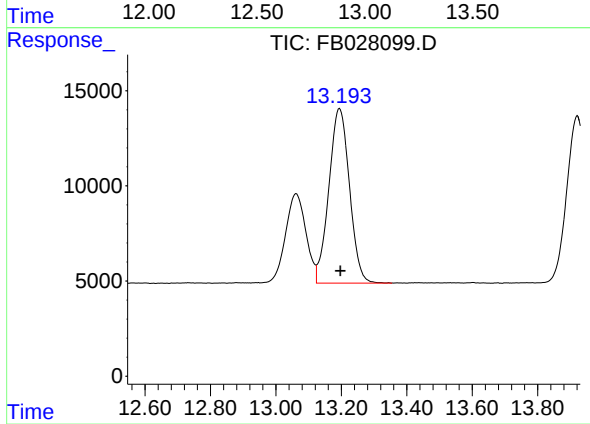

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: -0.002 min
Response: 402036
Conc: 19.65 ng/ml

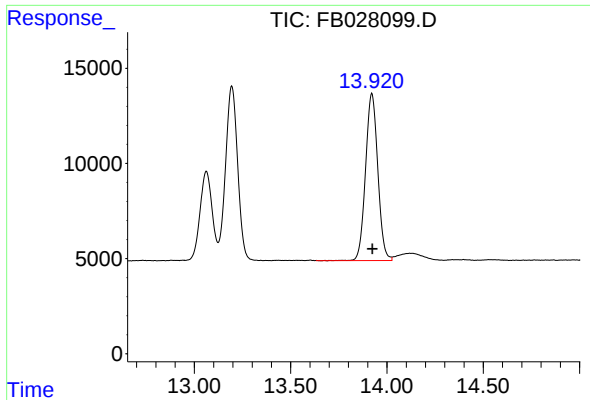

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.003 min
Response: 388456
Conc: 19.61 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

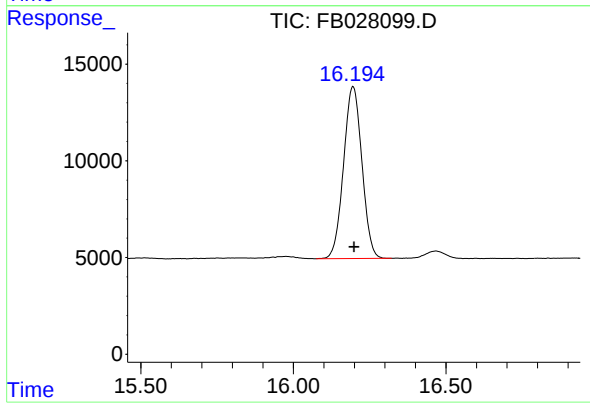

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: -0.003 min
Response: 371694
Conc: 19.06 ng/ml