

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090419\
Data File : FB022282.D
Signal(s) : FID2B.CH
Acq On : 4 Sep 2019 19:33
Operator : DD/AJ
Sample : K4668-02
Misc : 5.02G/5.00ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 05 01:19:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.977	521001	17.912 ng/ml
Target Compounds				
6) t	Toluene	10.819	8245	0.173 ng/ml
8) t	m-Xylene	13.396	7281	0.274 ng/ml
9) t	O-Xylene	14.131	11491	0.474 ng/ml
10) t	1,2,4-Trimethylbenzene	16.411	23555	0.903 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090419\
Data File : FB022282.D
Signal(s) : FID2B.CH
Acq On : 4 Sep 2019 19:33
Operator : DD/AJ
Sample : K4668-02
Misc : 5.02G/5.00ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 05 01:19:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

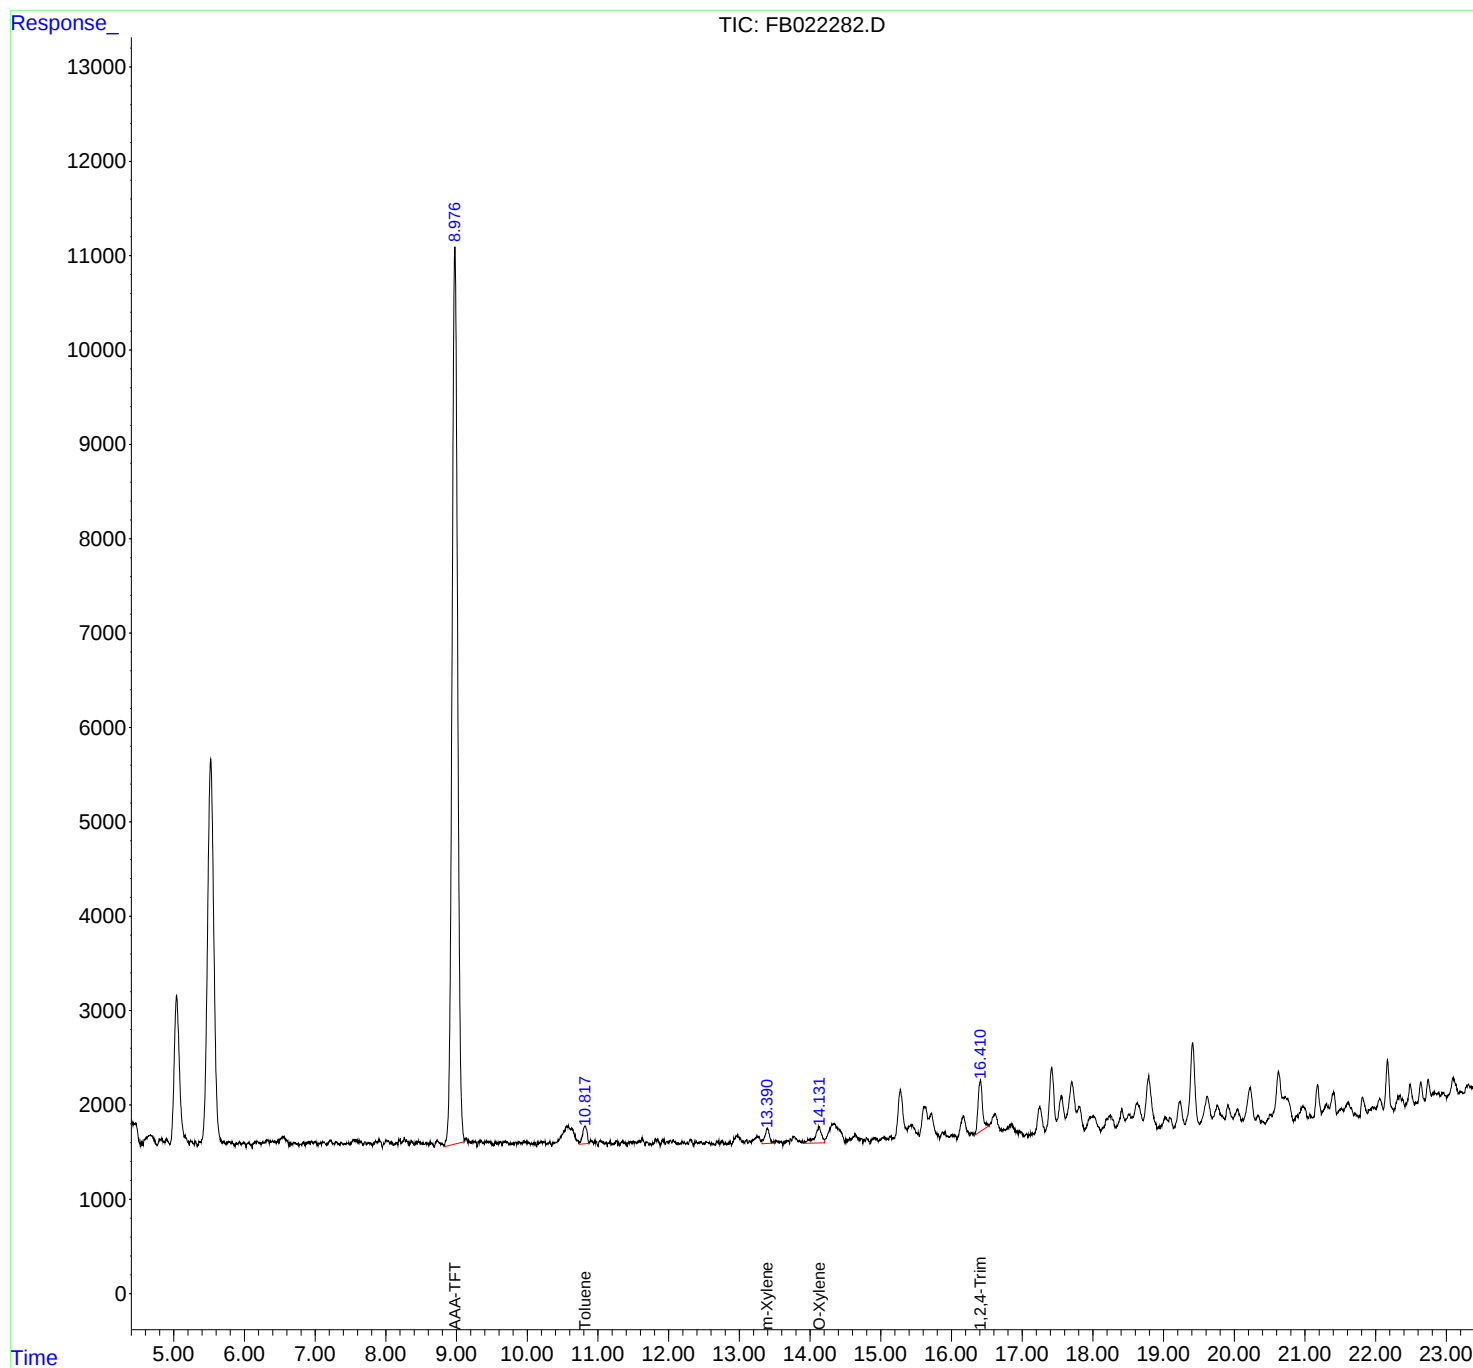


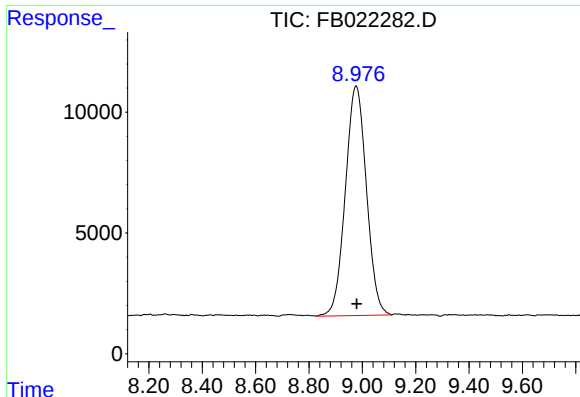

#5 AAA-TFT


R.T.: 8.977 min
Delta R.T.: -0.002 min
Response: 521001
Conc: 17.91 ng/ml

Instrument :
FID_B
ClientSampleId :

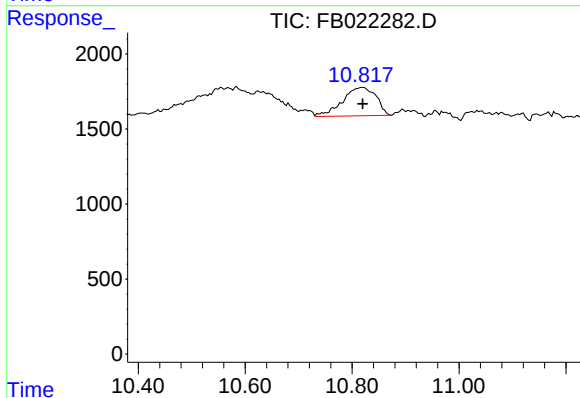


#6 Toluene

R.T.: 10.819 min
Delta R.T.: 0.000 min
Response: 8245
Conc: 0.17 ng/ml

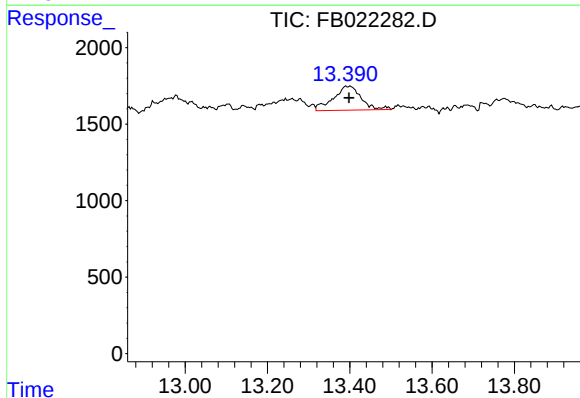


#8 m-Xylene

R.T.: 13.396 min
Delta R.T.: -0.001 min
Response: 7281
Conc: 0.27 ng/ml

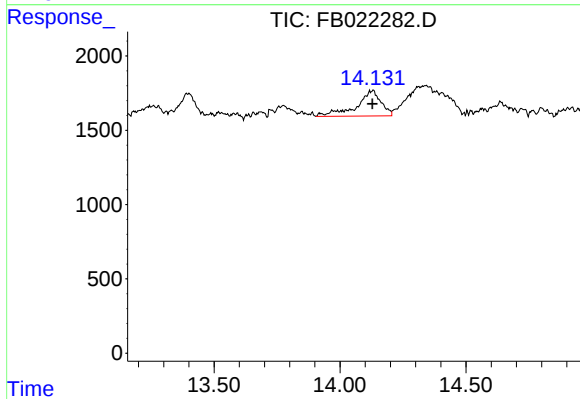

#9 O-Xylene

R.T.: 14.131 min
Delta R.T.: 0.003 min
Response: 11491
Conc: 0.47 ng/ml

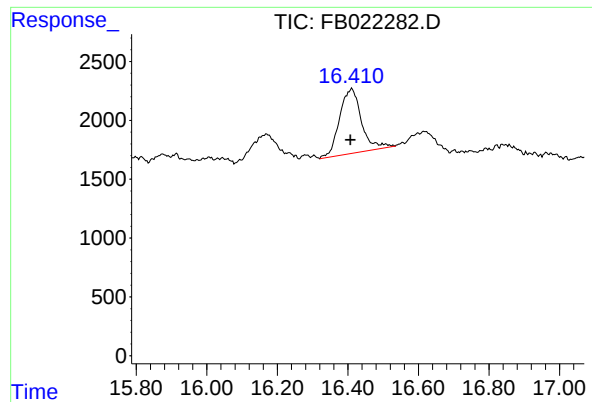

#10 1,2,4-Trimethylbenzene

R.T.: 16.411 min
Delta R.T.: 0.003 min
Response: 23555
Conc: 0.90 ng/ml

Instrument :
FID_B
ClientSampleId :