

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090419\
 Data File : FB022280.D
 Signal(s) : FID2B.CH
 Acq On : 4 Sep 2019 19:03
 Operator : DD/AJ
 Sample : BSF0904S1
 Misc : 5.00G/5.00ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0904S1

Integration File: Calibration.e
 Quant Time: Sep 05 01:19:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.977	567268	19.502 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.846	1438407	29.276 ng/ml
2) t 2,2,4-Trimethylpentane	7.596	1589579	30.783 ng/ml
3) t n-Heptane	7.935	513921	10.211 ng/ml
4) t Benzene	8.071	600255	10.114 ng/ml
6) t Toluene	10.818	1556564	32.719 ng/ml
7) t Ethylbenzene	13.263	354237	11.816 ng/ml
8) t m-Xylene	13.397	620927	23.373 ng/ml
9) t O-Xylene	14.126	527660	21.750 ng/ml
10) t 1,2,4-Trimethylbenzene	16.406	500686	19.204 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090419\
Data File : FB022280.D
Signal(s) : FID2B.CH
Acq On : 4 Sep 2019 19:03
Operator : DD/AJ
Sample : BSF0904S1
Misc : 5.00G/5.00ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0904S1

Integration File: Calibration.e
Quant Time: Sep 05 01:19:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

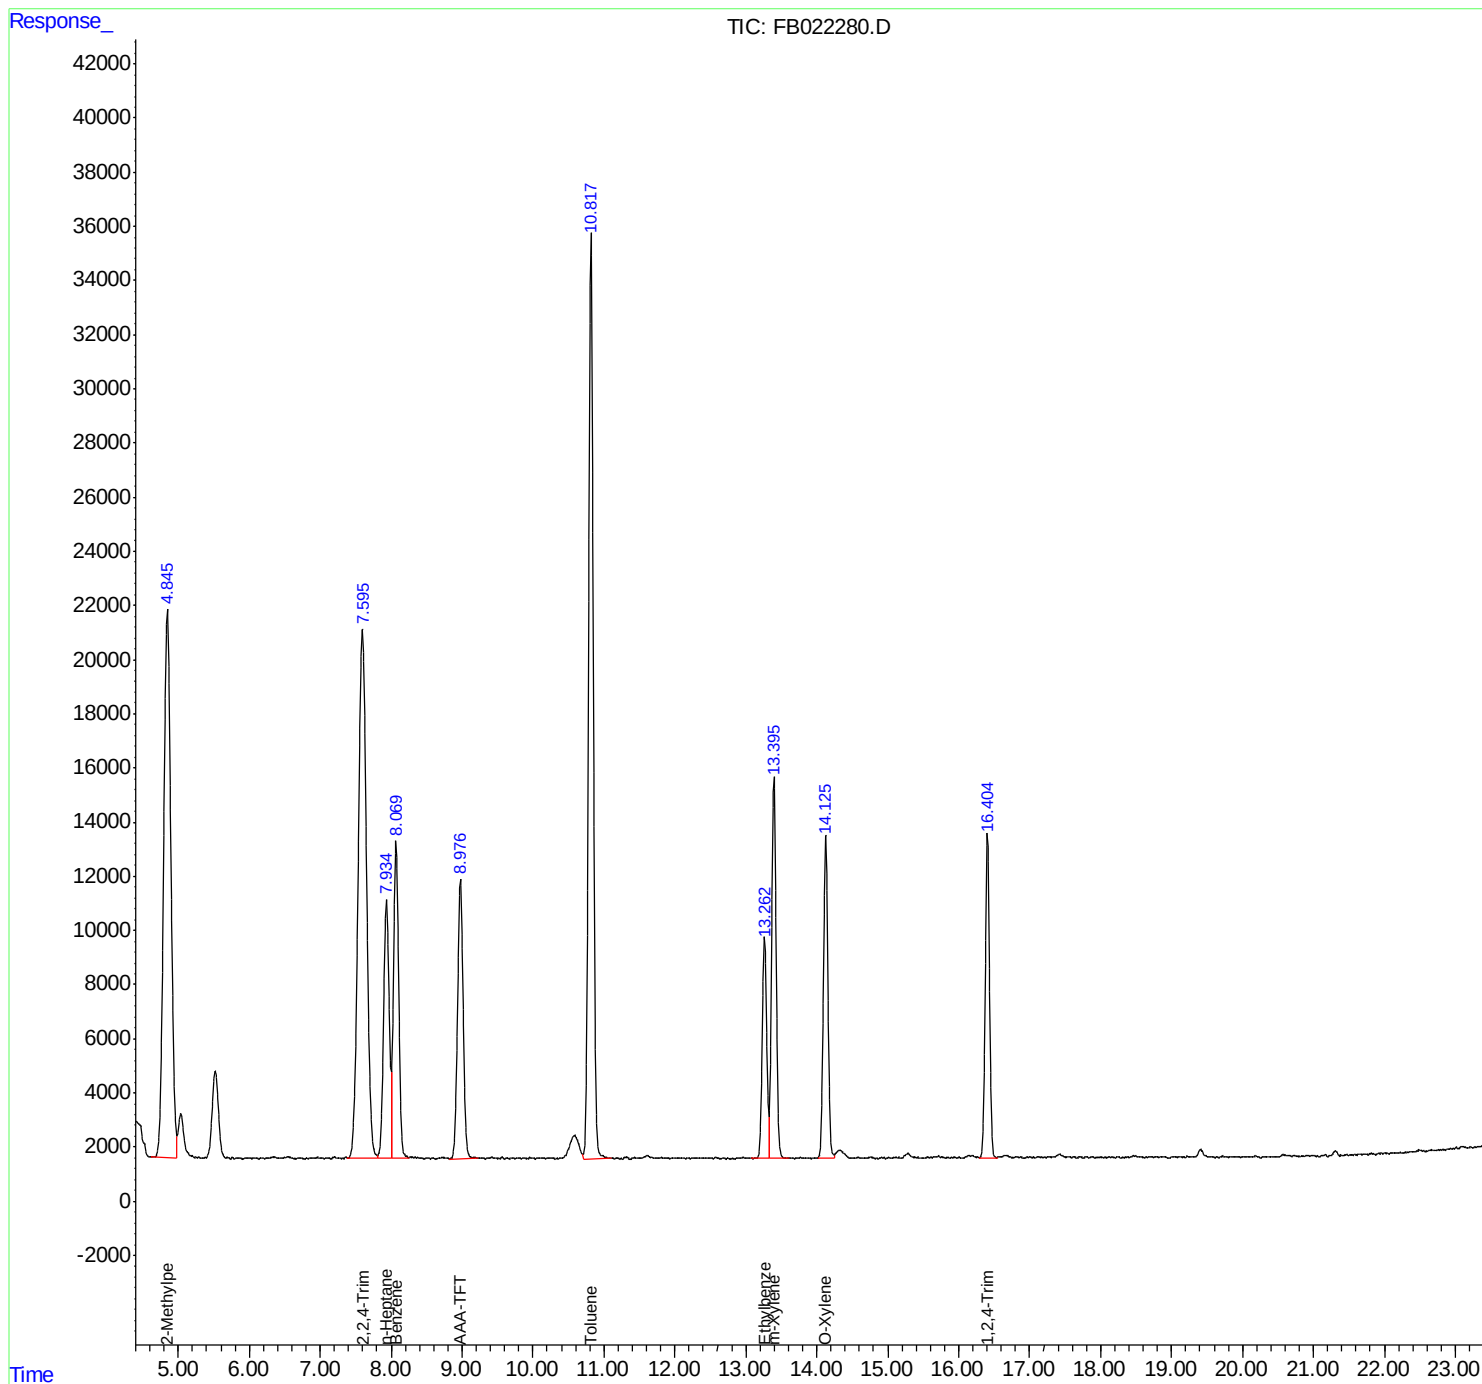


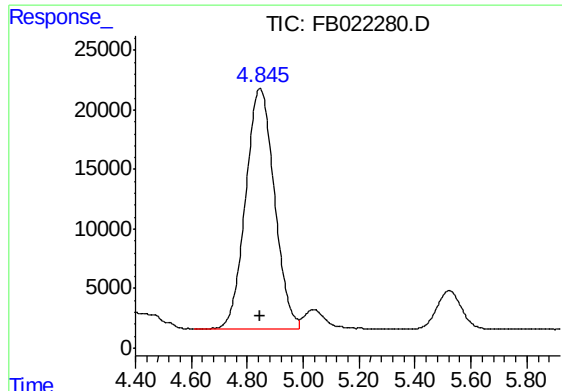

#1 2-Methylpentane


R.T.: 4.846 min
Delta R.T.: 0.000 min
Response: 1438407
Conc: 29.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0904S1

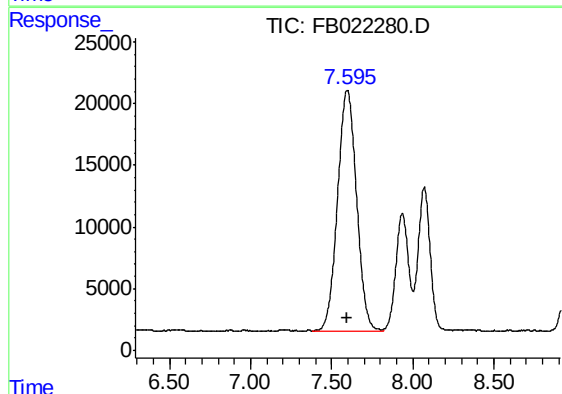


#2 2,2,4-Trimethylpentane

R.T.: 7.596 min
Delta R.T.: -0.002 min
Response: 1589579
Conc: 30.78 ng/ml

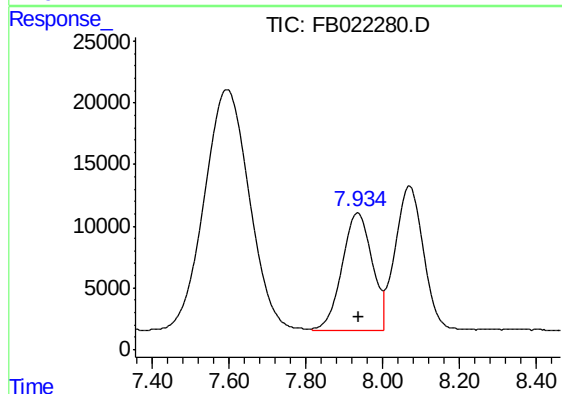


#3 n-Heptane

R.T.: 7.935 min
Delta R.T.: -0.002 min
Response: 513921
Conc: 10.21 ng/ml

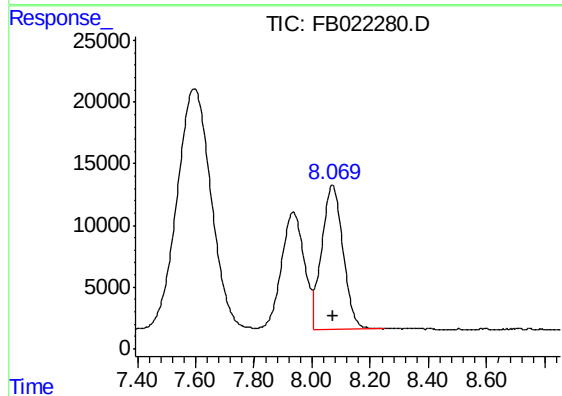

#4 Benzene


R.T.: 8.071 min
Delta R.T.: -0.002 min
Response: 600255
Conc: 10.11 ng/ml

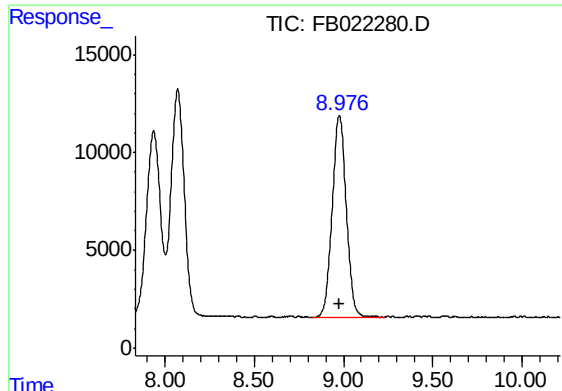

#5 AAA-TFT


R.T.: 8.977 min
Delta R.T.: -0.002 min
Response: 567268
Conc: 19.50 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0904S1

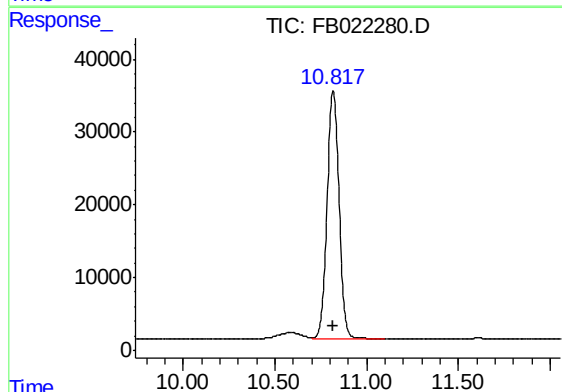


#6 Toluene

R.T.: 10.818 min
Delta R.T.: -0.001 min
Response: 1556564
Conc: 32.72 ng/ml

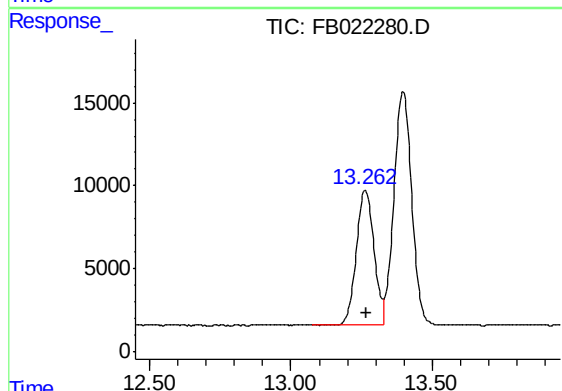


#7 Ethylbenzene

R.T.: 13.263 min
Delta R.T.: -0.002 min
Response: 354237
Conc: 11.82 ng/ml

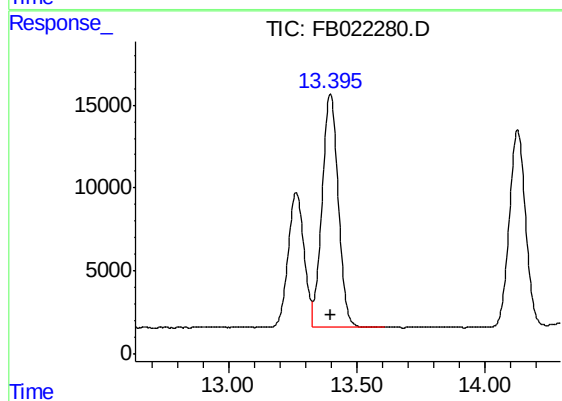

#8 m-Xylene


R.T.: 13.397 min
Delta R.T.: -0.001 min
Response: 620927
Conc: 23.37 ng/ml

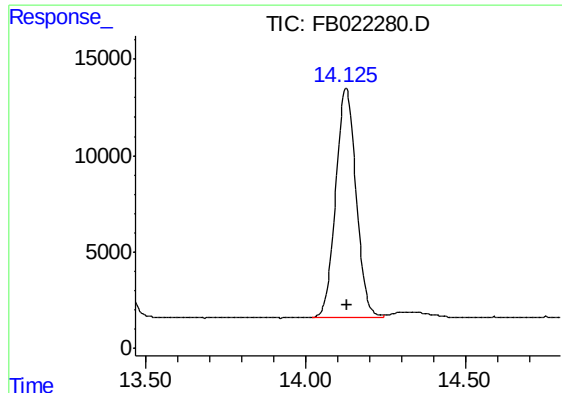

#9 O-Xylene

R.T.: 14.126 min
Delta R.T.: -0.002 min
Response: 527660
Conc: 21.75 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0904S1

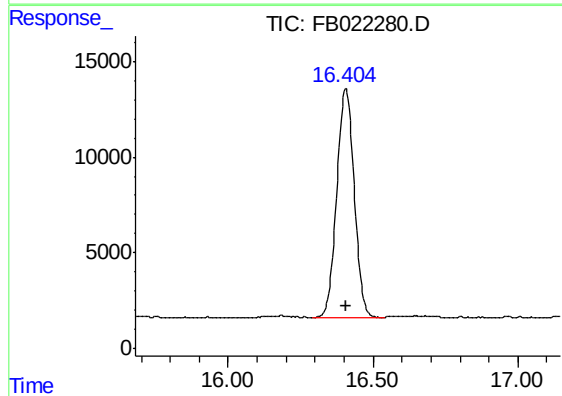

#10 1,2,4-Trimethylbenzene

R.T.: 16.406 min
Delta R.T.: -0.001 min
Response: 500686
Conc: 19.20 ng/ml