

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090419\
 Data File : FB022286.D
 Signal(s) : FID2B.CH
 Acq On : 4 Sep 2019 22:06
 Operator : DD/AJ
 Sample : K4688-02MS
 Misc : 5.02G/5.00ML DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 CLEARWELLMS

Integration File: Calibration.e
 Quant Time: Sep 05 01:20:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.976	664248	22.836 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.846	1407955	28.656 ng/ml
2) t 2,2,4-Trimethylpentane	7.595	1559622	30.203 ng/ml
3) t n-Heptane	7.934	502196	9.978 ng/ml
4) t Benzene	8.069	609816	10.275 ng/ml
6) t Toluene	10.817	1631800	34.301 ng/ml
7) t Ethylbenzene	13.262	392511	13.093 ng/ml
8) t m-Xylene	13.395	687010	25.860 ng/ml
9) t O-Xylene	14.124	580243	23.918 ng/ml
10) t 1,2,4-Trimethylbenzene	16.405	508297	19.496 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090419\
Data File : FB022286.D
Signal(s) : FID2B.CH
Acq On : 4 Sep 2019 22:06
Operator : DD/AJ
Sample : K4688-02MS
Misc : 5.02G/5.00ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
CLEARWELLMS

Integration File: Calibration.e
Quant Time: Sep 05 01:20:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

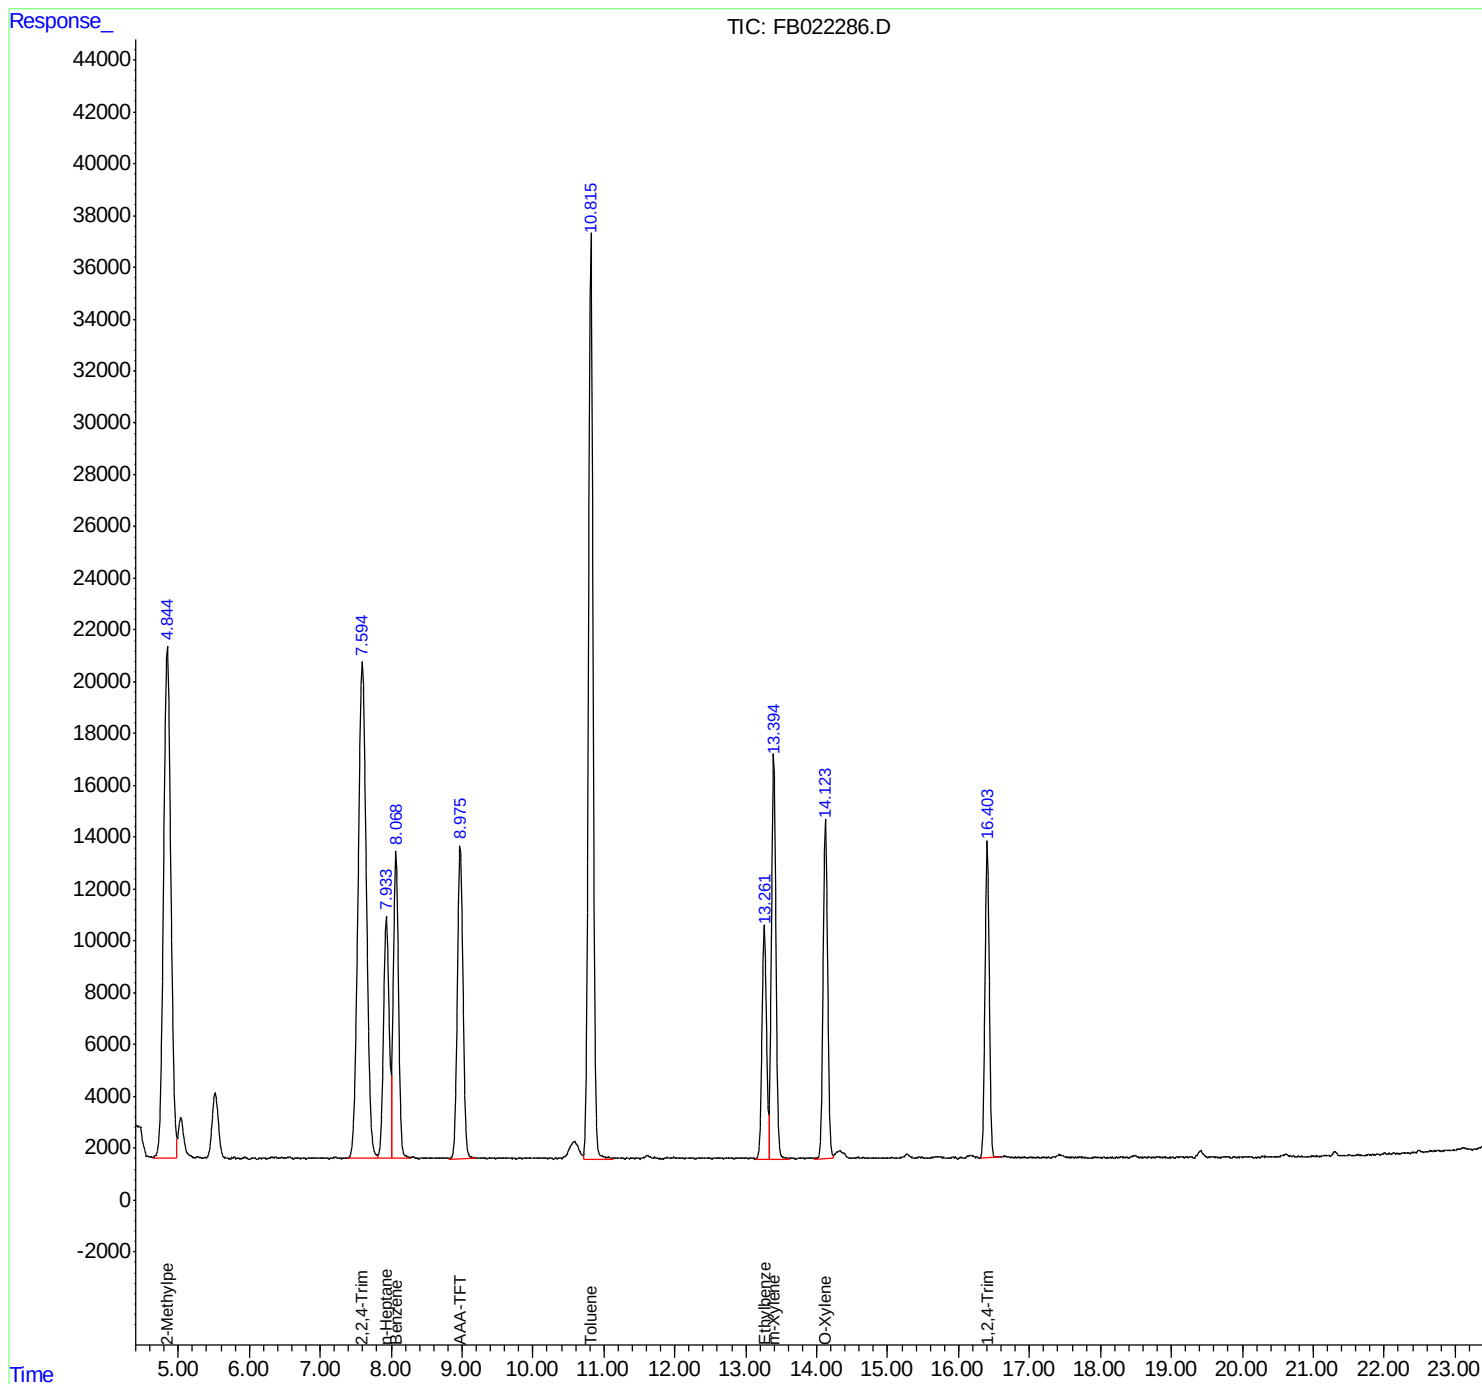


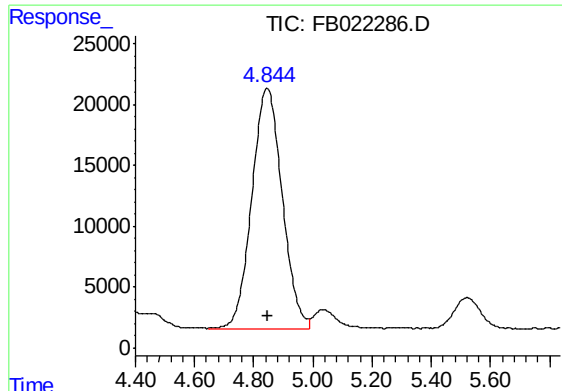

#1 2-Methylpentane


R.T.: 4.846 min
Delta R.T.: -0.001 min
Response: 1407955
Conc: 28.66 ng/ml

Instrument :
FID_B
ClientSampleId :
CLEARWELLMS

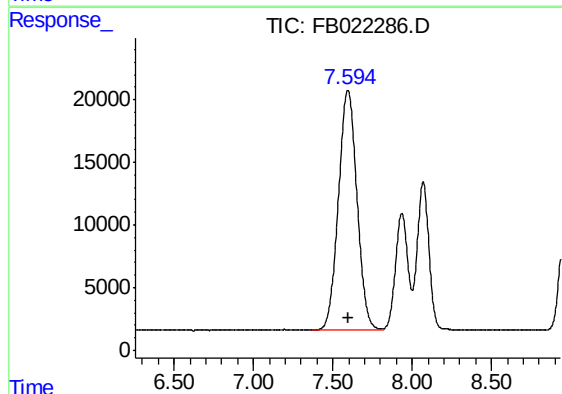


#2 2,2,4-Trimethylpentane

R.T.: 7.595 min
Delta R.T.: -0.003 min
Response: 1559622
Conc: 30.20 ng/ml

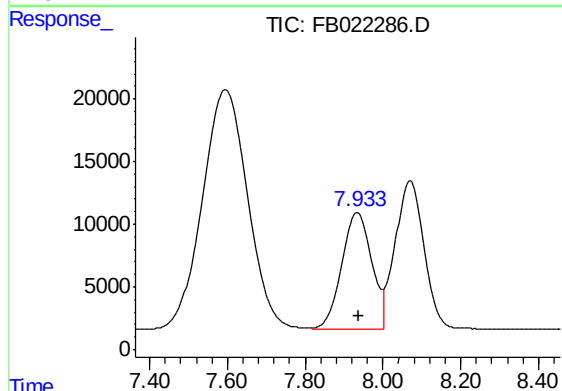


#3 n-Heptane

R.T.: 7.934 min
Delta R.T.: -0.003 min
Response: 502196
Conc: 9.98 ng/ml

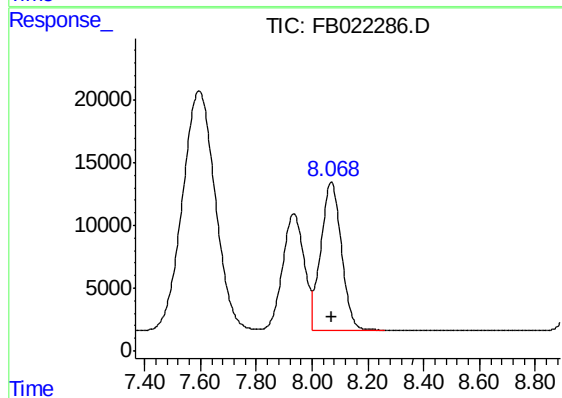

#4 Benzene


R.T.: 8.069 min
Delta R.T.: -0.003 min
Response: 609816
Conc: 10.28 ng/ml

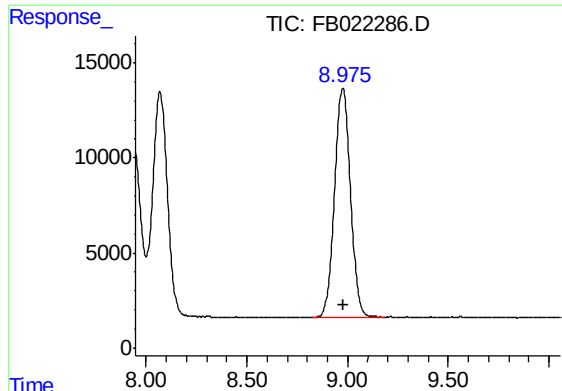

#5 AAA-TFT


R.T.: 8.976 min
Delta R.T.: -0.003 min
Response: 664248
Conc: 22.84 ng/ml

Instrument :
FID_B
ClientSampleId :
CLEARWELLMS

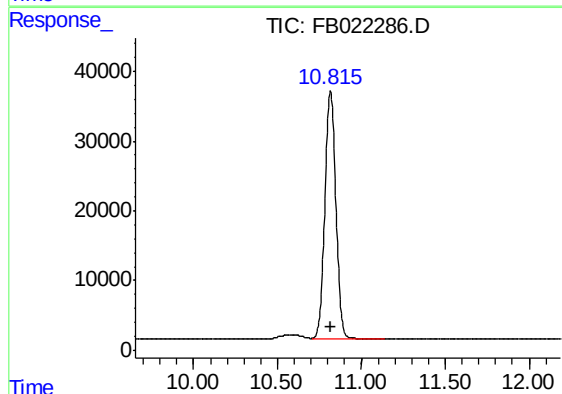


#6 Toluene

R.T.: 10.817 min
Delta R.T.: -0.003 min
Response: 1631800
Conc: 34.30 ng/ml

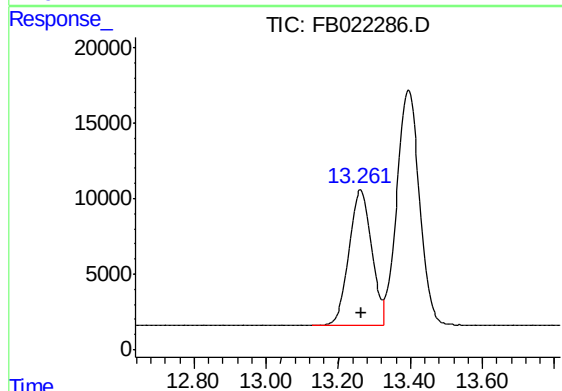


#7 Ethylbenzene

R.T.: 13.262 min
Delta R.T.: -0.003 min
Response: 392511
Conc: 13.09 ng/ml

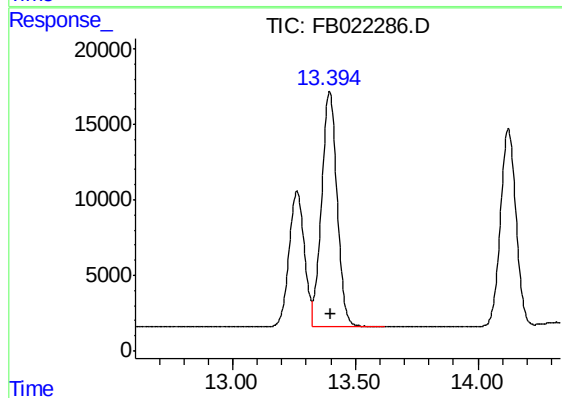

#8 m-Xylene


R.T.: 13.395 min
Delta R.T.: -0.003 min
Response: 687010
Conc: 25.86 ng/ml

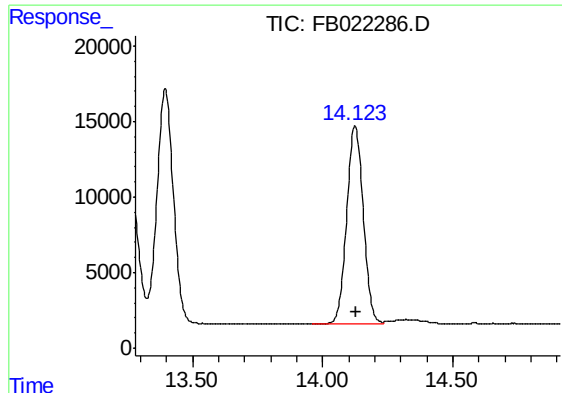

#9 O-Xylene

R.T.: 14.124 min
Delta R.T.: -0.004 min
Response: 580243
Conc: 23.92 ng/ml

Instrument :
FID_B
ClientSampleId :
CLEARWELLMS

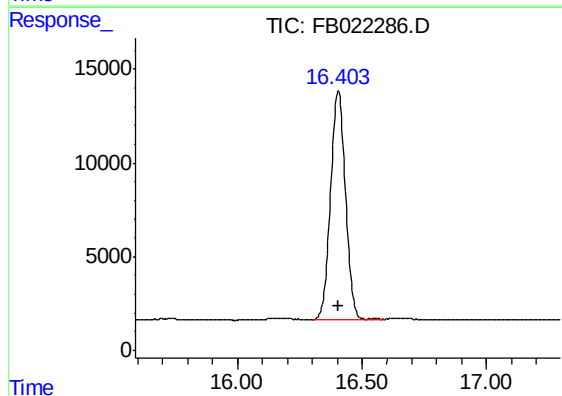

#10 1,2,4-Trimethylbenzene

R.T.: 16.405 min
Delta R.T.: -0.003 min
Response: 508297
Conc: 19.50 ng/ml