

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090419\
 Data File : FB022287.D
 Signal(s) : FID2B.CH
 Acq On : 4 Sep 2019 22:37
 Operator : DD/AJ
 Sample : K4688-02MSD
 Misc : 5.04G/5.00ML DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 CLEARWELLMSD

Integration File: Calibration.e
 Quant Time: Sep 05 01:21:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.974	647216	22.251 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.842	1420614	28.914 ng/ml
2) t 2,2,4-Trimethylpentane	7.592	1623516	31.440 ng/ml
3) t n-Heptane	7.932	523760	10.406 ng/ml
4) t Benzene	8.067	627485	10.573 ng/ml
6) t Toluene	10.815	1676006	35.230 ng/ml
7) t Ethylbenzene	13.261	410916	13.707 ng/ml
8) t m-Xylene	13.394	715999	26.951 ng/ml
9) t O-Xylene	14.124	614917	25.347 ng/ml
10) t 1,2,4-Trimethylbenzene	16.405	522493	20.041 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090419\
Data File : FB022287.D
Signal(s) : FID2B.CH
Acq On : 4 Sep 2019 22:37
Operator : DD/AJ
Sample : K4688-02MSD
Misc : 5.04G/5.00ML DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
CLEARWELLMSD

Integration File: Calibration.e
Quant Time: Sep 05 01:21:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

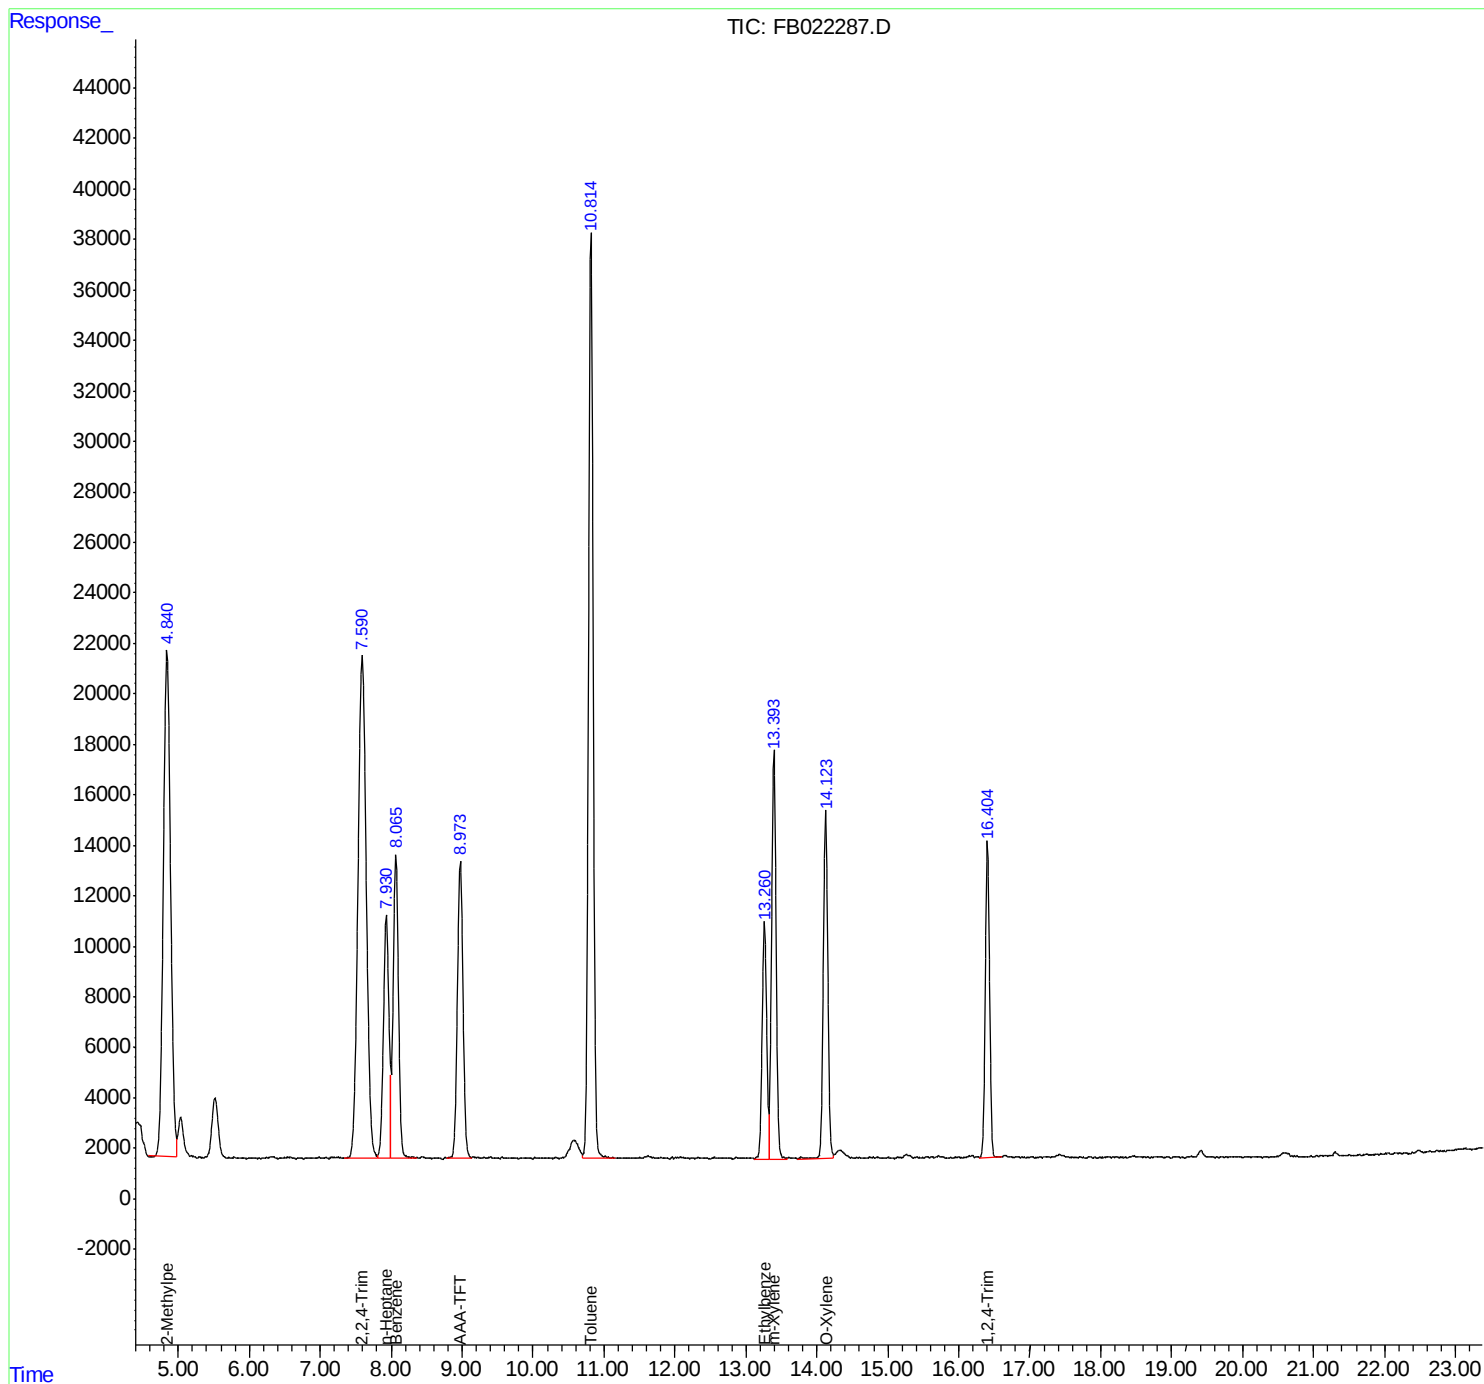


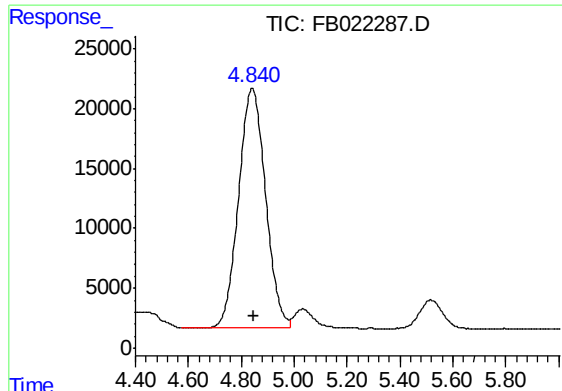

#1 2-Methylpentane


R.T.: 4.842 min
Delta R.T.: -0.005 min
Response: 1420614
Conc: 28.91 ng/ml

Instrument :
FID_B
ClientSampleId :
CLEARWELLMSD

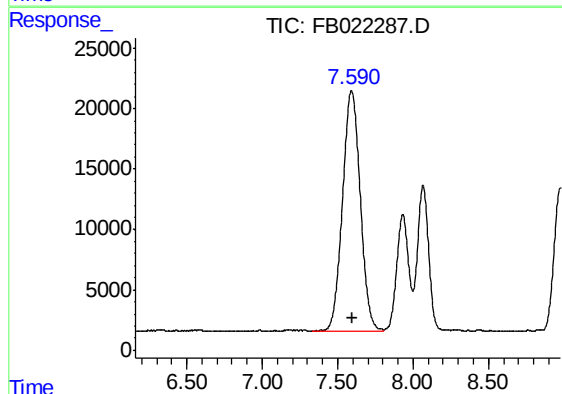


#2 2,2,4-Trimethylpentane

R.T.: 7.592 min
Delta R.T.: -0.005 min
Response: 1623516
Conc: 31.44 ng/ml

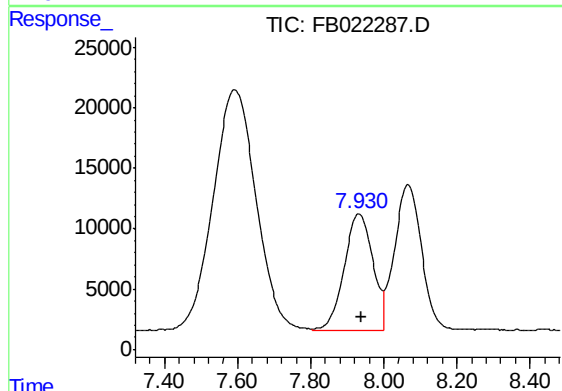


#3 n-Heptane

R.T.: 7.932 min
Delta R.T.: -0.005 min
Response: 523760
Conc: 10.41 ng/ml

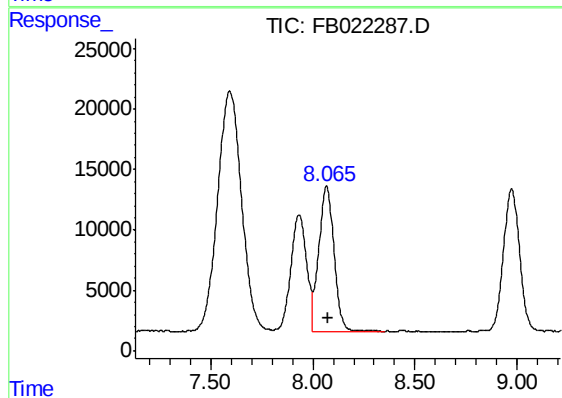

#4 Benzene


R.T.: 8.067 min
Delta R.T.: -0.005 min
Response: 627485
Conc: 10.57 ng/ml

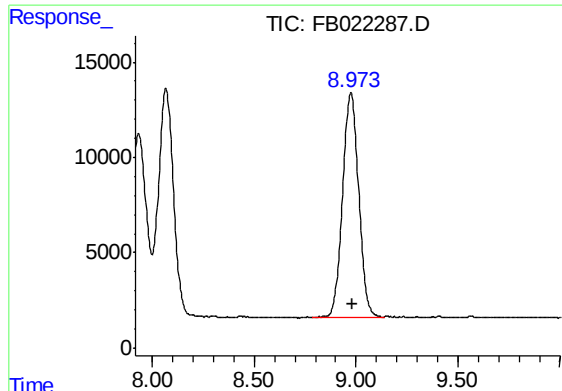

#5 AAA-TFT


R.T.: 8.974 min
Delta R.T.: -0.005 min
Response: 647216
Conc: 22.25 ng/ml

Instrument :
FID_B
ClientSampleId :
CLEARWELLMSD

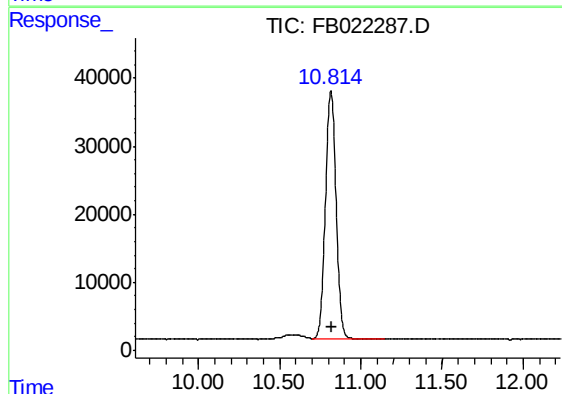


#6 Toluene

R.T.: 10.815 min
Delta R.T.: -0.004 min
Response: 1676006
Conc: 35.23 ng/ml

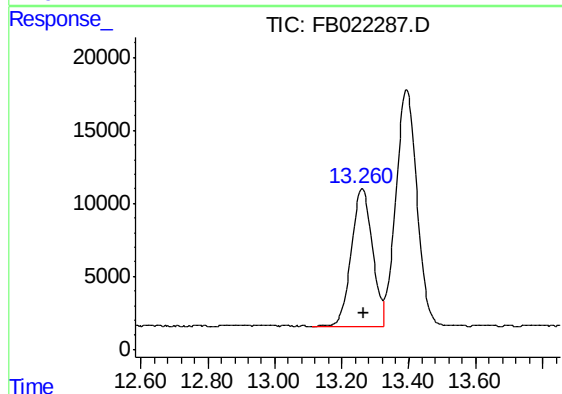


#7 Ethylbenzene

R.T.: 13.261 min
Delta R.T.: -0.004 min
Response: 410916
Conc: 13.71 ng/ml

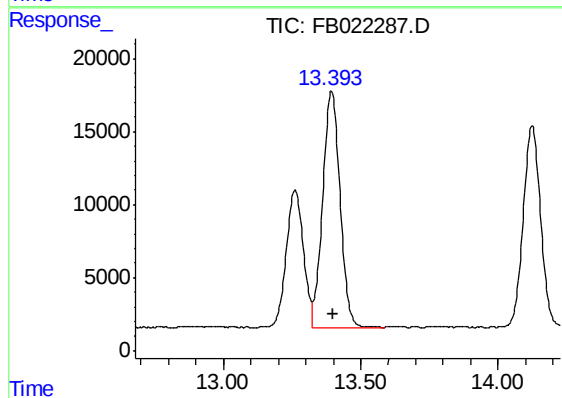

#8 m-Xylene


R.T.: 13.394 min
Delta R.T.: -0.004 min
Response: 715999
Conc: 26.95 ng/ml

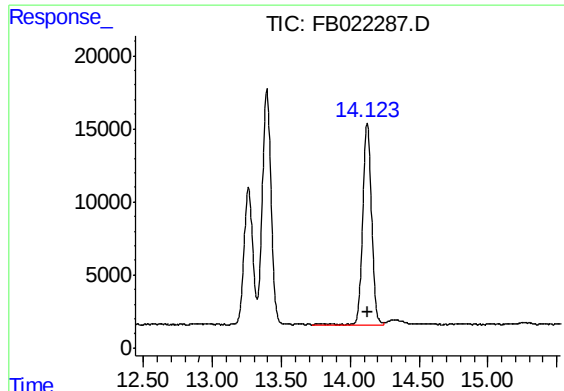

#9 O-Xylene

R.T.: 14.124 min
Delta R.T.: -0.004 min
Response: 614917
Conc: 25.35 ng/ml

Instrument :
FID_B
ClientSampleId :
CLEARWELLMSD

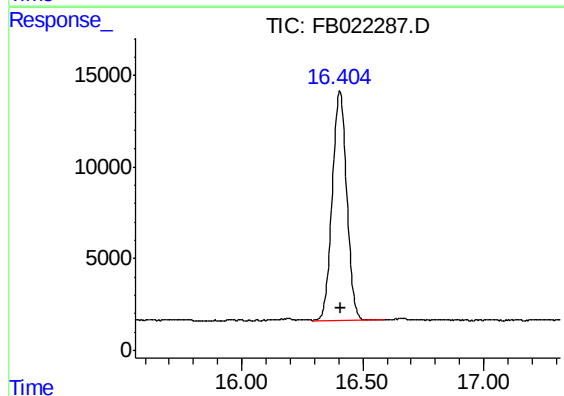

#10 1,2,4-Trimethylbenzene

R.T.: 16.405 min
Delta R.T.: -0.002 min
Response: 522493
Conc: 20.04 ng/ml