

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090518\
 Data File : FB017613.D
 Signal(s) : FID2B.CH
 Acq On : 5 Sep 2018 9:40
 Operator : MJ/SJ
 Sample : BSF0905S1
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 05 13:35:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
 Quant Title :
 QLast Update : Mon Aug 20 13:42:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.111	183585	22.267 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.964	348358	24.861 ng/ml
2) t	2,2,4-Trimethylpentane	7.728	411161	29.177 ng/ml
3) t	n-Heptane	8.067	109234	7.926 ng/ml
4) t	Benzene	8.206	181739	10.308 ng/ml
6) t	Toluene	10.960	448152	31.152 ng/ml
7) t	Ethylbenzene	13.409	156372	10.603 ng/ml
8) t	m-Xylene	13.542	332400	21.383 ng/ml
9) t	O-Xylene	14.274	354232	21.579 ng/ml
10) t	1,2,4-Trimethylbenzene	16.556	423706	21.755 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090518\
Data File : FB017613.D
Signal(s) : FID2B.CH
Acq On : 5 Sep 2018 9:40
Operator : MJ/SJ
Sample : BSF0905S1
Misc : 5.02g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 05 13:35:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

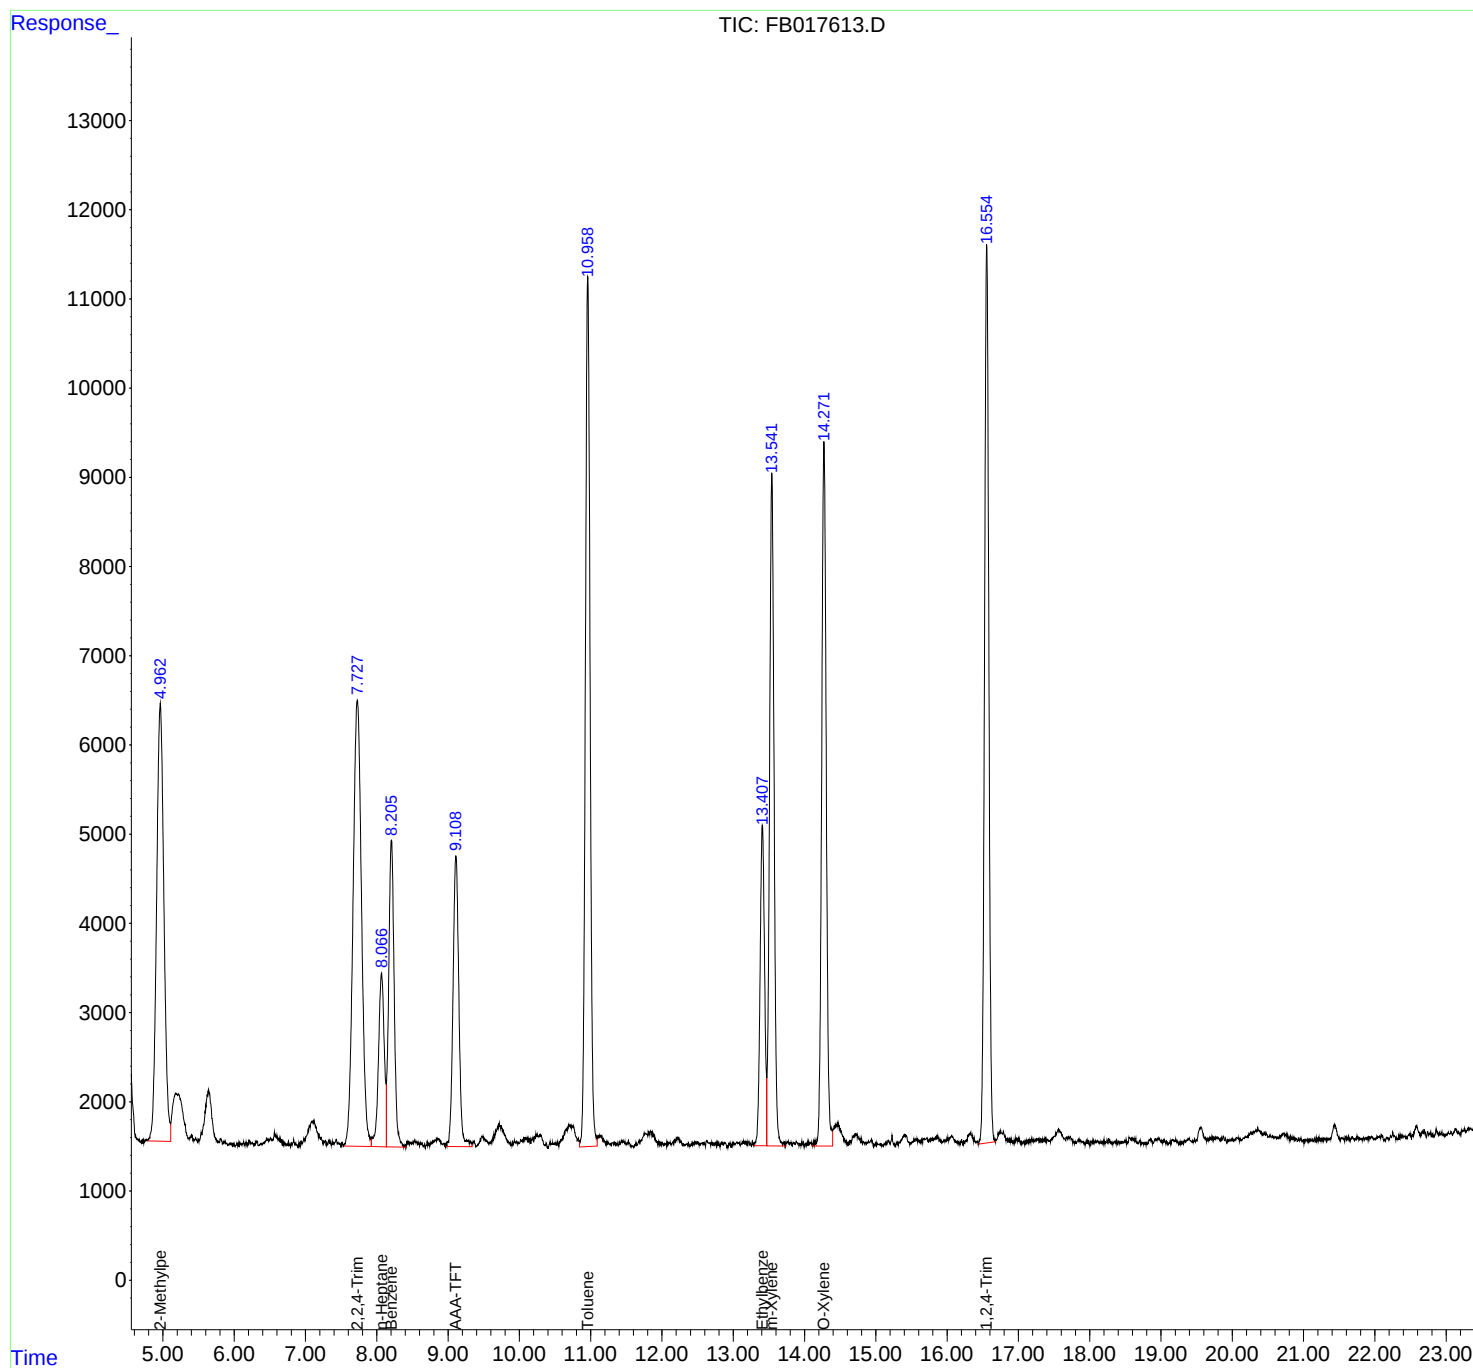

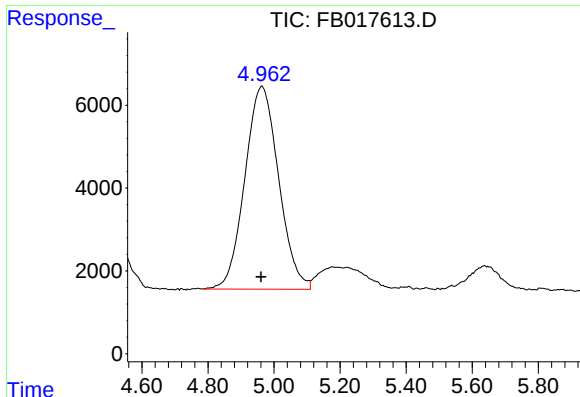


#1 2-Methylpentane

R.T.: 4.964 min
Delta R.T.: 0.003 min
Response: 348358
Conc: 24.86 ng/ml

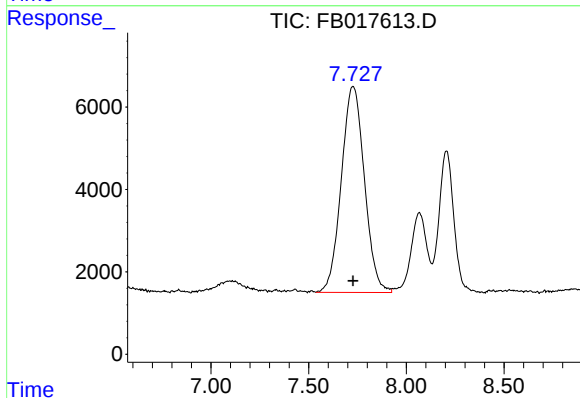


#2 2,2,4-Trimethylpentane

R.T.: 7.728 min
Delta R.T.: 0.000 min
Response: 411161
Conc: 29.18 ng/ml

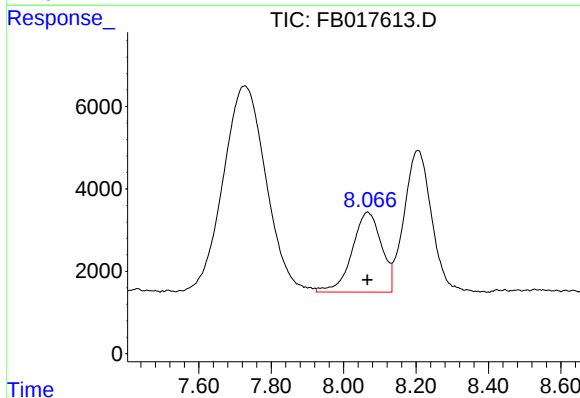


#3 n-Heptane

R.T.: 8.067 min
Delta R.T.: 0.000 min
Response: 109234
Conc: 7.93 ng/ml

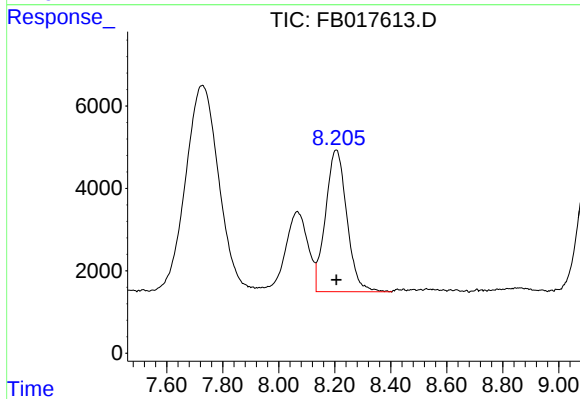


#4 Benzene

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 181739
Conc: 10.31 ng/ml

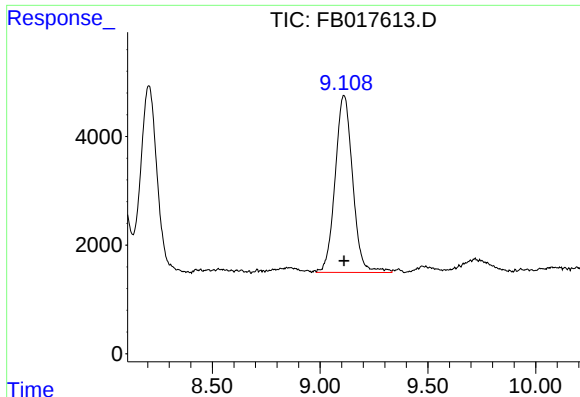


#5 AAA-TFT

R.T.: 9.111 min
Delta R.T.: 0.000 min
Response: 183585
Conc: 22.27 ng/ml

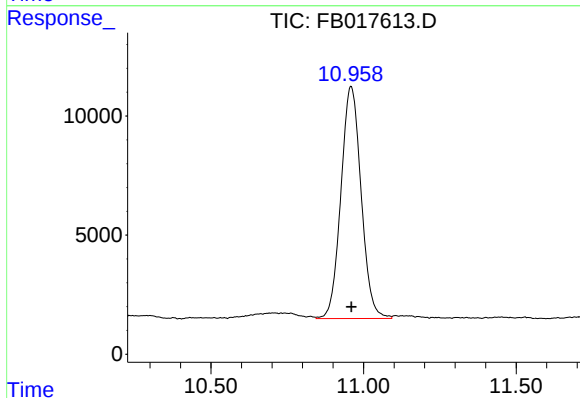


#6 Toluene

R.T.: 10.960 min
Delta R.T.: 0.000 min
Response: 448152
Conc: 31.15 ng/ml

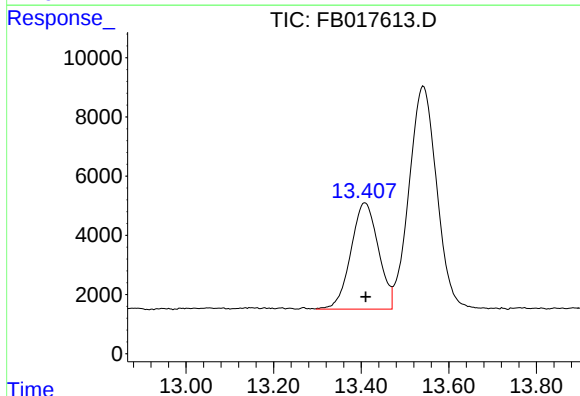


#7 Ethylbenzene

R.T.: 13.409 min
Delta R.T.: -0.002 min
Response: 156372
Conc: 10.60 ng/ml

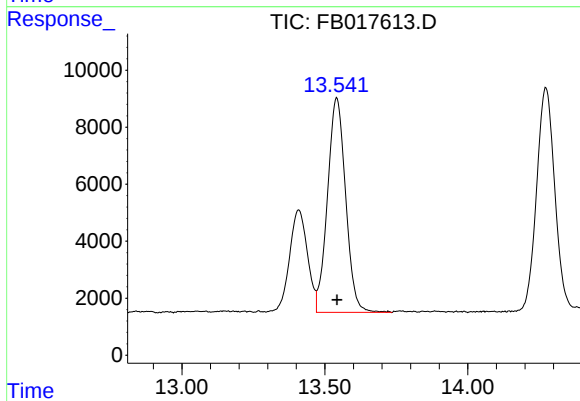


#8 m-Xylene

R.T.: 13.542 min
Delta R.T.: 0.000 min
Response: 332400
Conc: 21.38 ng/ml

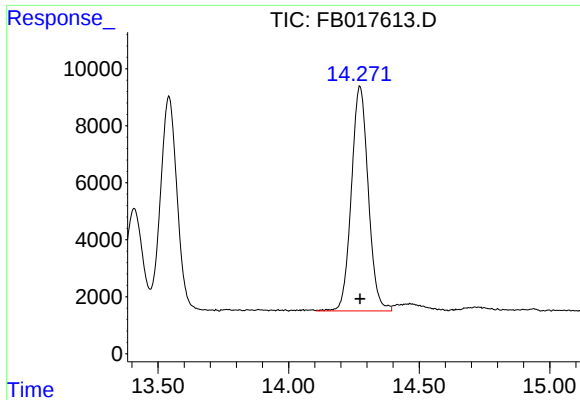

#9 O-Xylene

R.T.: 14.274 min
Delta R.T.: 0.000 min
Response: 354232
Conc: 21.58 ng/ml

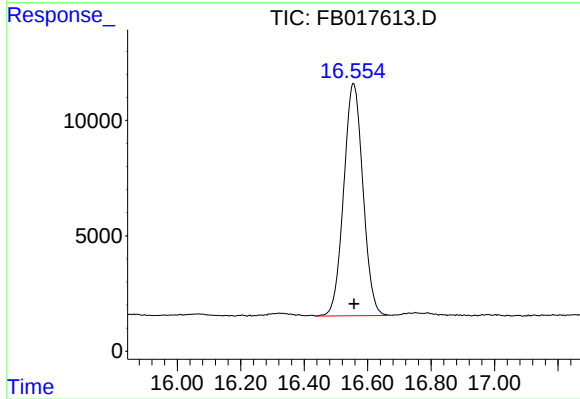

#10 1,2,4-Trimethylbenzene

R.T.: 16.556 min
Delta R.T.: -0.001 min
Response: 423706
Conc: 21.75 ng/ml