

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090518\
 Data File : FB017615.D
 Signal(s) : FID2B.CH
 Acq On : 5 Sep 2018 10:41
 Operator : MJ/SJ
 Sample : J4781-01MS
 Misc : 5.03g/5.00mL DI Water
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Sep 05 13:36:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
 Quant Title :
 QLast Update : Mon Aug 20 13:42:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.110	180102	21.844 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.962	292463	20.872 ng/ml
2) t 2,2,4-Trimethylpentane	7.727	302380	21.458 ng/ml
3) t n-Heptane	8.066	76023	5.516 ng/ml
4) t Benzene	8.205	179800	10.198 ng/ml
6) t Toluene	10.959	434609	30.211 ng/ml
7) t Ethylbenzene	13.408	144764	9.816 ng/ml
8) t m-Xylene	13.541	300945	19.359 ng/ml
9) t O-Xylene	14.273	318950	19.430 ng/ml
10) t 1,2,4-Trimethylbenzene	16.556	350856	18.014 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090518\
Data File : FB017615.D
Signal(s) : FID2B.CH
Acq On : 5 Sep 2018 10:41
Operator : MJ/SJ
Sample : J4781-01MS
Misc : 5.03g/5.00mL DI Water
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Sep 05 13:36:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

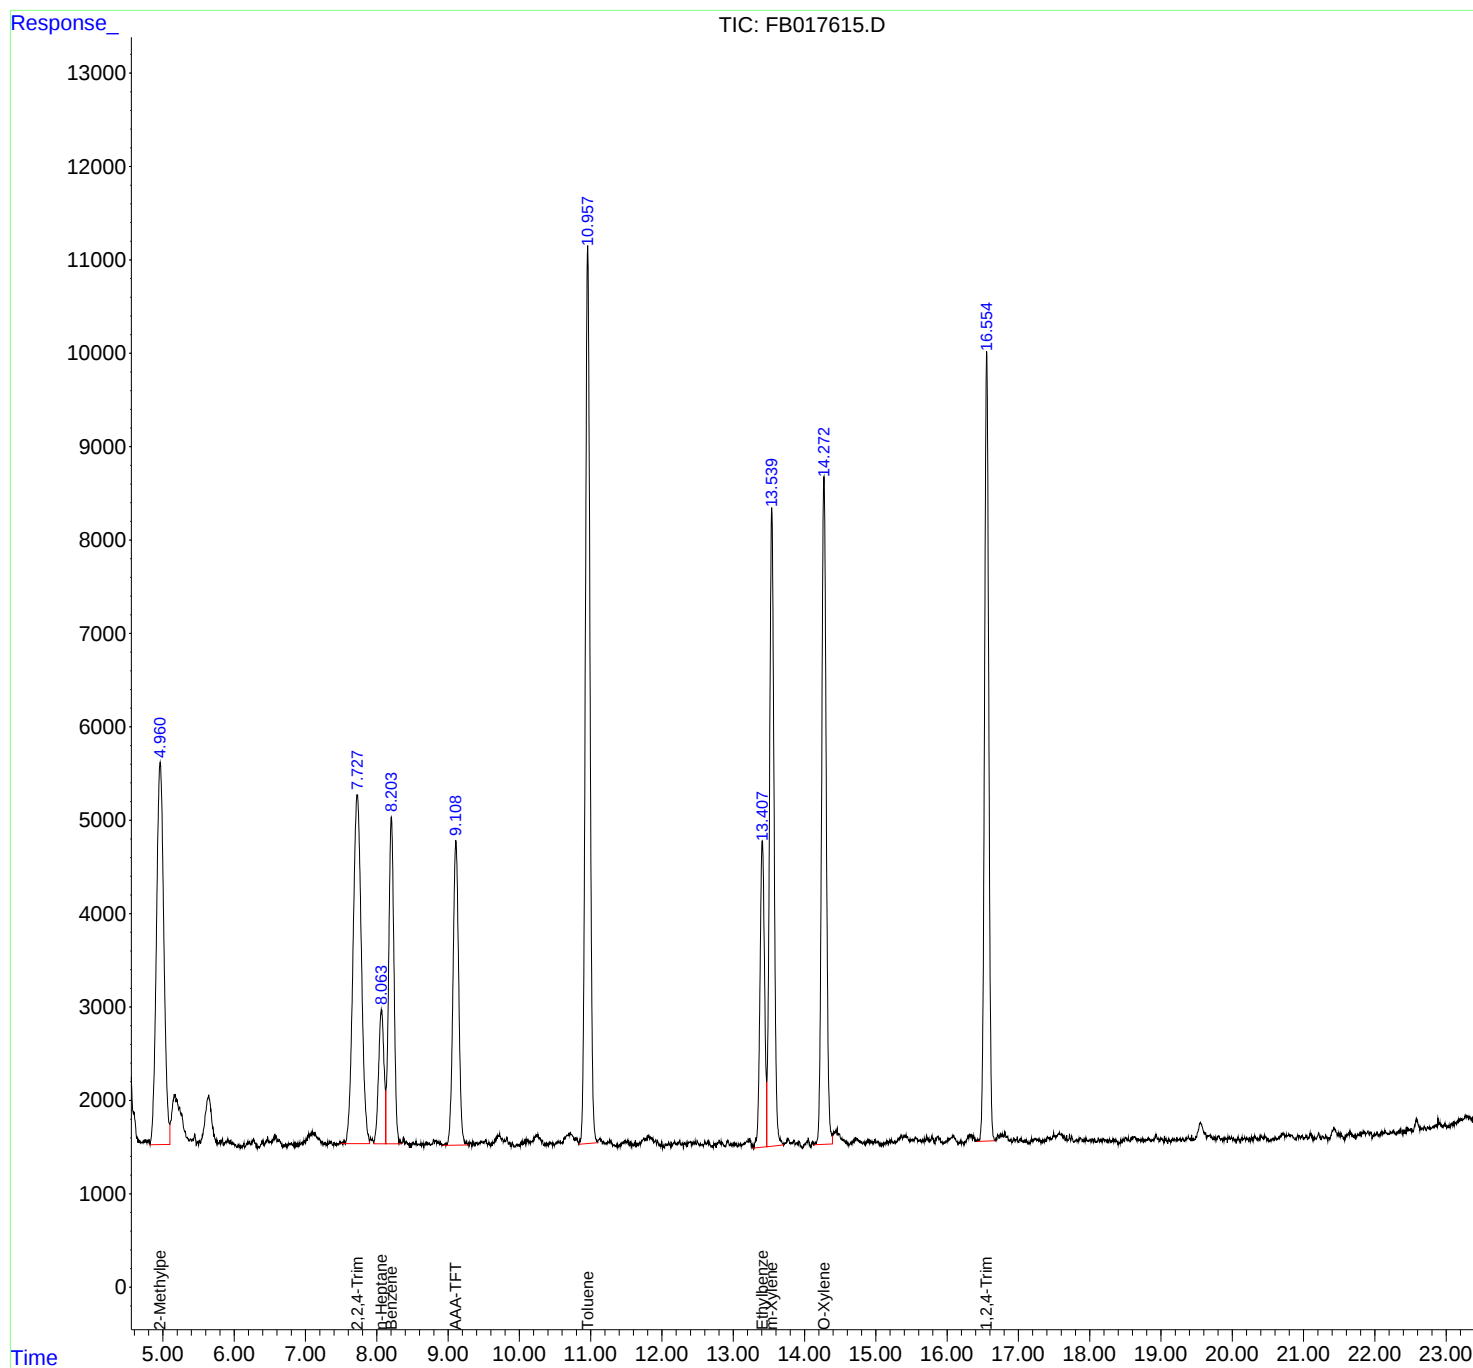

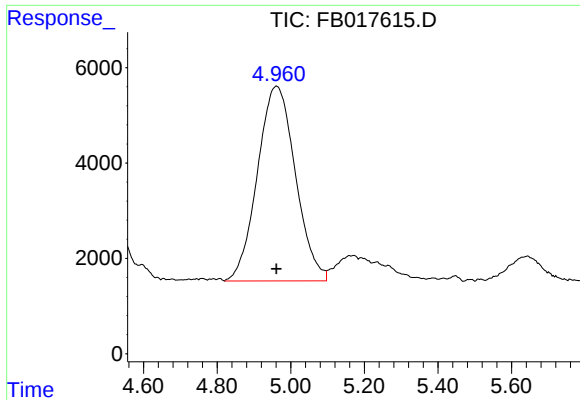


#1 2-Methylpentane

R.T.: 4.962 min
Delta R.T.: 0.001 min
Response: 292463
Conc: 20.87 ng/ml

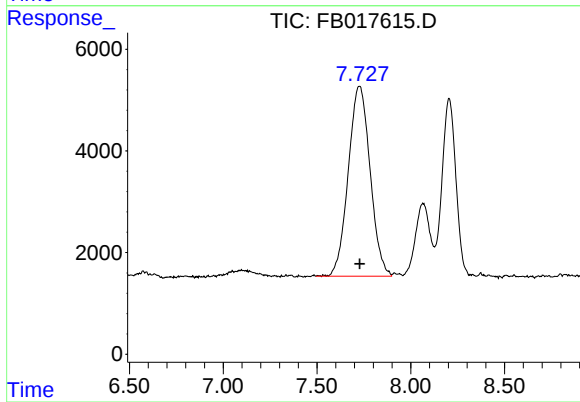


#2 2,2,4-Trimethylpentane

R.T.: 7.727 min
Delta R.T.: 0.000 min
Response: 302380
Conc: 21.46 ng/ml

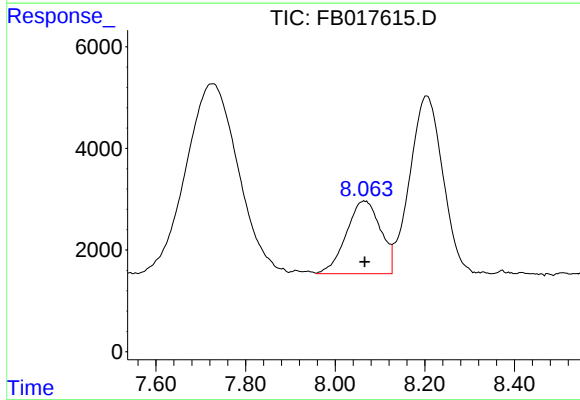


#3 n-Heptane

R.T.: 8.066 min
Delta R.T.: 0.000 min
Response: 76023
Conc: 5.52 ng/ml

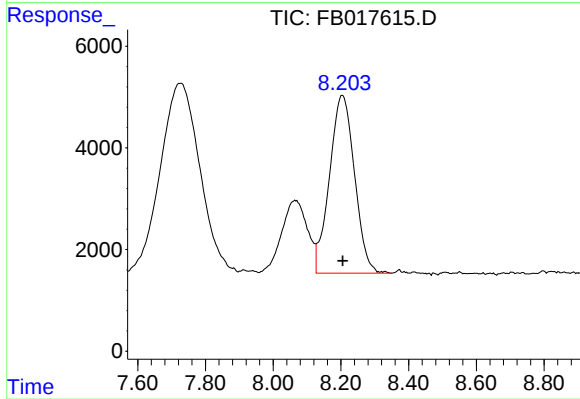


#4 Benzene

R.T.: 8.205 min
Delta R.T.: 0.000 min
Response: 179800
Conc: 10.20 ng/ml

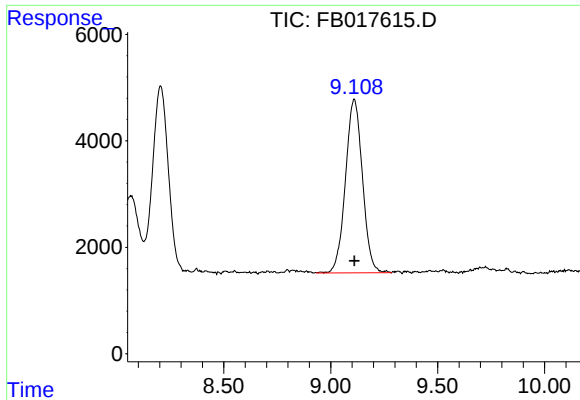


#5 AAA-TFT

R.T.: 9.110 min
 Delta R.T.: 0.000 min
 Response: 180102
 Conc: 21.84 ng/ml

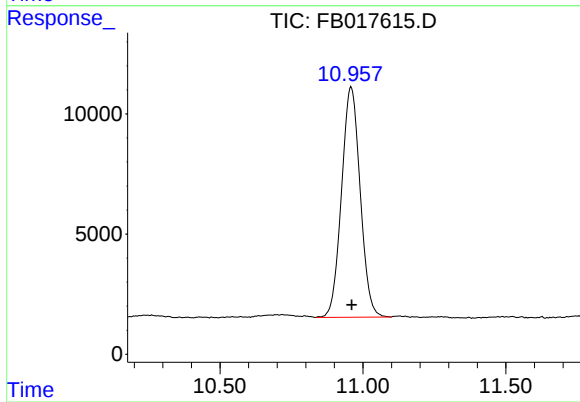


#6 Toluene

R.T.: 10.959 min
 Delta R.T.: -0.002 min
 Response: 434609
 Conc: 30.21 ng/ml

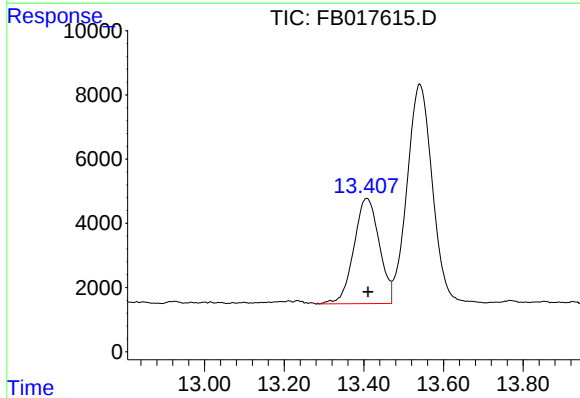


#7 Ethylbenzene

R.T.: 13.408 min
 Delta R.T.: -0.003 min
 Response: 144764
 Conc: 9.82 ng/ml

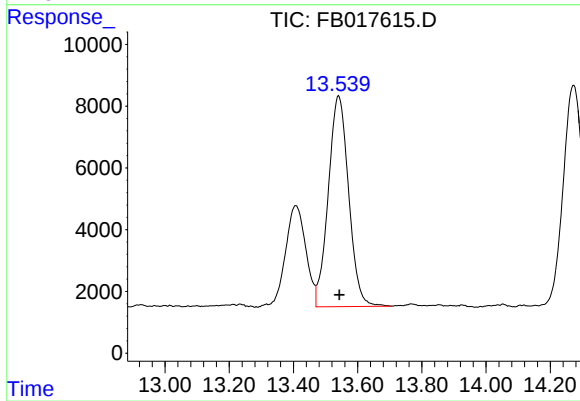


#8 m-Xylene

R.T.: 13.541 min
 Delta R.T.: -0.002 min
 Response: 300945
 Conc: 19.36 ng/ml

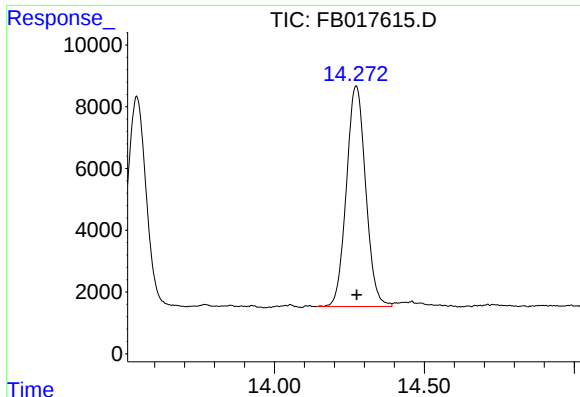

#9 O-Xylene

R.T.: 14.273 min
Delta R.T.: -0.001 min
Response: 318950
Conc: 19.43 ng/ml

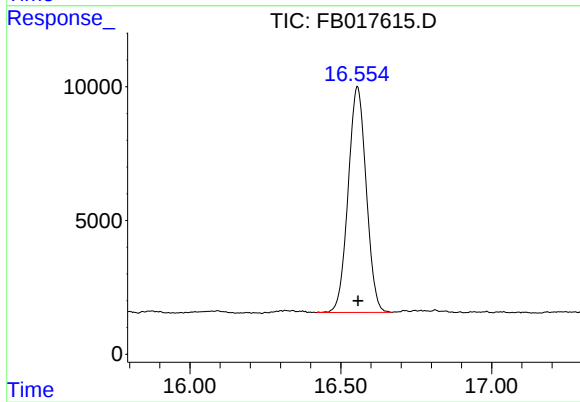

#10 1,2,4-Trimethylbenzene

R.T.: 16.556 min
Delta R.T.: -0.002 min
Response: 350856
Conc: 18.01 ng/ml