

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090519\
Data File : FB022298.D
Signal(s) : FID2B.CH
Acq On : 5 Sep 2019 13:40
Operator : DD/AJ
Sample : K4696-02
Misc : 5.04g/5.00ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 06 00:46:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.966	707427	24.321 ng/ml
Target Compounds			
6) t Toluene	10.808	11532	0.242 ng/ml
9) t O-Xylene	14.114	5585	0.230 ng/ml
10) t 1,2,4-Trimethylbenzene	16.395	10217	0.392 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090519\
Data File : FB022298.D
Signal(s) : FID2B.CH
Acq On : 5 Sep 2019 13:40
Operator : DD/AJ
Sample : K4696-02
Misc : 5.04g/5.00ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 06 00:46:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

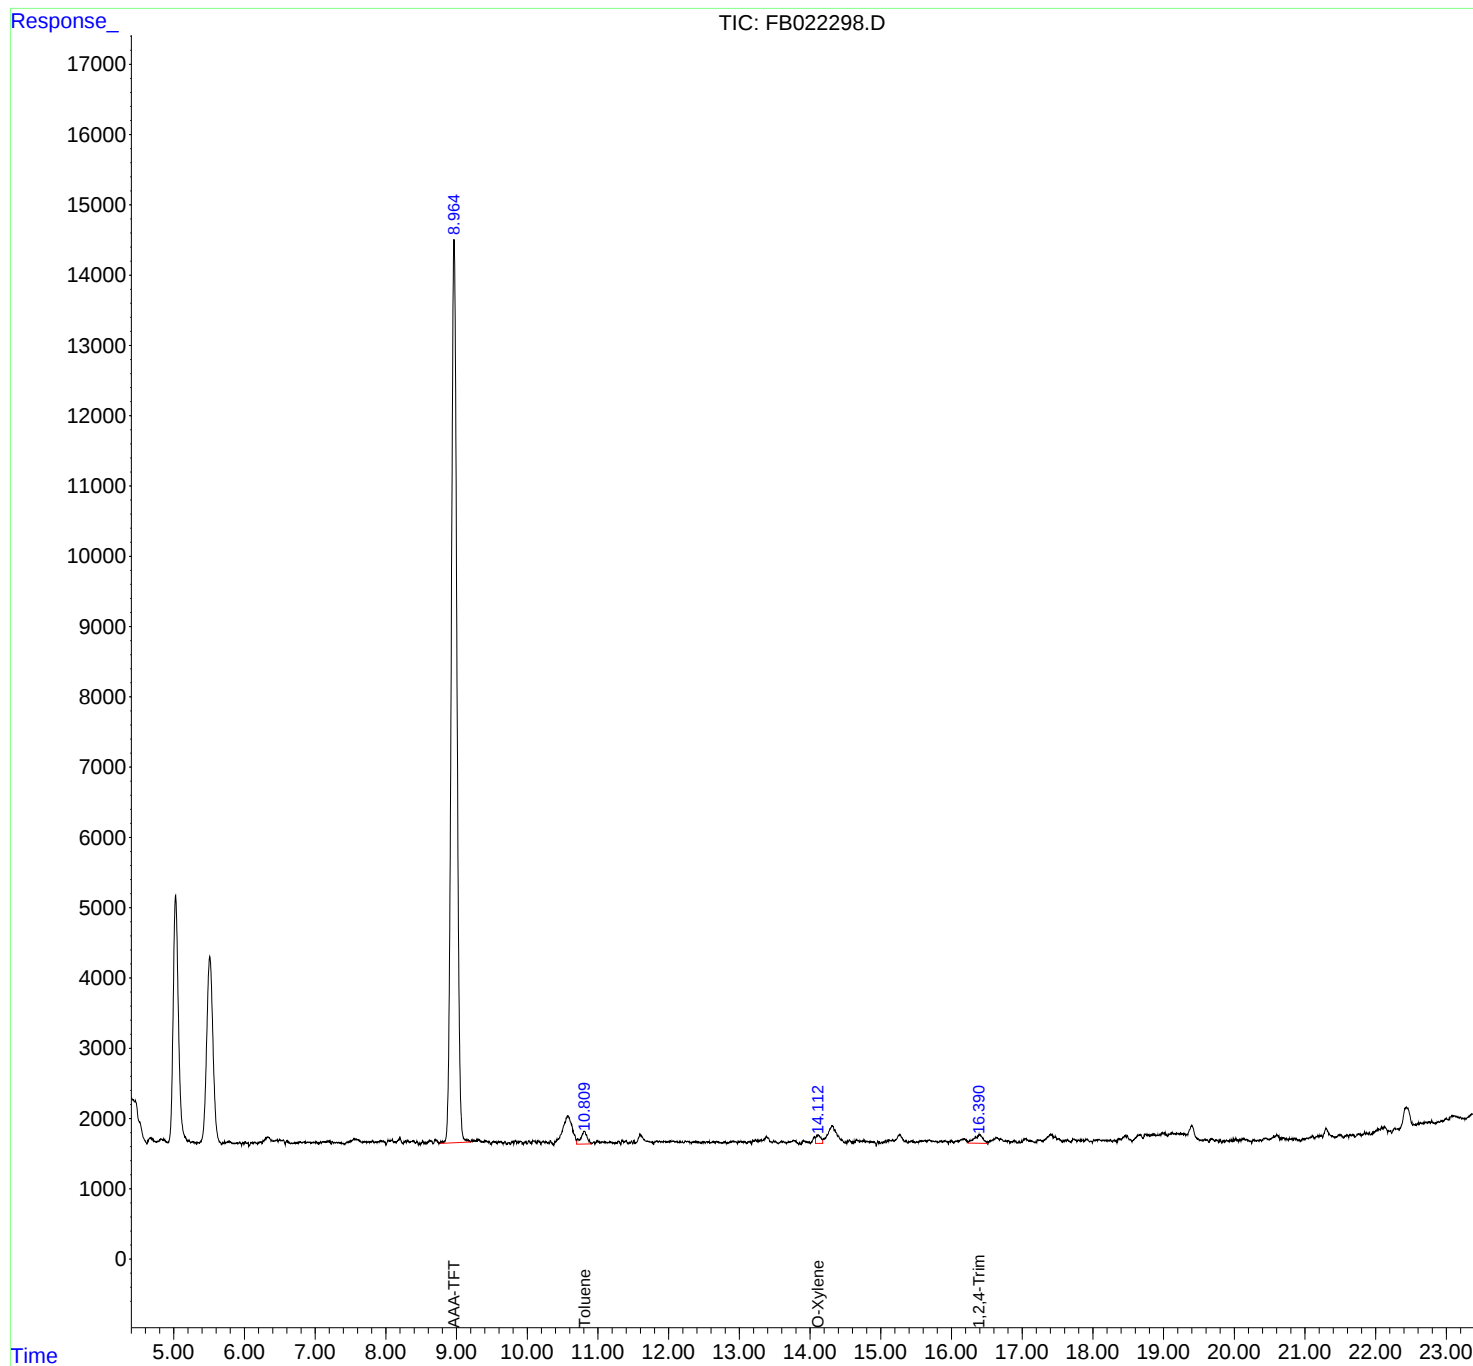


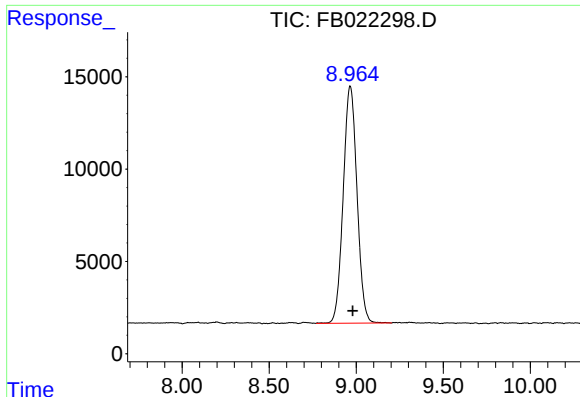

#5 AAA-TFT


R.T.: 8.966 min
Delta R.T.: -0.013 min
Response: 707427
Conc: 24.32 ng/ml

Instrument :
FID_B
ClientSampleId :

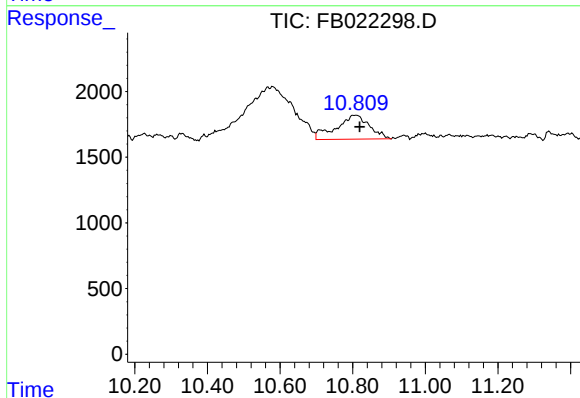


#6 Toluene

R.T.: 10.808 min
Delta R.T.: -0.012 min
Response: 11532
Conc: 0.24 ng/ml

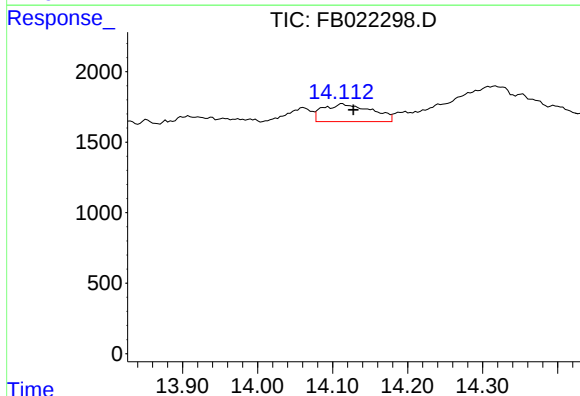

#9 O-Xylene

R.T.: 14.114 min
Delta R.T.: -0.014 min
Response: 5585
Conc: 0.23 ng/ml

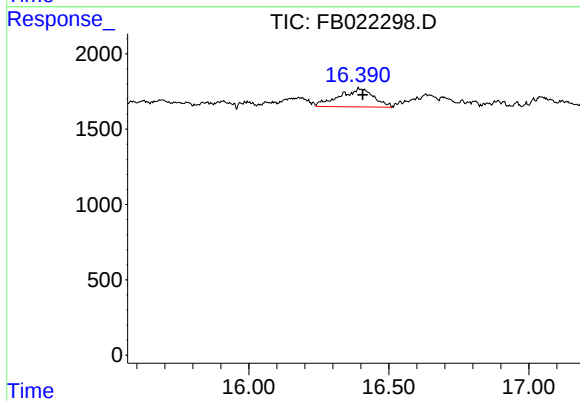

#10 1,2,4-Trimethylbenzene

R.T.: 16.395 min
Delta R.T.: -0.013 min
Response: 10217
Conc: 0.39 ng/ml