

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090519\
 Data File : FB022302.D
 Signal(s) : FID2B.CH
 Acq On : 5 Sep 2019 15:41
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 2.15g/5.00ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 06 00:47:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.972	591054	20.320 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.839	1278145	26.014 ng/ml
2) t 2,2,4-Trimethylpentane	7.590	1421595	27.530 ng/ml
3) t n-Heptane	7.930	463526	9.210 ng/ml
4) t Benzene	8.065	573519	9.663 ng/ml
6) t Toluene	10.813	1615684	33.962 ng/ml
7) t Ethylbenzene	13.259	459973	15.343 ng/ml
8) t m-Xylene	13.392	871842	32.818 ng/ml
9) t O-Xylene	14.122	774057	31.907 ng/ml
10) t 1,2,4-Trimethylbenzene	16.403	511883	19.634 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090519\
Data File : FB022302.D
Signal(s) : FID2B.CH
Acq On : 5 Sep 2019 15:41
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 2.15g/5.00ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 06 00:47:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

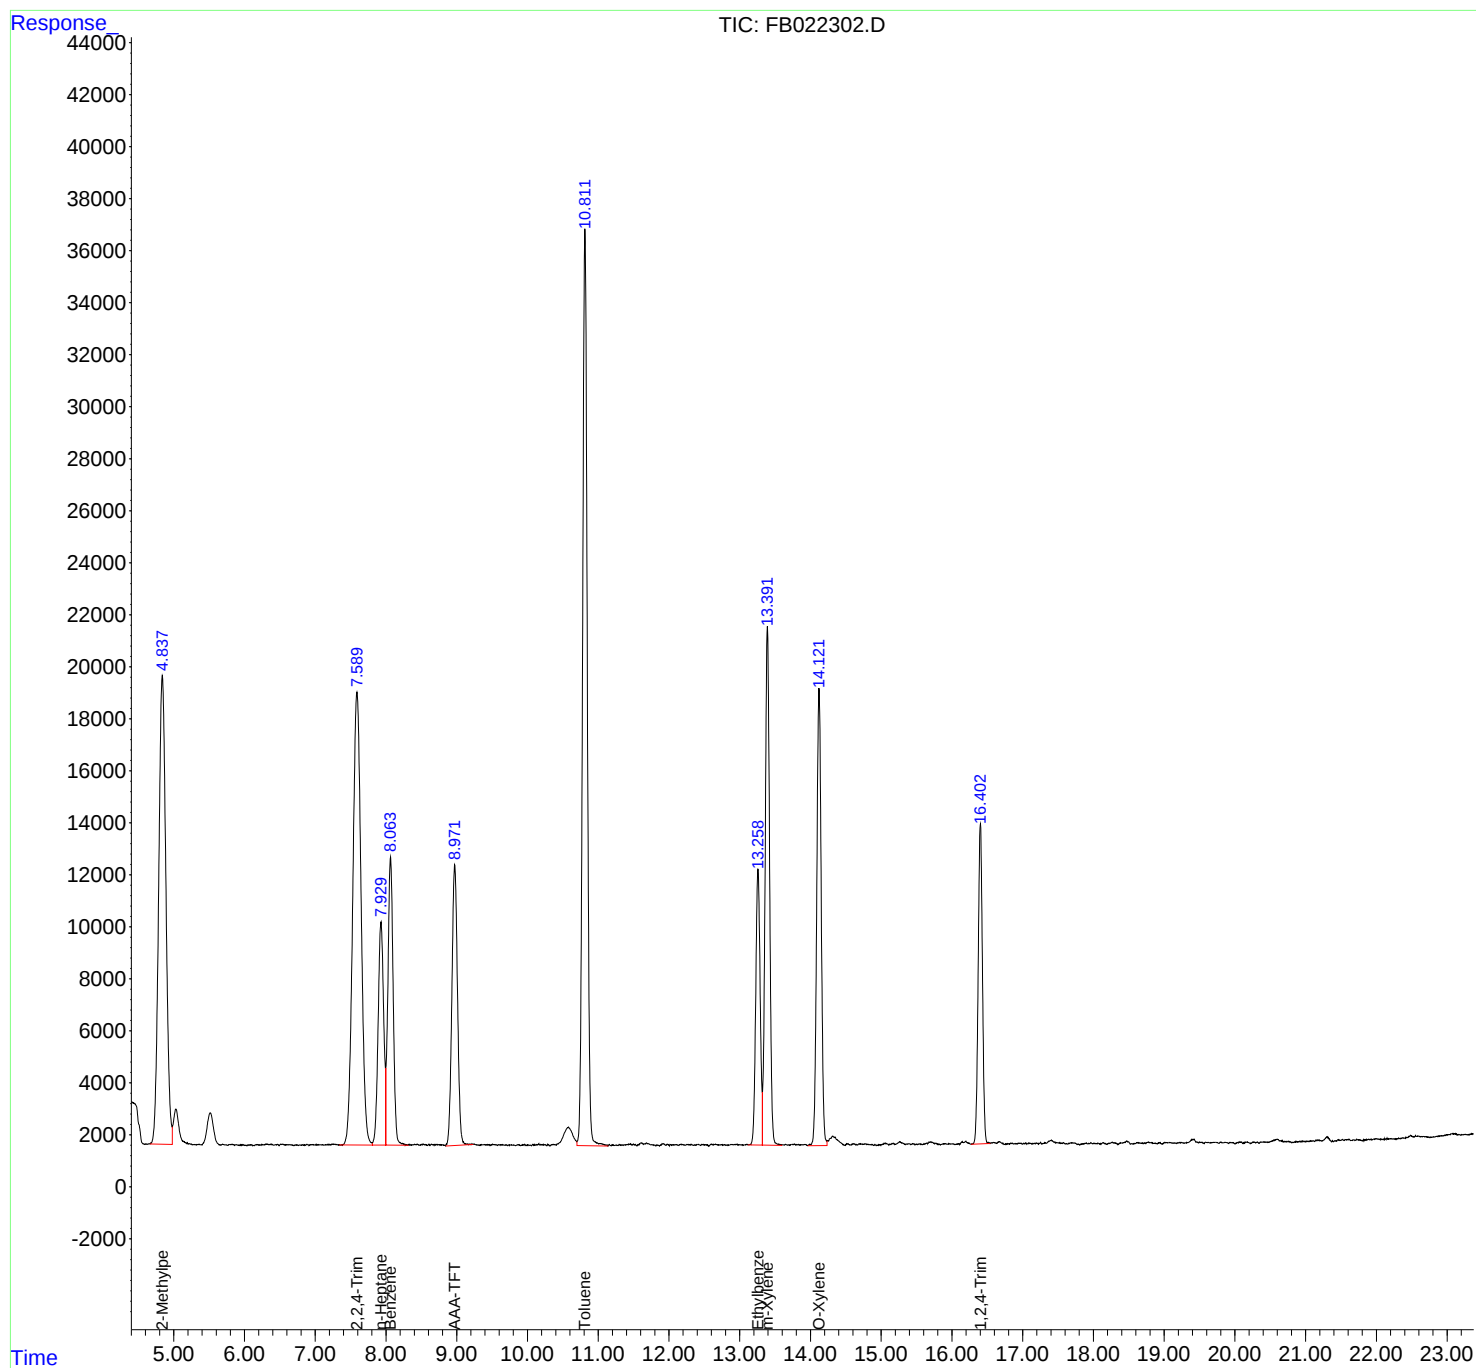


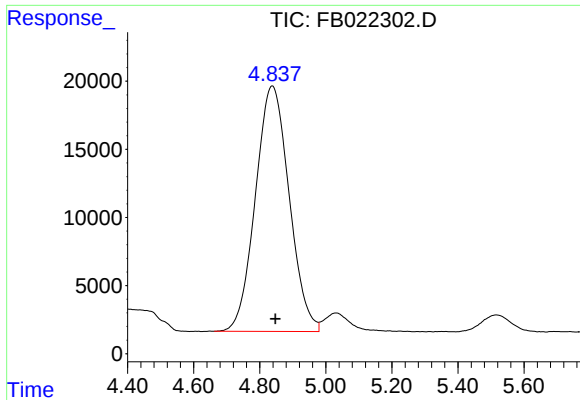

#1 2-Methylpentane


R.T.: 4.839 min
Delta R.T.: -0.008 min
Response: 1278145
Conc: 26.01 ng/ml

Instrument :
FID_B
ClientSampleId :

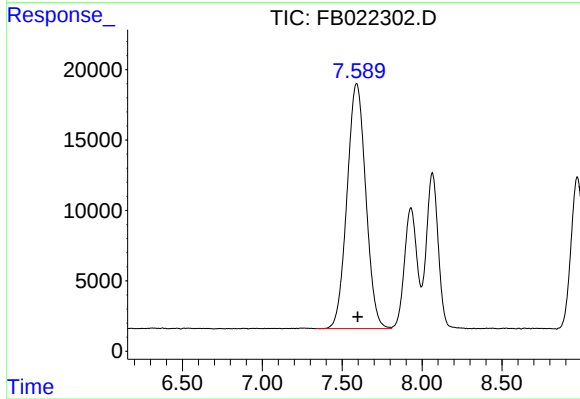


#2 2,2,4-Trimethylpentane

R.T.: 7.590 min
Delta R.T.: -0.007 min
Response: 1421595
Conc: 27.53 ng/ml

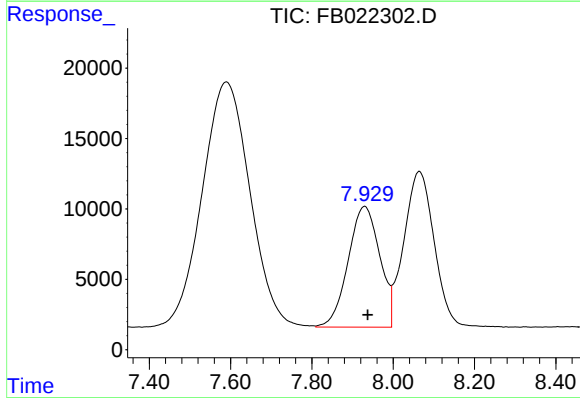


#3 n-Heptane

R.T.: 7.930 min
Delta R.T.: -0.008 min
Response: 463526
Conc: 9.21 ng/ml

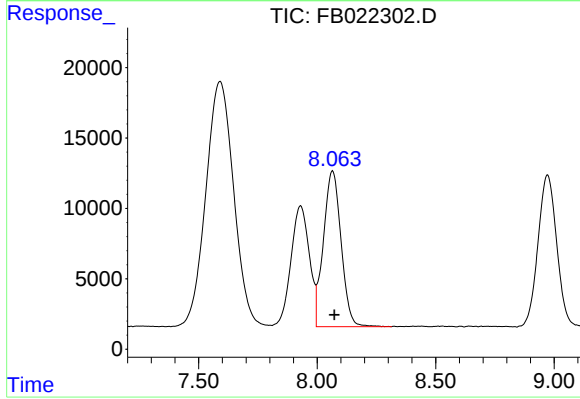

#4 Benzene


R.T.: 8.065 min
Delta R.T.: -0.008 min
Response: 573519
Conc: 9.66 ng/ml

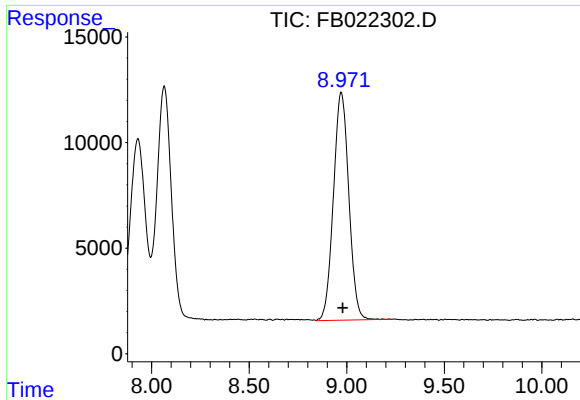

#5 AAA-TFT


R.T.: 8.972 min
Delta R.T.: -0.007 min
Response: 591054
Conc: 20.32 ng/ml

Instrument :
FID_B
ClientSampleId :

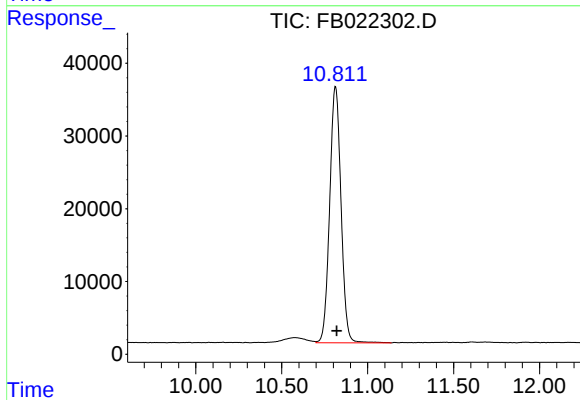


#6 Toluene

R.T.: 10.813 min
Delta R.T.: -0.007 min
Response: 1615684
Conc: 33.96 ng/ml

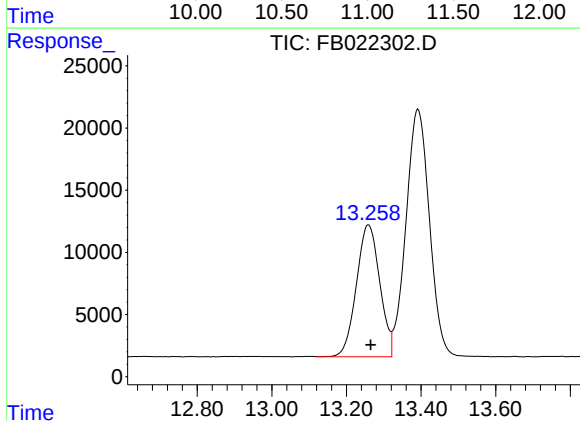


#7 Ethylbenzene

R.T.: 13.259 min
Delta R.T.: -0.006 min
Response: 459973
Conc: 15.34 ng/ml

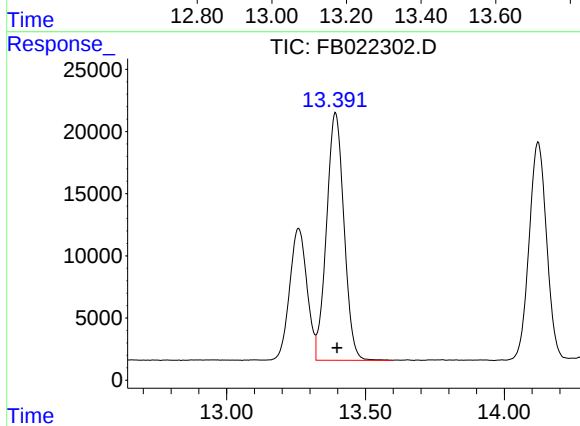

#8 m-Xylene


R.T.: 13.392 min
Delta R.T.: -0.006 min
Response: 871842
Conc: 32.82 ng/ml

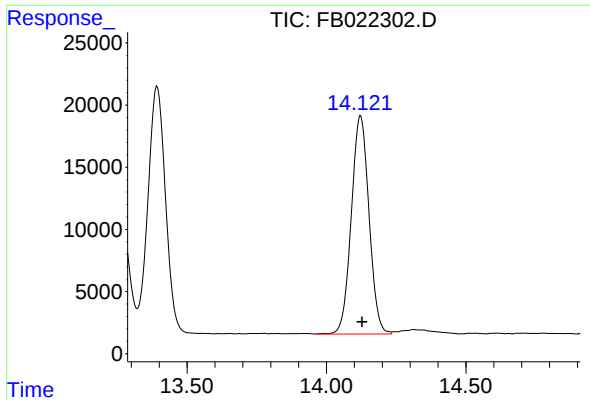

#9 O-Xylene

R.T.: 14.122 min
Delta R.T.: -0.006 min
Response: 774057
Conc: 31.91 ng/ml

Instrument :
FID_B
ClientSampleId :

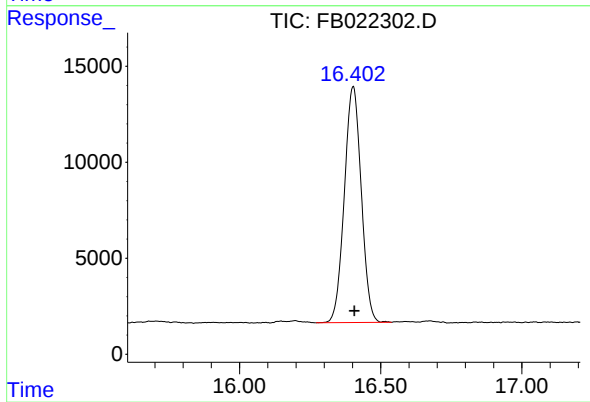

#10 1,2,4-Trimethylbenzene

R.T.: 16.403 min
Delta R.T.: -0.004 min
Response: 511883
Conc: 19.63 ng/ml