

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090519\
Data File : FB022311.D
Signal(s) : FID2B.CH
Acq On : 5 Sep 2019 20:14
Operator : DD/AJ
Sample : K4692-08
Misc : 5.05g/5.00ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 06 00:49:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.972	607611	20.889 ng/ml
Target Compounds			
6) t Toluene	10.820	4466	0.094 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090519\
Data File : FB022311.D
Signal(s) : FID2B.CH
Acq On : 5 Sep 2019 20:14
Operator : DD/AJ
Sample : K4692-08
Misc : 5.05g/5.00ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 06 00:49:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

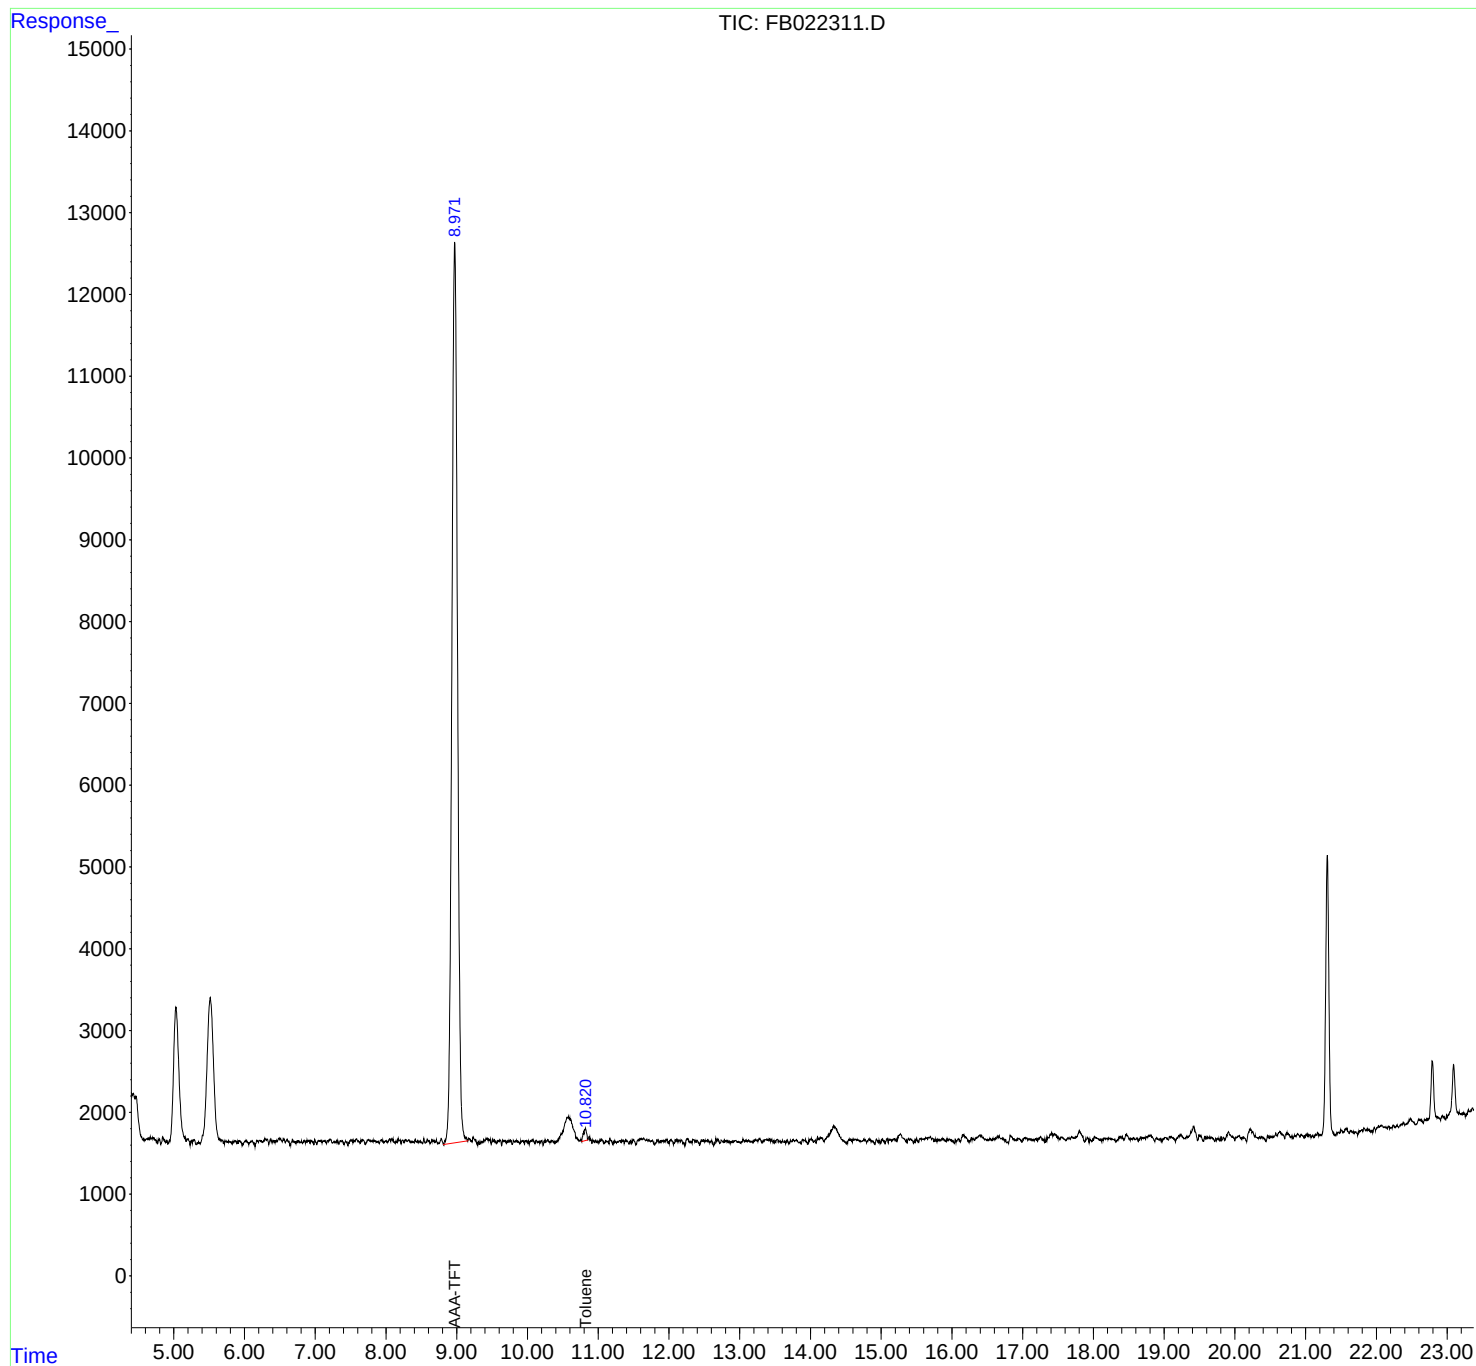


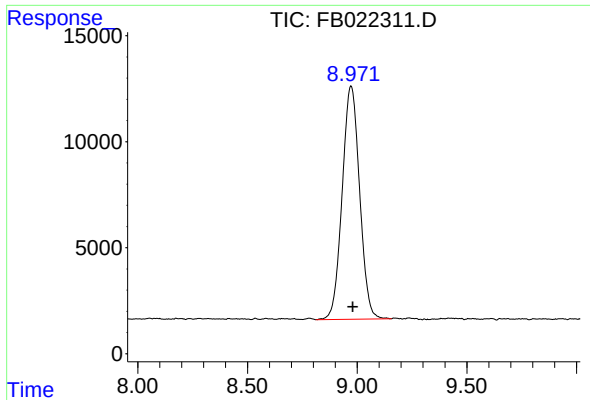

#5 AAA-TFT

R.T.: 8.972 min
Delta R.T.: -0.007 min
Response: 607611
Conc: 20.89 ng/ml

Instrument :
FID_B
ClientSampleId :

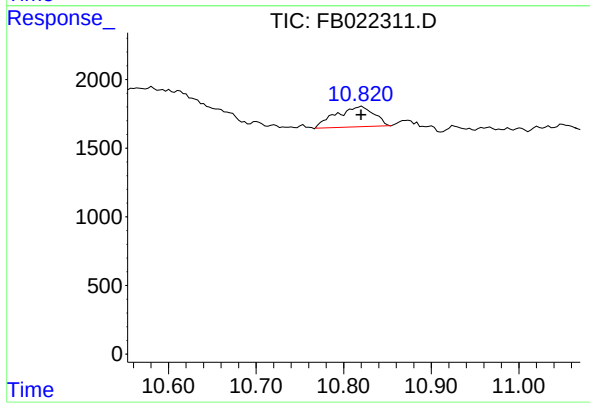

#6 Toluene

R.T.: 10.820 min
Delta R.T.: 0.000 min
Response: 4466
Conc: 0.09 ng/ml