

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB090519\  
 Data File : FB022315.D  
 Signal(s) : FID2B.CH  
 Acq On : 5 Sep 2019 22:15  
 Operator : DD/AJ  
 Sample : K4692-16  
 Misc : 5.02g/5.00ML DI WATER  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Sep 06 00:50:18 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB090419.M  
 Quant Title :  
 QLast Update : Wed Sep 04 17:01:40 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.971  | 572970   | 19.698 ng/ml |
| Target Compounds             |        |          |              |
| 3) t n-Heptane               | 7.946  | 1713     | 0.034 ng/ml  |
| 4) t Benzene                 | 8.066  | 5663     | 0.095 ng/ml  |
| 6) t Toluene                 | 10.808 | 7255     | 0.153 ng/ml  |
| 7) t Ethylbenzene            | 13.256 | 7522     | 0.251 ng/ml  |
| 8) t m-Xylene                | 13.380 | 12430    | 0.468 ng/ml  |
| 9) t O-Xylene                | 14.118 | 4609     | 0.190 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.408 | 6313     | 0.242 ng/ml  |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB090519\  
Data File : FB022315.D  
Signal(s) : FID2B.CH  
Acq On : 5 Sep 2019 22:15  
Operator : DD/AJ  
Sample : K4692-16  
Misc : 5.02g/5.00ML DI WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Sep 06 00:50:18 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB090419.M  
Quant Title :  
QLast Update : Wed Sep 04 17:01:40 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

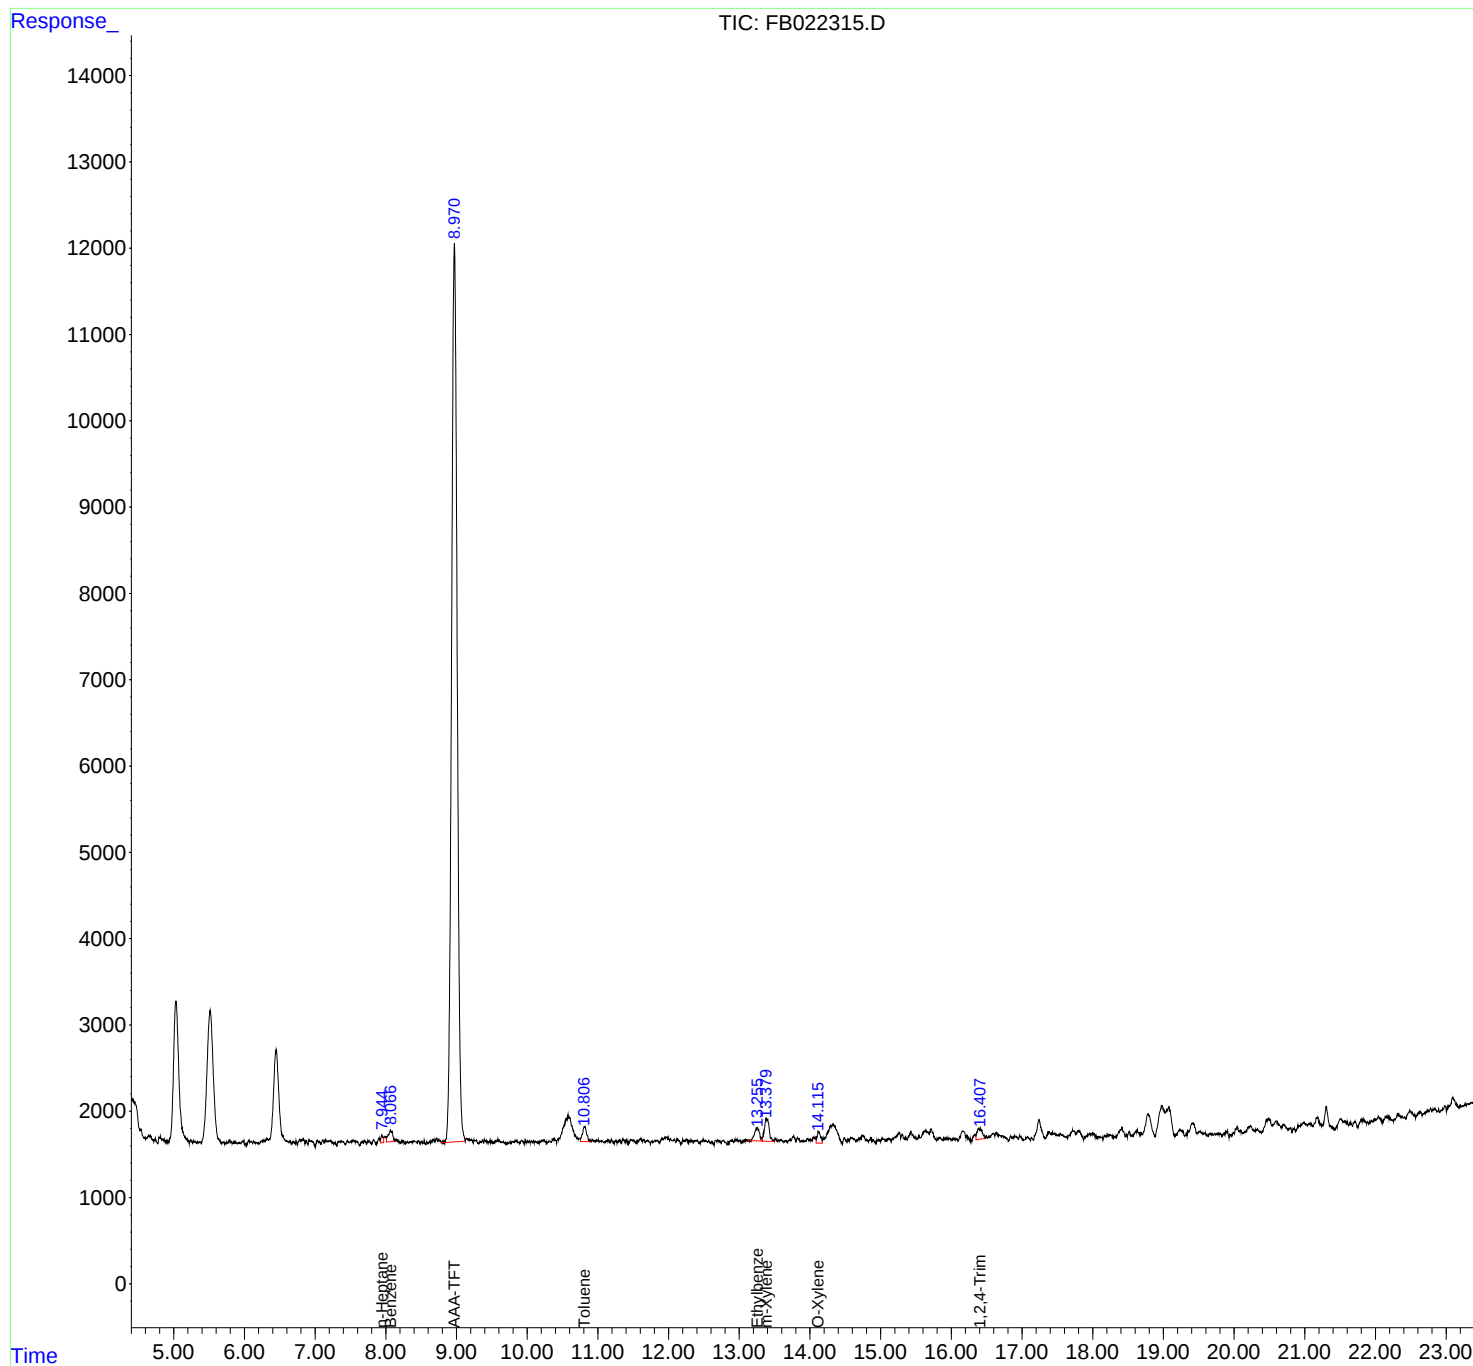


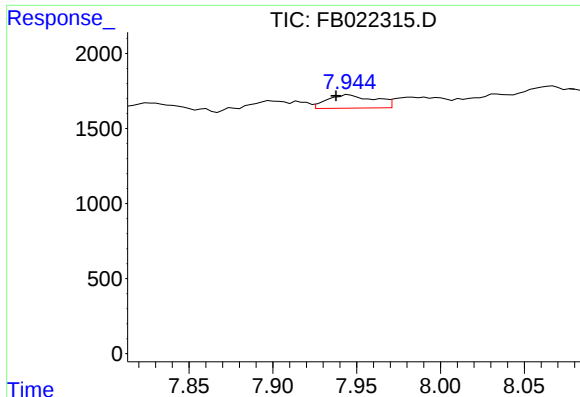

#3 n-Heptane


R.T.: 7.946 min  
Delta R.T.: 0.008 min  
Response: 1713  
Conc: 0.03 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

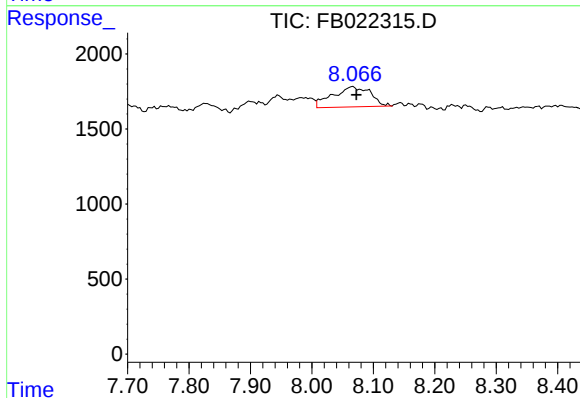


#4 Benzene

R.T.: 8.066 min  
Delta R.T.: -0.006 min  
Response: 5663  
Conc: 0.10 ng/ml

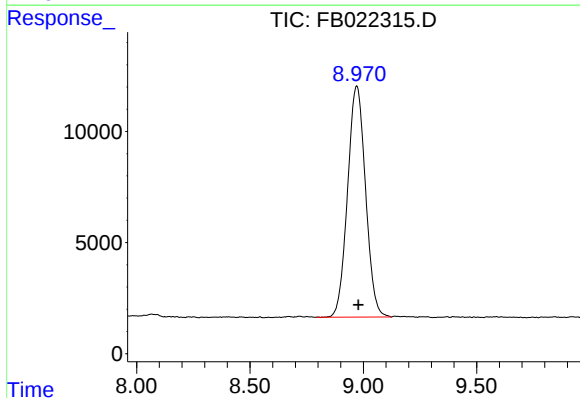


#5 AAA-TFT

R.T.: 8.971 min  
Delta R.T.: -0.008 min  
Response: 572970  
Conc: 19.70 ng/ml

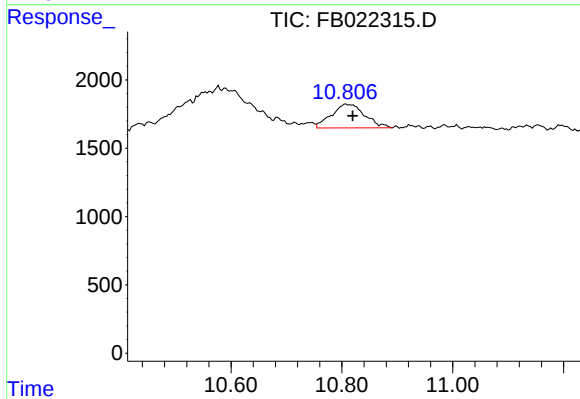

#6 Toluene


R.T.: 10.808 min  
Delta R.T.: -0.012 min  
Response: 7255  
Conc: 0.15 ng/ml

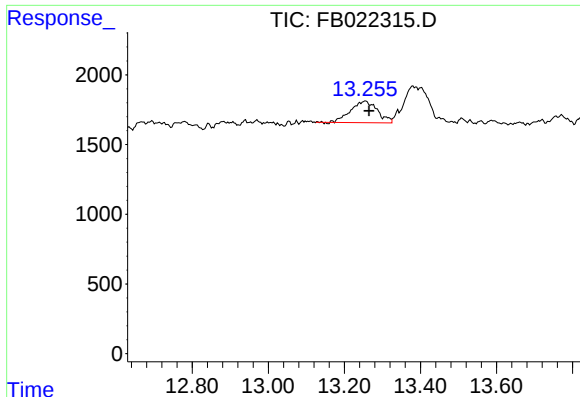

#7 Ethylbenzene


R.T.: 13.256 min  
Delta R.T.: -0.009 min  
Response: 7522  
Conc: 0.25 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

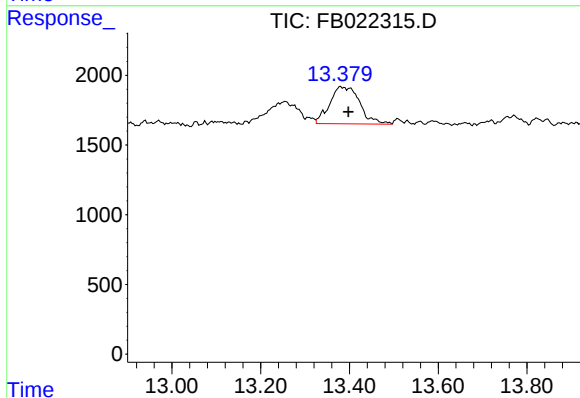


#8 m-Xylene

R.T.: 13.380 min  
Delta R.T.: -0.018 min  
Response: 12430  
Conc: 0.47 ng/ml

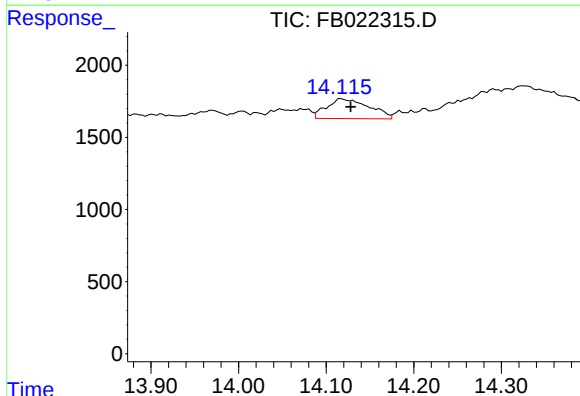

#9 O-Xylene

R.T.: 14.118 min  
Delta R.T.: -0.010 min  
Response: 4609  
Conc: 0.19 ng/ml

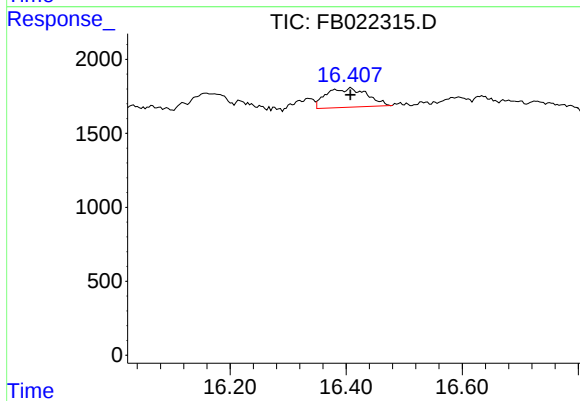

#10 1,2,4-Trimethylbenzene

R.T.: 16.408 min  
Delta R.T.: 0.001 min  
Response: 6313  
Conc: 0.24 ng/ml