

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090519\
 Data File : FB022297.D
 Signal(s) : FID2B.CH
 Acq On : 5 Sep 2019 10:11
 Operator : DD/AJ
 Sample : BSF0905S1
 Misc : 5.01G/5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0905S1

Integration File: Calibration.e
 Quant Time: Sep 06 00:46:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.972	626209	21.528 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.839	1422755	28.957 ng/ml
2) t	2,2,4-Trimethylpentane	7.590	1593335	30.856 ng/ml
3) t	n-Heptane	7.929	518840	10.309 ng/ml
4) t	Benzene	8.065	616829	10.393 ng/ml
6) t	Toluene	10.813	1711283	35.972 ng/ml
7) t	Ethylbenzene	13.259	467294	15.587 ng/ml
8) t	m-Xylene	13.392	852151	32.076 ng/ml
9) t	O-Xylene	14.122	733834	30.249 ng/ml
10) t	1,2,4-Trimethylbenzene	16.403	524909	20.134 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090519\
Data File : FB022297.D
Signal(s) : FID2B.CH
Acq On : 5 Sep 2019 10:11
Operator : DD/AJ
Sample : BSF0905S1
Misc : 5.01G/5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0905S1

Integration File: Calibration.e
Quant Time: Sep 06 00:46:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

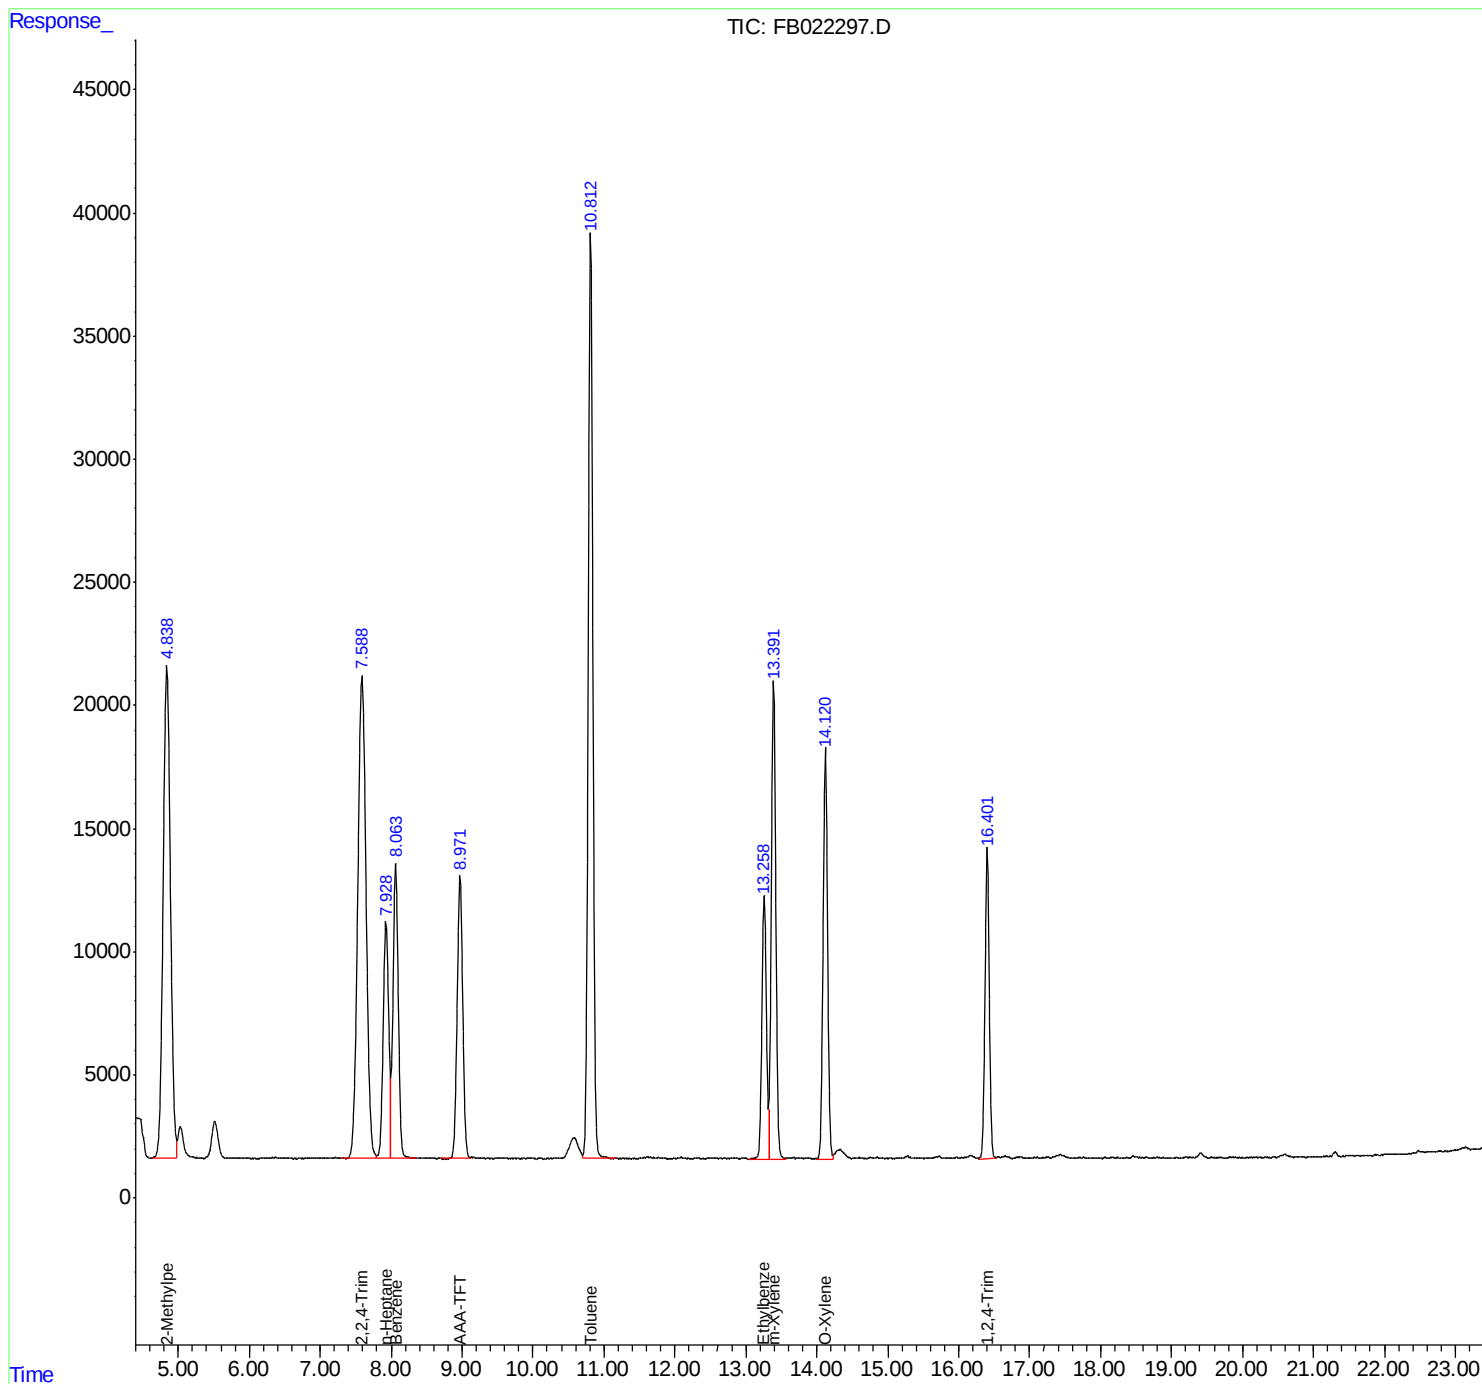


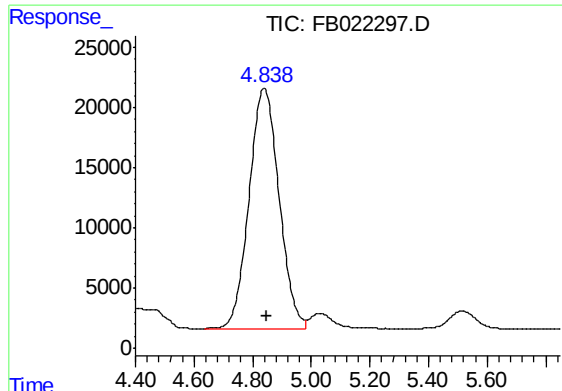

#1 2-Methylpentane


R.T.: 4.839 min
Delta R.T.: -0.008 min
Response: 1422755
Conc: 28.96 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0905S1

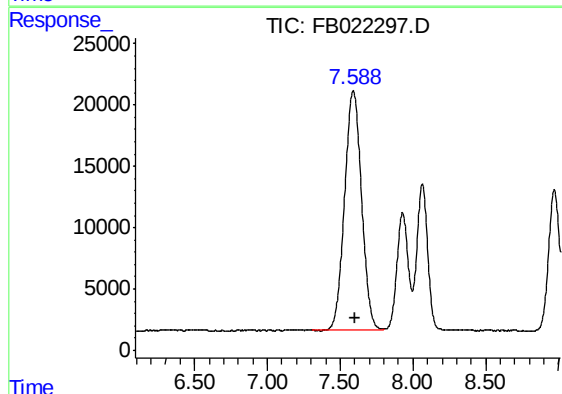


#2 2,2,4-Trimethylpentane

R.T.: 7.590 min
Delta R.T.: -0.008 min
Response: 1593335
Conc: 30.86 ng/ml

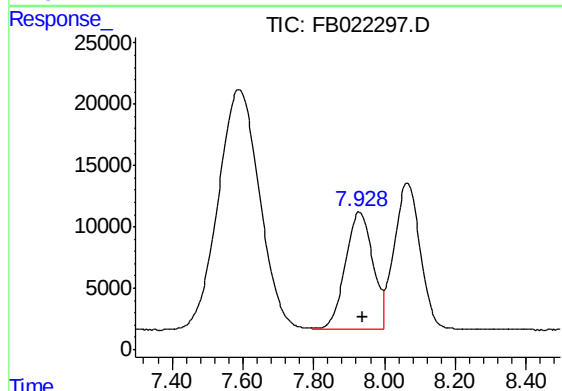


#3 n-Heptane

R.T.: 7.929 min
Delta R.T.: -0.008 min
Response: 518840
Conc: 10.31 ng/ml

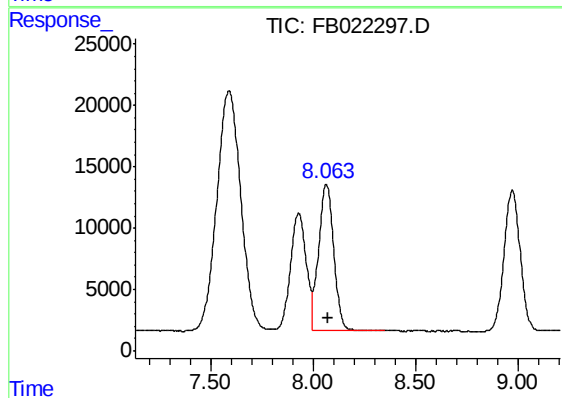

#4 Benzene


R.T.: 8.065 min
Delta R.T.: -0.008 min
Response: 616829
Conc: 10.39 ng/ml

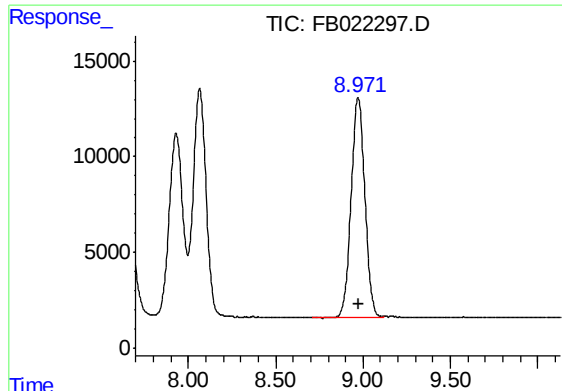

#5 AAA-TFT


R.T.: 8.972 min
Delta R.T.: -0.007 min
Response: 626209
Conc: 21.53 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0905S1

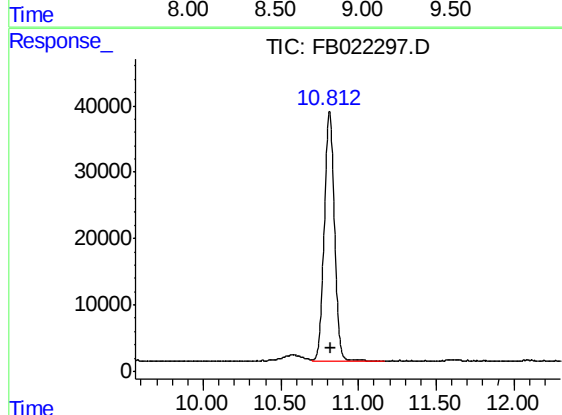


#6 Toluene

R.T.: 10.813 min
Delta R.T.: -0.007 min
Response: 1711283
Conc: 35.97 ng/ml

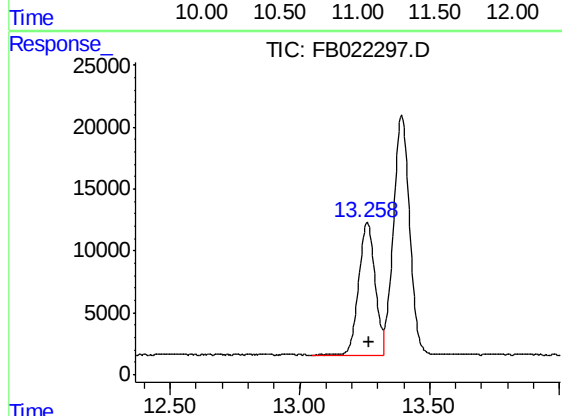


#7 Ethylbenzene

R.T.: 13.259 min
Delta R.T.: -0.006 min
Response: 467294
Conc: 15.59 ng/ml

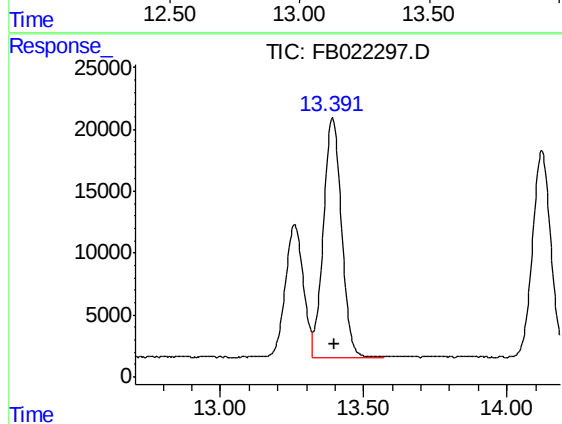

#8 m-Xylene


R.T.: 13.392 min
Delta R.T.: -0.006 min
Response: 852151
Conc: 32.08 ng/ml

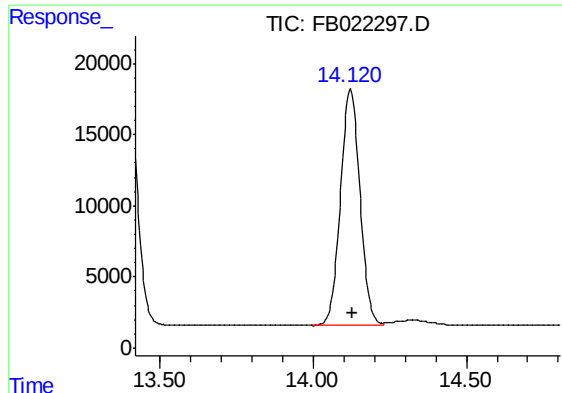

#9 O-Xylene

R.T.: 14.122 min
Delta R.T.: -0.006 min
Response: 733834
Conc: 30.25 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0905S1

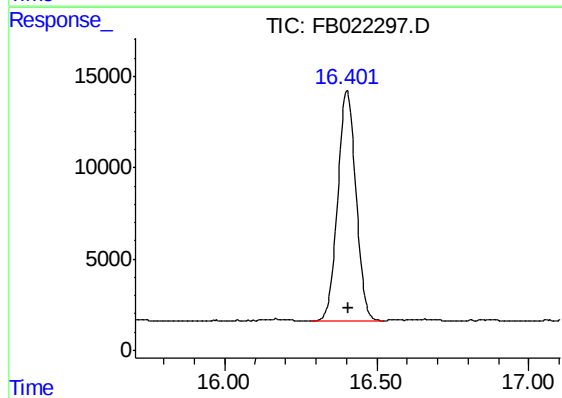

#10 1,2,4-Trimethylbenzene

R.T.: 16.403 min
Delta R.T.: -0.005 min
Response: 524909
Conc: 20.13 ng/ml