

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090519\
 Data File : FB022307.D
 Signal(s) : FID2B.CH
 Acq On : 5 Sep 2019 18:13
 Operator : DD/AJ
 Sample : K4696-04MSD
 Misc : 5.01g/5.00ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WS-SB05-COMPMSD

Integration File: Calibration.e
 Quant Time: Sep 06 00:48:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.971	639659	21.991 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.838	1097154	22.330 ng/ml
2) t 2,2,4-Trimethylpentane	7.590	1221272	23.651 ng/ml
3) t n-Heptane	7.929	390334	7.755 ng/ml
4) t Benzene	8.064	544183	9.169 ng/ml
6) t Toluene	10.812	1499257	31.515 ng/ml
7) t Ethylbenzene	13.259	418129	13.947 ng/ml
8) t m-Xylene	13.392	783043	29.475 ng/ml
9) t O-Xylene	14.122	697581	28.754 ng/ml
10) t 1,2,4-Trimethylbenzene	16.402	453384	17.390 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090519\
Data File : FB022307.D
Signal(s) : FID2B.CH
Acq On : 5 Sep 2019 18:13
Operator : DD/AJ
Sample : K4696-04MSD
Misc : 5.01g/5.00ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
WS-SB05-COMPMSD

Integration File: Calibration.e
Quant Time: Sep 06 00:48:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

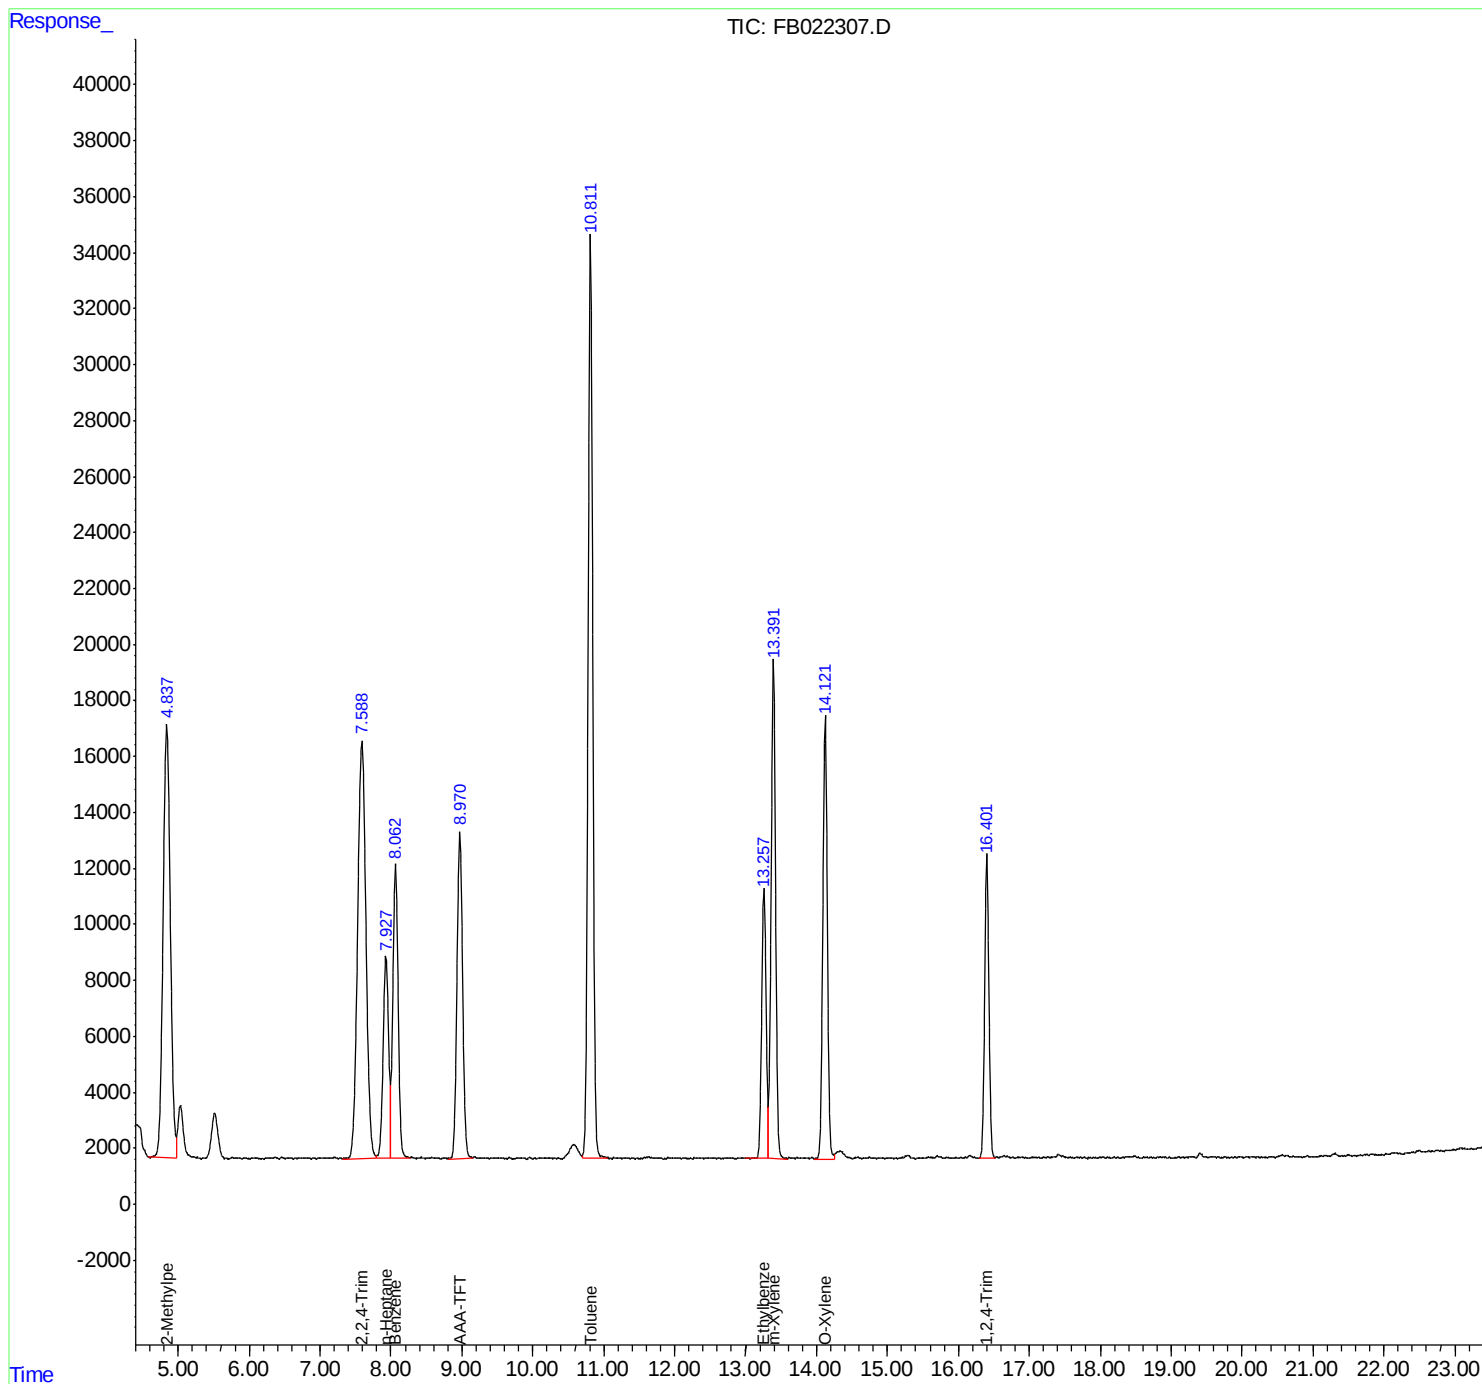


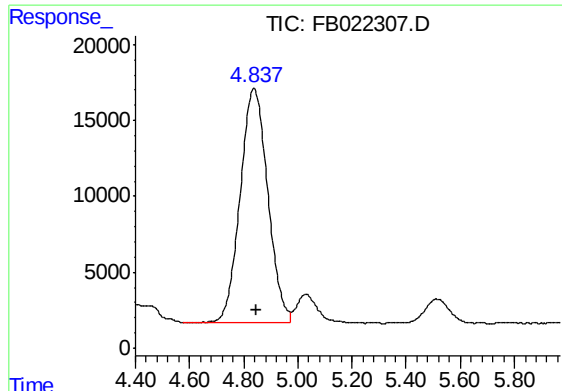

#1 2-Methylpentane


R.T.: 4.838 min
Delta R.T.: -0.009 min
Response: 1097154
Conc: 22.33 ng/ml

Instrument :
FID_B
ClientSampleId :
WS-SB05-COMPMSD

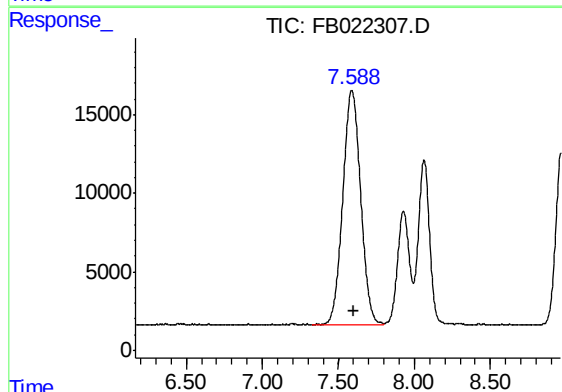


#2 2,2,4-Trimethylpentane

R.T.: 7.590 min
Delta R.T.: -0.008 min
Response: 1221272
Conc: 23.65 ng/ml

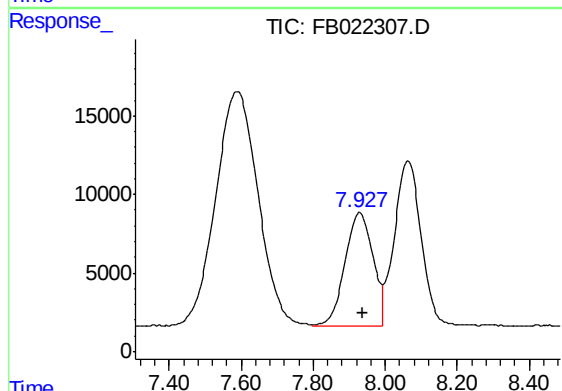


#3 n-Heptane

R.T.: 7.929 min
Delta R.T.: -0.008 min
Response: 390334
Conc: 7.76 ng/ml

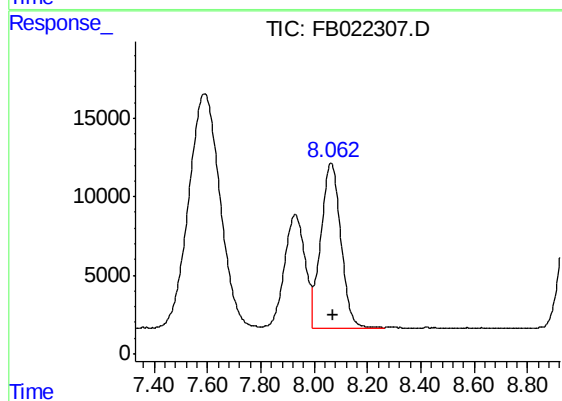

#4 Benzene


R.T.: 8.064 min
Delta R.T.: -0.008 min
Response: 544183
Conc: 9.17 ng/ml

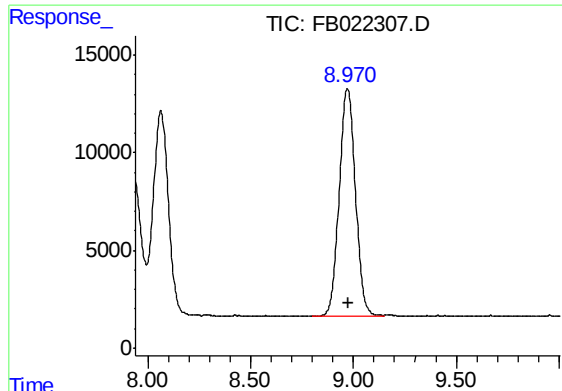

#5 AAA-TFT


R.T.: 8.971 min
Delta R.T.: -0.008 min
Response: 639659
Conc: 21.99 ng/ml

Instrument :
FID_B
ClientSampleId :
WS-SB05-COMPMSD

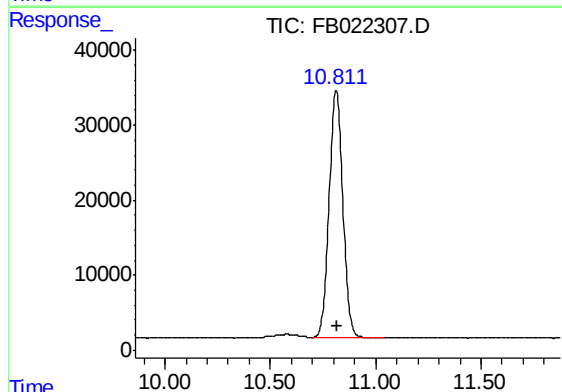


#6 Toluene

R.T.: 10.812 min
Delta R.T.: -0.007 min
Response: 1499257
Conc: 31.51 ng/ml

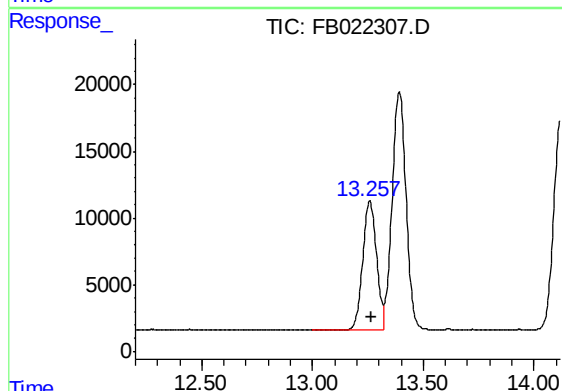


#7 Ethylbenzene

R.T.: 13.259 min
Delta R.T.: -0.006 min
Response: 418129
Conc: 13.95 ng/ml

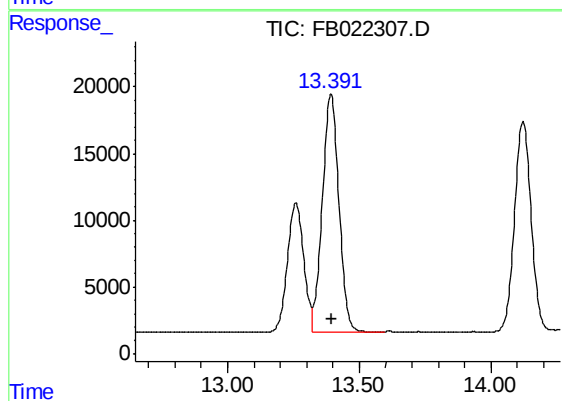

#8 m-Xylene


R.T.: 13.392 min
Delta R.T.: -0.006 min
Response: 783043
Conc: 29.48 ng/ml

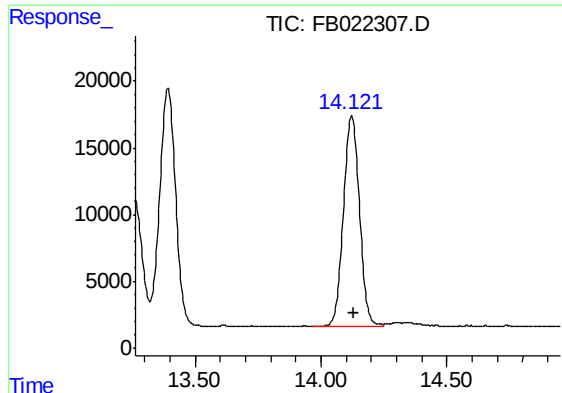

#9 O-Xylene

R.T.: 14.122 min
Delta R.T.: -0.006 min
Response: 697581
Conc: 28.75 ng/ml

Instrument :
FID_B
ClientSampleId :
WS-SB05-COMPMSD

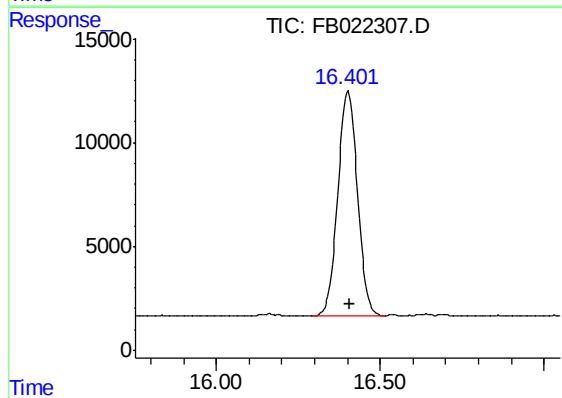

#10 1,2,4-Trimethylbenzene

R.T.: 16.402 min
Delta R.T.: -0.005 min
Response: 453384
Conc: 17.39 ng/ml