

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB090619\  
 Data File : FB022320.D  
 Signal(s) : FID2B.CH  
 Acq On : 6 Sep 2019 11:01  
 Operator : DD/AJ  
 Sample : K4661-02  
 Misc : 5.06g/5.00ML DI WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Sep 06 22:57:49 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB090419.M  
 Quant Title :  
 QLast Update : Wed Sep 04 17:01:40 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

|                             | Compound               | R.T.   | Response | Conc Units   |
|-----------------------------|------------------------|--------|----------|--------------|
| -----                       |                        |        |          |              |
| System Monitoring Compounds |                        |        |          |              |
| 5) s                        | AAA-TFT                | 8.972  | 581661   | 19.997 ng/ml |
| Target Compounds            |                        |        |          |              |
| 6) t                        | Toluene                | 10.812 | 33948    | 0.714 ng/ml  |
| 7) t                        | Ethylbenzene           | 13.254 | 24258    | 0.809 ng/ml  |
| 8) t                        | m-Xylene               | 13.391 | 74963    | 2.822 ng/ml  |
| 9) t                        | O-Xylene               | 14.126 | 77983    | 3.214 ng/ml  |
| 10) t                       | 1,2,4-Trimethylbenzene | 16.404 | 82792    | 3.176 ng/ml  |
| -----                       |                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB090619\  
Data File : FB022320.D  
Signal(s) : FID2B.CH  
Acq On : 6 Sep 2019 11:01  
Operator : DD/AJ  
Sample : K4661-02  
Misc : 5.06g/5.00ML DI WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Sep 06 22:57:49 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB090419.M  
Quant Title :  
QLast Update : Wed Sep 04 17:01:40 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

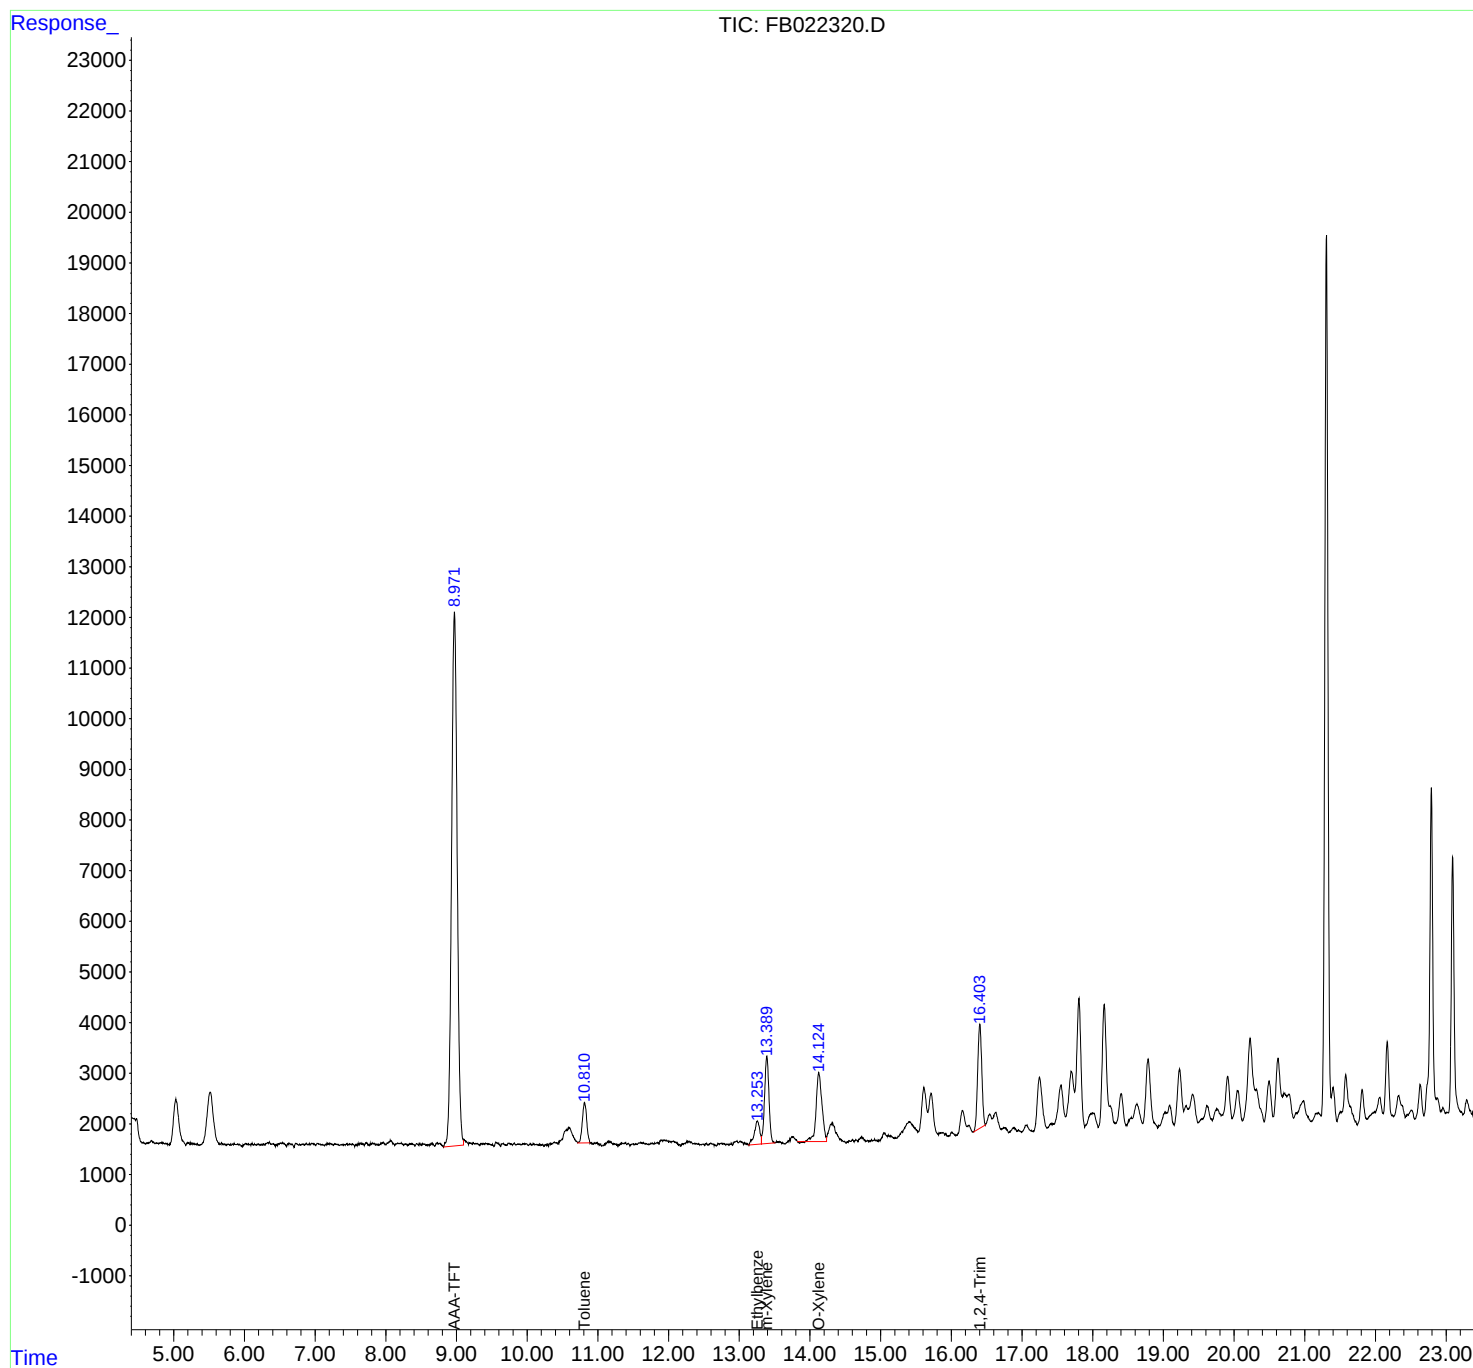


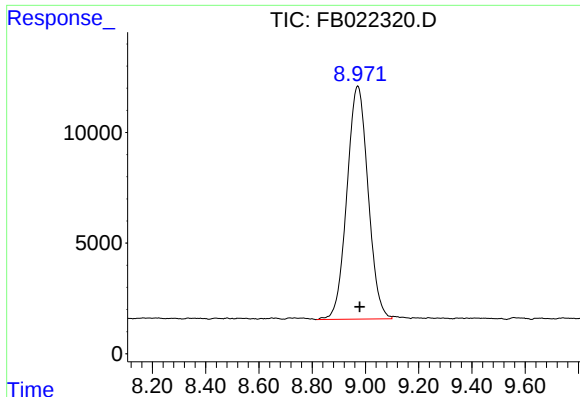

#5 AAA-TFT


R.T.: 8.972 min  
Delta R.T.: -0.007 min  
Response: 581661  
Conc: 20.00 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

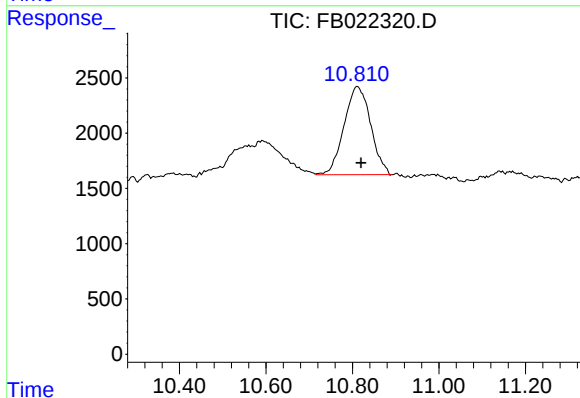


#6 Toluene

R.T.: 10.812 min  
Delta R.T.: -0.008 min  
Response: 33948  
Conc: 0.71 ng/ml

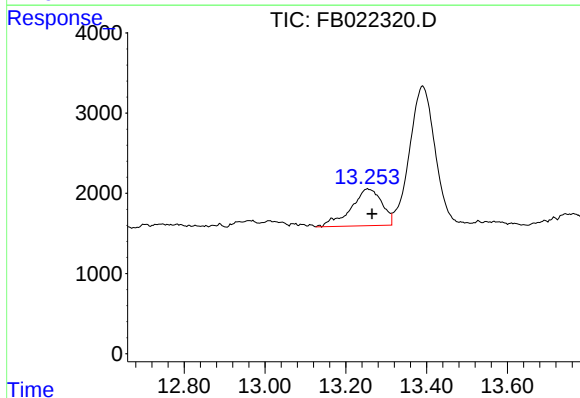


#7 Ethylbenzene

R.T.: 13.254 min  
Delta R.T.: -0.011 min  
Response: 24258  
Conc: 0.81 ng/ml

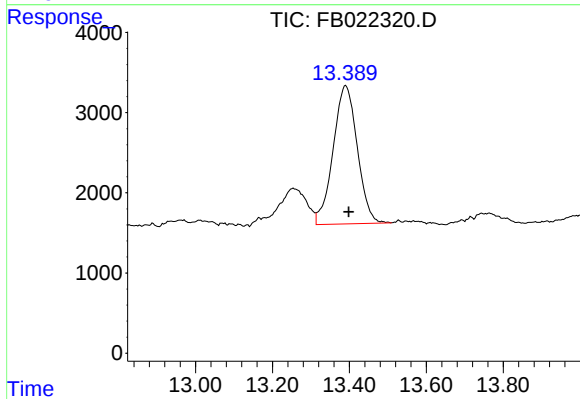

#8 m-Xylene


R.T.: 13.391 min  
Delta R.T.: -0.007 min  
Response: 74963  
Conc: 2.82 ng/ml

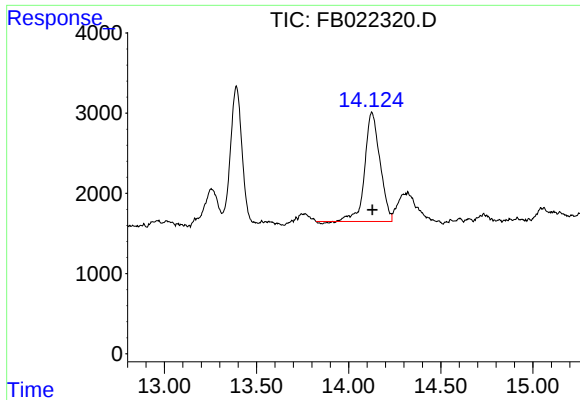

#9 O-Xylene

R.T.: 14.126 min  
Delta R.T.: -0.002 min  
Response: 77983  
Conc: 3.21 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

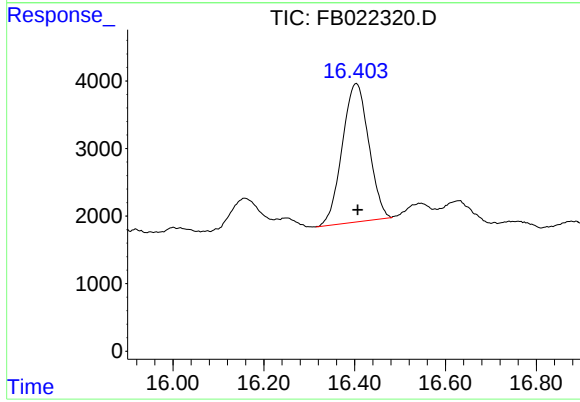

#10 1,2,4-Trimethylbenzene

R.T.: 16.404 min  
Delta R.T.: -0.003 min  
Response: 82792  
Conc: 3.18 ng/ml