

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090619\
Data File : FB022322.D
Signal(s) : FID2B.CH
Acq On : 6 Sep 2019 12:02
Operator : DD/AJ
Sample : K4656-02
Misc : 5.04g/5.00ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 06 22:58:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.973	601591	20.682 ng/ml
Target Compounds			
6) t Toluene	10.814	12344	0.259 ng/ml
8) t m-Xylene	13.397	8523	0.321 ng/ml
9) t O-Xylene	14.105	8300	0.342 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090619\
Data File : FB022322.D
Signal(s) : FID2B.CH
Acq On : 6 Sep 2019 12:02
Operator : DD/AJ
Sample : K4656-02
Misc : 5.04g/5.00ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 06 22:58:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

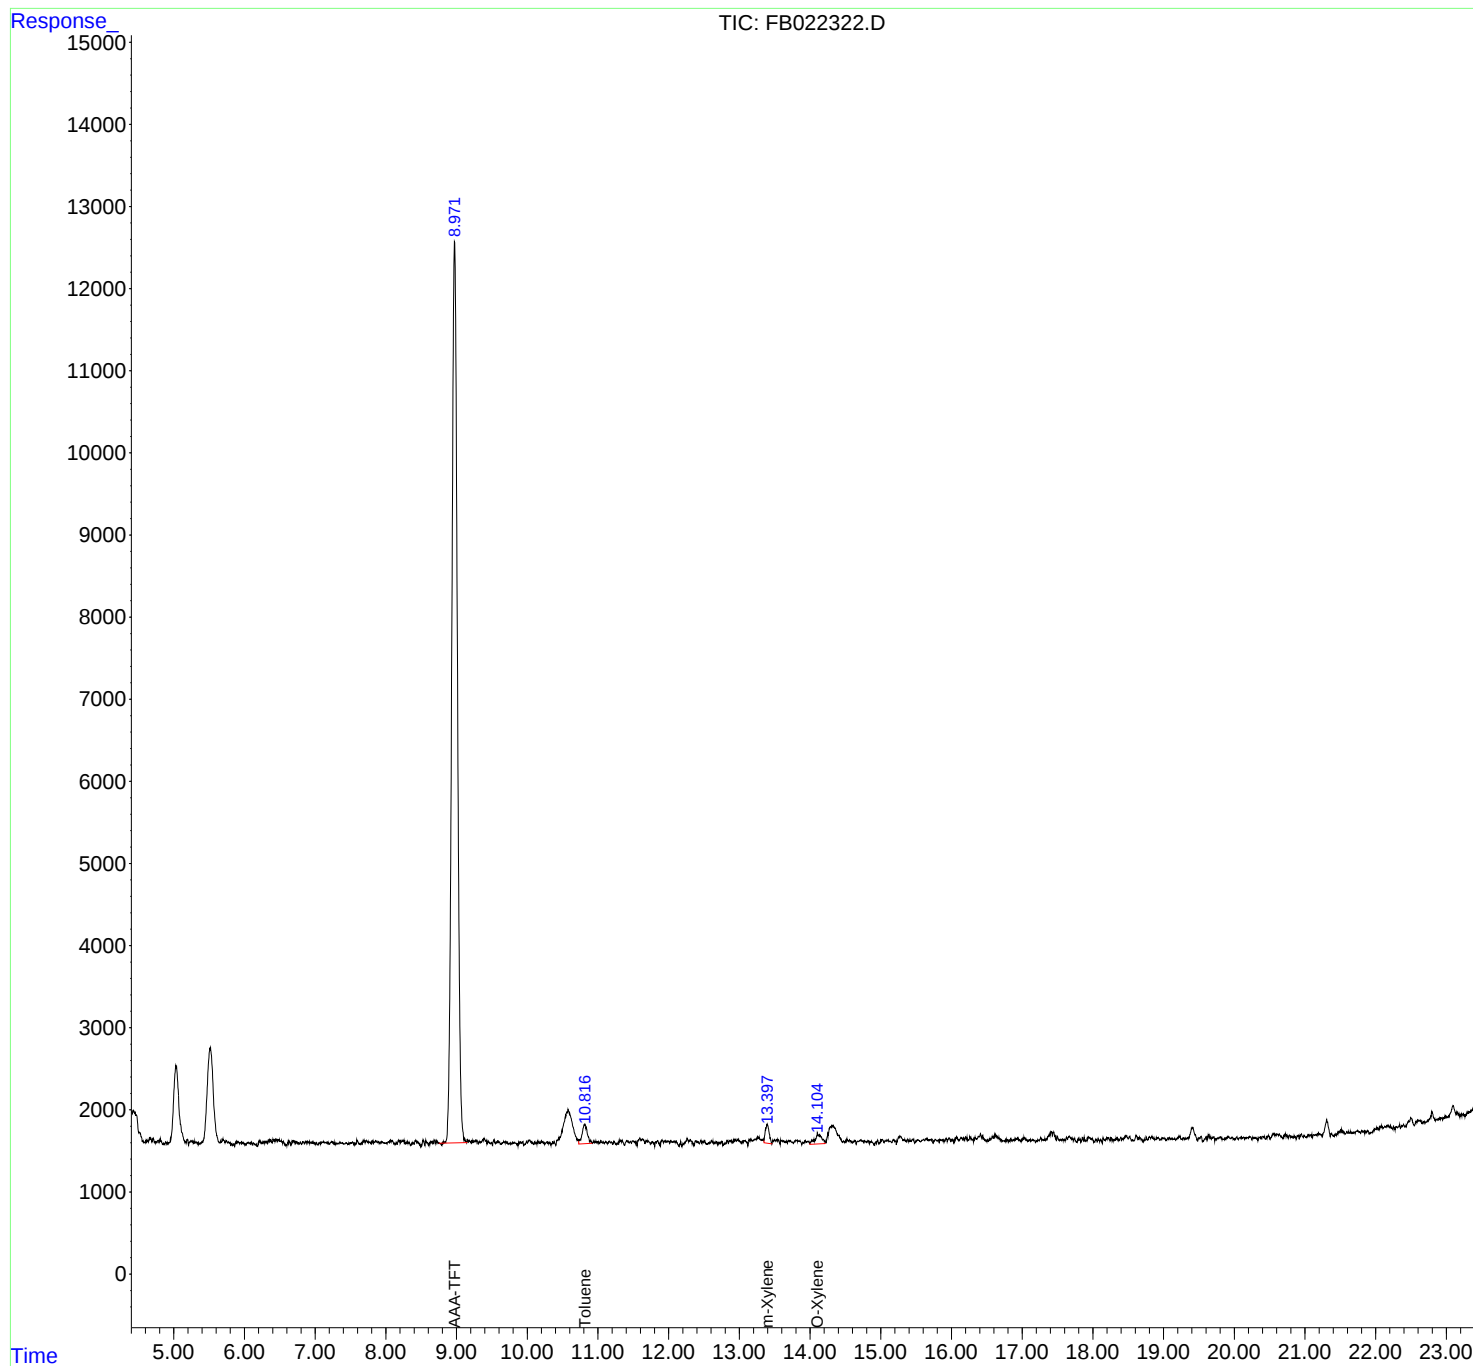


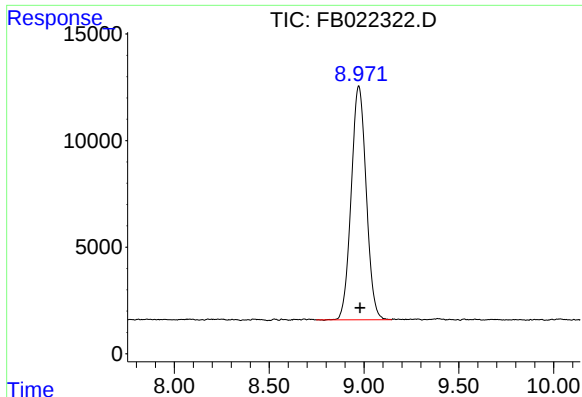

#5 AAA-TFT


R.T.: 8.973 min
Delta R.T.: -0.006 min
Response: 601591
Conc: 20.68 ng/ml

Instrument :
FID_B
ClientSampleId :

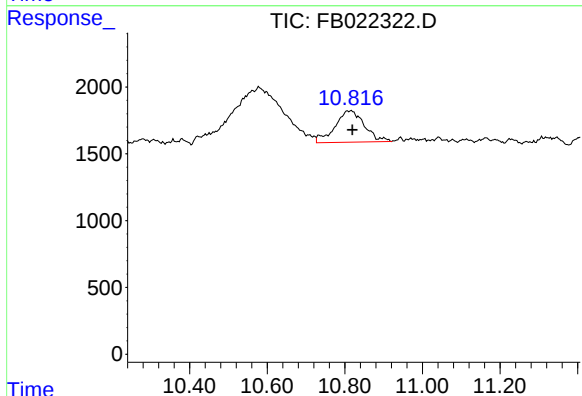


#6 Toluene

R.T.: 10.814 min
Delta R.T.: -0.005 min
Response: 12344
Conc: 0.26 ng/ml

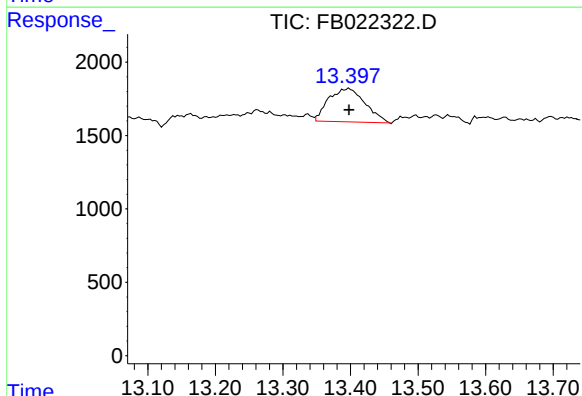

#8 m-Xylene

R.T.: 13.397 min
Delta R.T.: -0.001 min
Response: 8523
Conc: 0.32 ng/ml

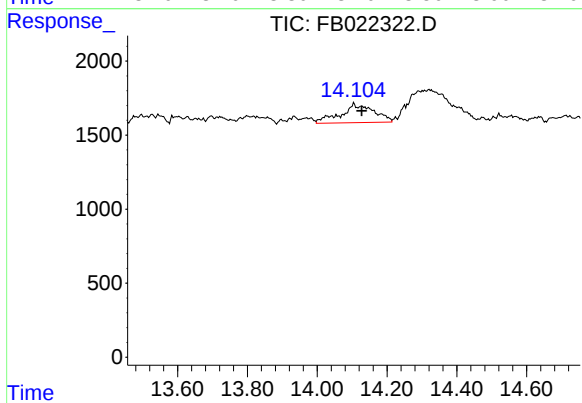

#9 O-Xylene

R.T.: 14.105 min
Delta R.T.: -0.022 min
Response: 8300
Conc: 0.34 ng/ml