

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090619\
 Data File : FB022327.D
 Signal(s) : FID2B.CH
 Acq On : 6 Sep 2019 16:57
 Operator : DD/AJ
 Sample : K4758-05
 Misc : 5.02g/5.00ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 06 22:59:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.969	549551	18.893 ng/ml
Target Compounds			
6) t Toluene	10.821	5645	0.119 ng/ml
8) t m-Xylene	13.390	5136	0.193 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090619\
Data File : FB022327.D
Signal(s) : FID2B.CH
Acq On : 6 Sep 2019 16:57
Operator : DD/AJ
Sample : K4758-05
Misc : 5.02g/5.00ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 06 22:59:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

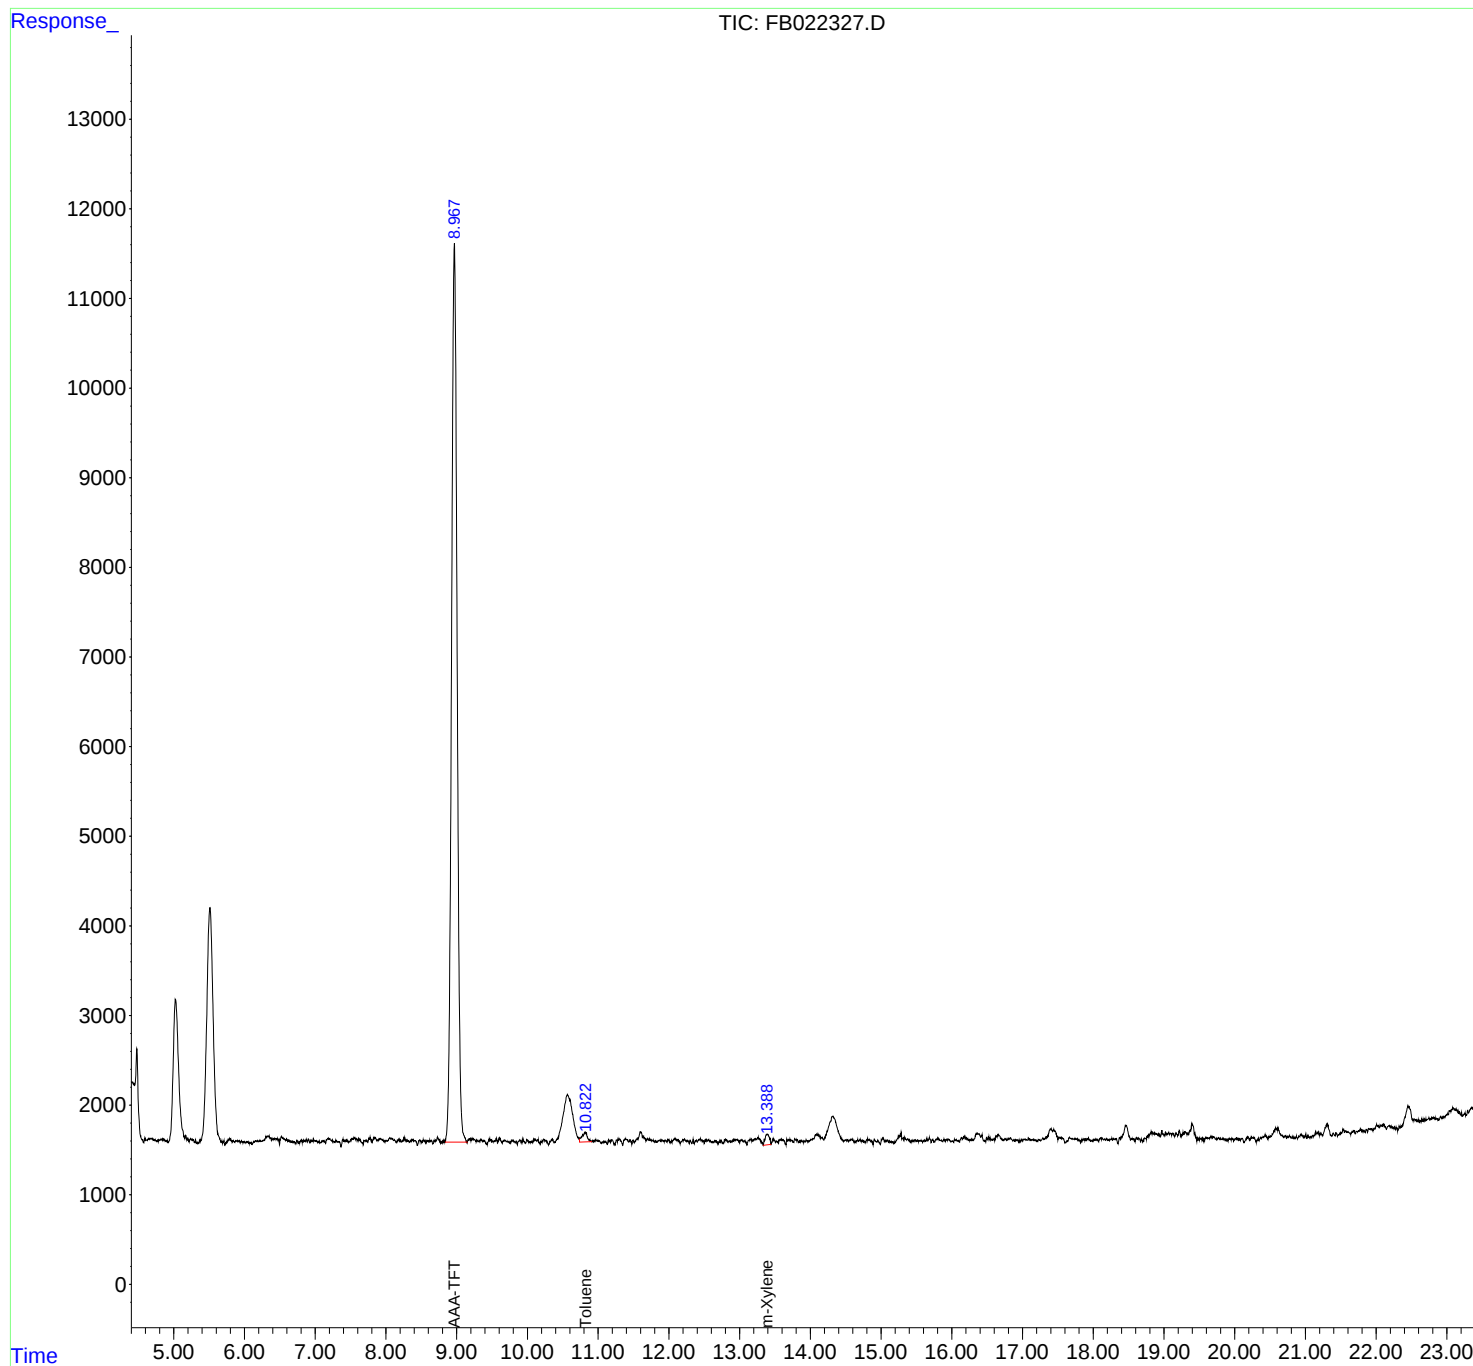


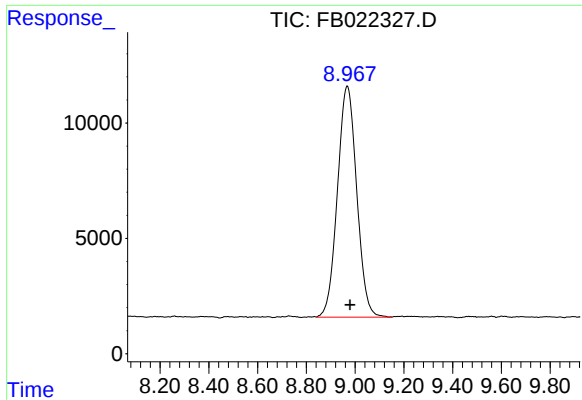

#5 AAA-TFT


R.T.: 8.969 min
Delta R.T.: -0.011 min
Response: 549551
Conc: 18.89 ng/ml

Instrument :
FID_B
ClientSampleId :

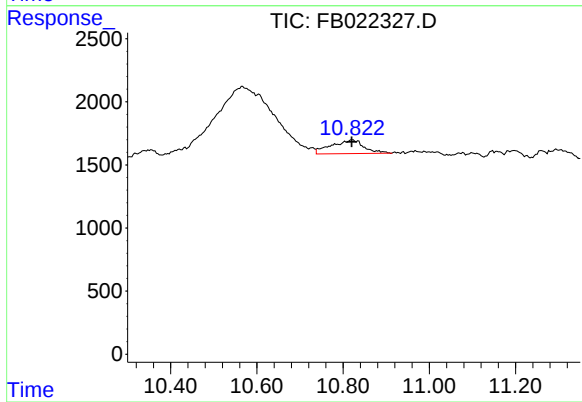

#6 Toluene

R.T.: 10.821 min
Delta R.T.: 0.002 min
Response: 5645
Conc: 0.12 ng/ml

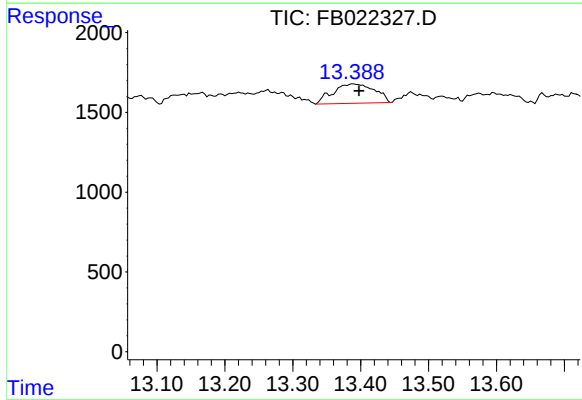

#8 m-Xylene

R.T.: 13.390 min
Delta R.T.: -0.008 min
Response: 5136
Conc: 0.19 ng/ml