

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090619\
Data File : FB022344.D
Signal(s) : FID2B.CH
Acq On : 7 Sep 2019 2:34
Operator : DD/AJ
Sample : K4759-05
Misc : 5.04g/5.00ML DI WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 07 06:24:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.972	586774	20.173 ng/ml
Target Compounds			
6) t Toluene	10.817	7053	0.148 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090619\
Data File : FB022344.D
Signal(s) : FID2B.CH
Acq On : 7 Sep 2019 2:34
Operator : DD/AJ
Sample : K4759-05
Misc : 5.04g/5.00ML DI WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 07 06:24:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

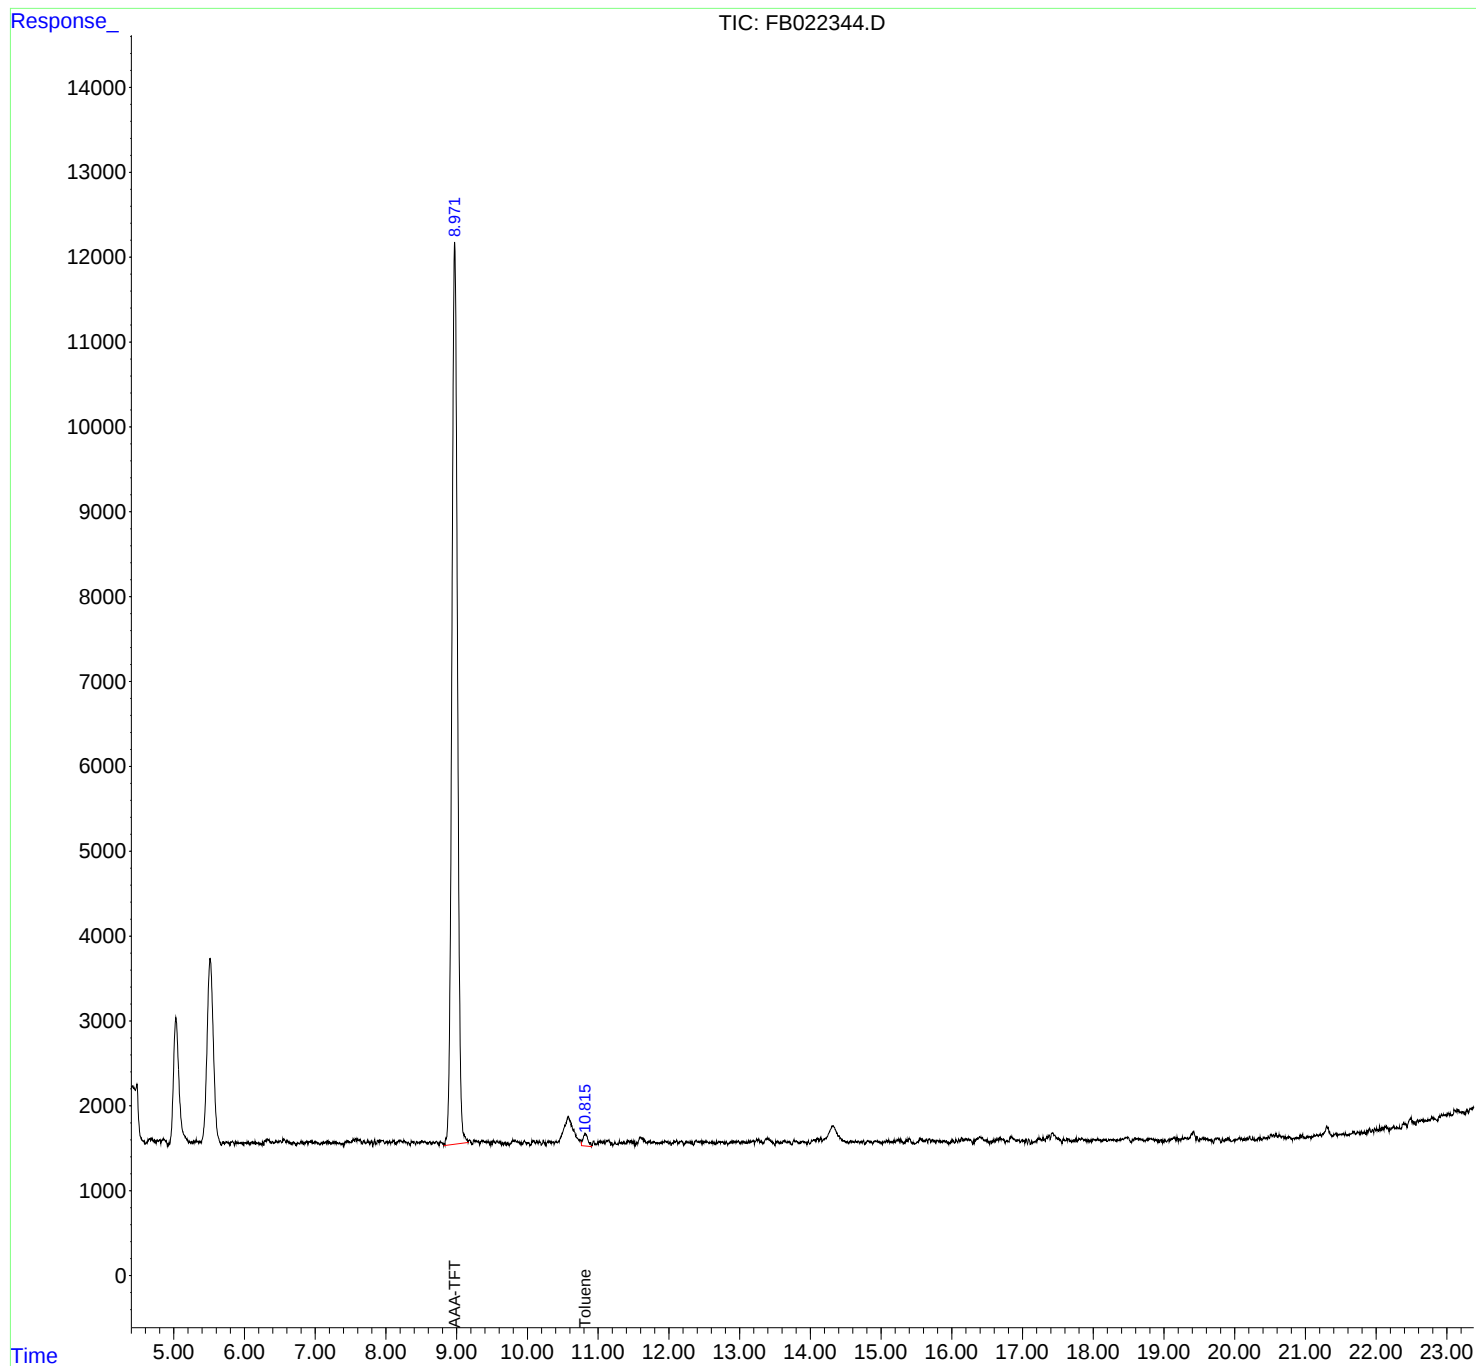


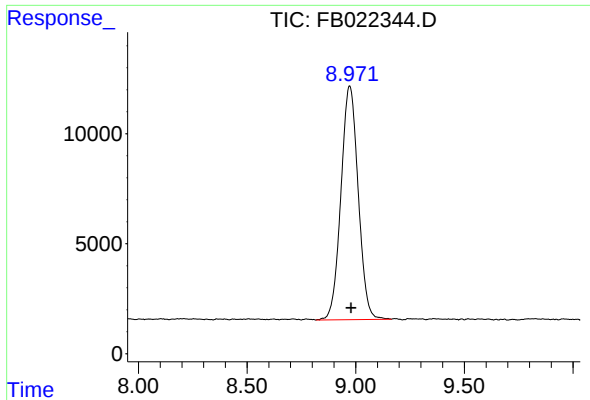

#5 AAA-TFT

R.T.: 8.972 min
Delta R.T.: -0.007 min
Response: 586774
Conc: 20.17 ng/ml

Instrument :
FID_B
ClientSampleId :

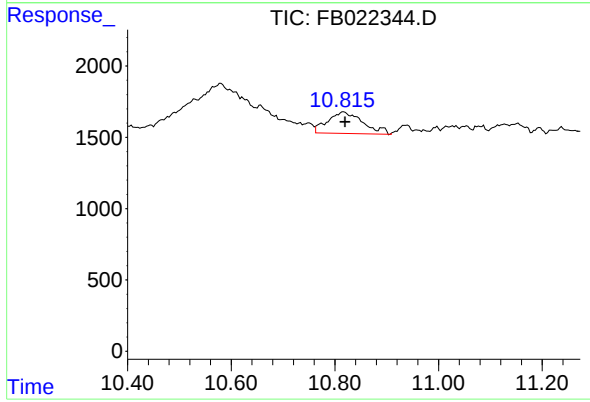

#6 Toluene

R.T.: 10.817 min
Delta R.T.: -0.003 min
Response: 7053
Conc: 0.15 ng/ml