

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090619\
Data File : FB022321.D
Signal(s) : FID2B.CH
Acq On : 6 Sep 2019 11:31
Operator : DD/AJ
Sample : K4663-02
Misc : 5.02g/5.00ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OK-03-090519

Integration File: Calibration.e
Quant Time: Sep 06 22:58:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.972	563532	19.374 ng/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090619\
Data File : FB022321.D
Signal(s) : FID2B.CH
Acq On : 6 Sep 2019 11:31
Operator : DD/AJ
Sample : K4663-02
Misc : 5.02g/5.00ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OK-03-090519

Integration File: Calibration.e
Quant Time: Sep 06 22:58:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

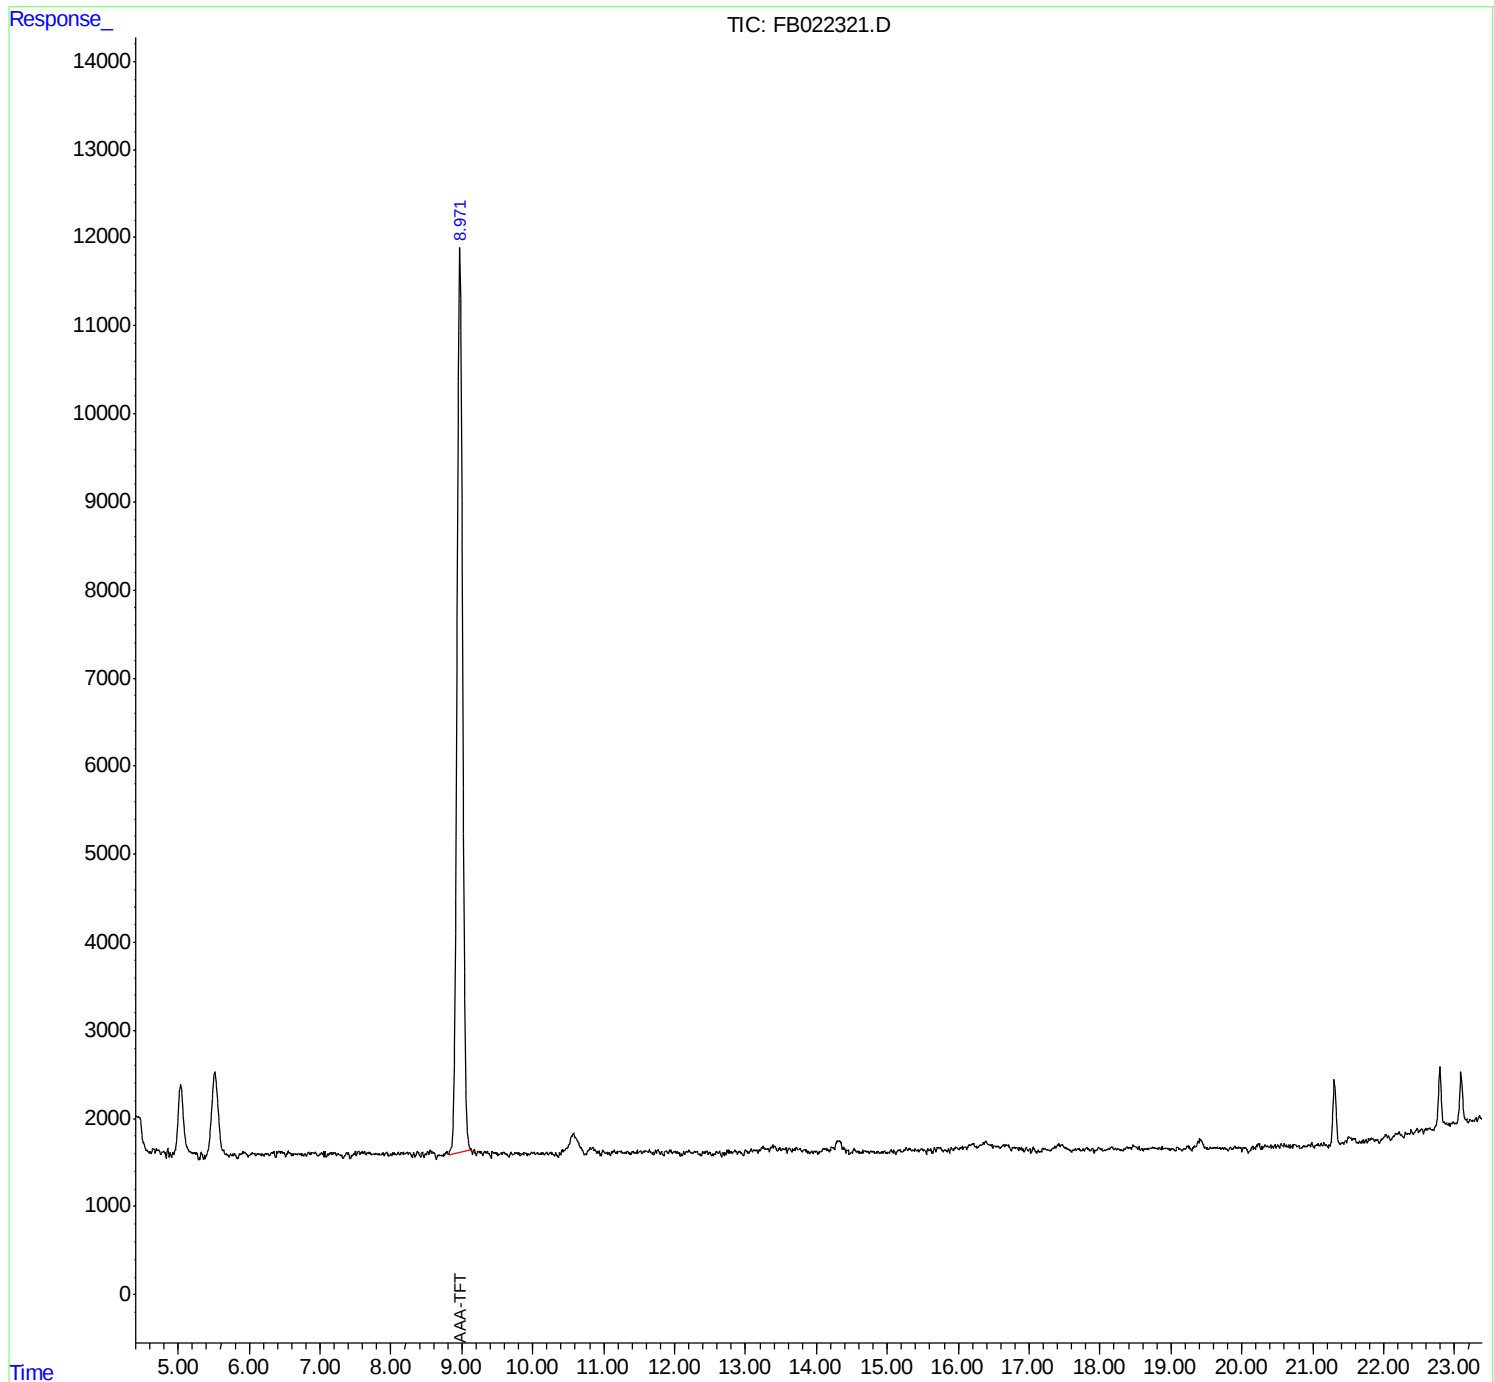

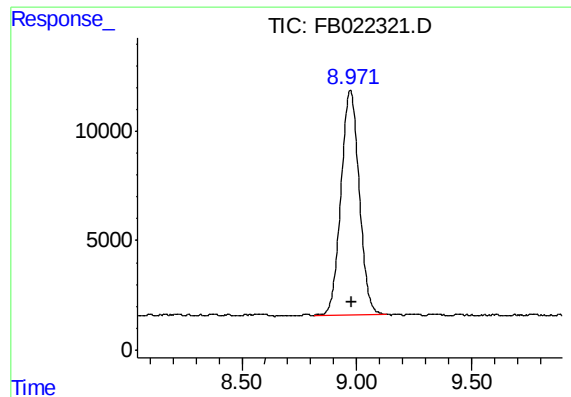

#5 AAA-TFT

R.T.: 8.972 min
Delta R.T.: -0.007 min
Response: 563532
Conc: 19.37 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-03-090519