

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090619\
 Data File : FB022324.D
 Signal(s) : FID2B.CH
 Acq On : 6 Sep 2019 13:02
 Operator : DD/AJ
 Sample : K4656-02MS
 Misc : 5.04g/5.00ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-06-090519MS

Integration File: Calibration.e
 Quant Time: Sep 06 22:58:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.972	610314	20.982 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.839	990816	20.166 ng/ml
2) t 2,2,4-Trimethylpentane	7.590	1073616	20.791 ng/ml
3) t n-Heptane	7.930	347010	6.895 ng/ml
4) t Benzene	8.065	536240	9.035 ng/ml
6) t Toluene	10.813	1490024	31.321 ng/ml
7) t Ethylbenzene	13.259	425055	14.178 ng/ml
8) t m-Xylene	13.392	812625	30.589 ng/ml
9) t O-Xylene	14.121	728554	30.031 ng/ml
10) t 1,2,4-Trimethylbenzene	16.403	449625	17.246 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090619\
Data File : FB022324.D
Signal(s) : FID2B.CH
Acq On : 6 Sep 2019 13:02
Operator : DD/AJ
Sample : K4656-02MS
Misc : 5.04g/5.00ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
AU-06-090519MS

Integration File: Calibration.e
Quant Time: Sep 06 22:58:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

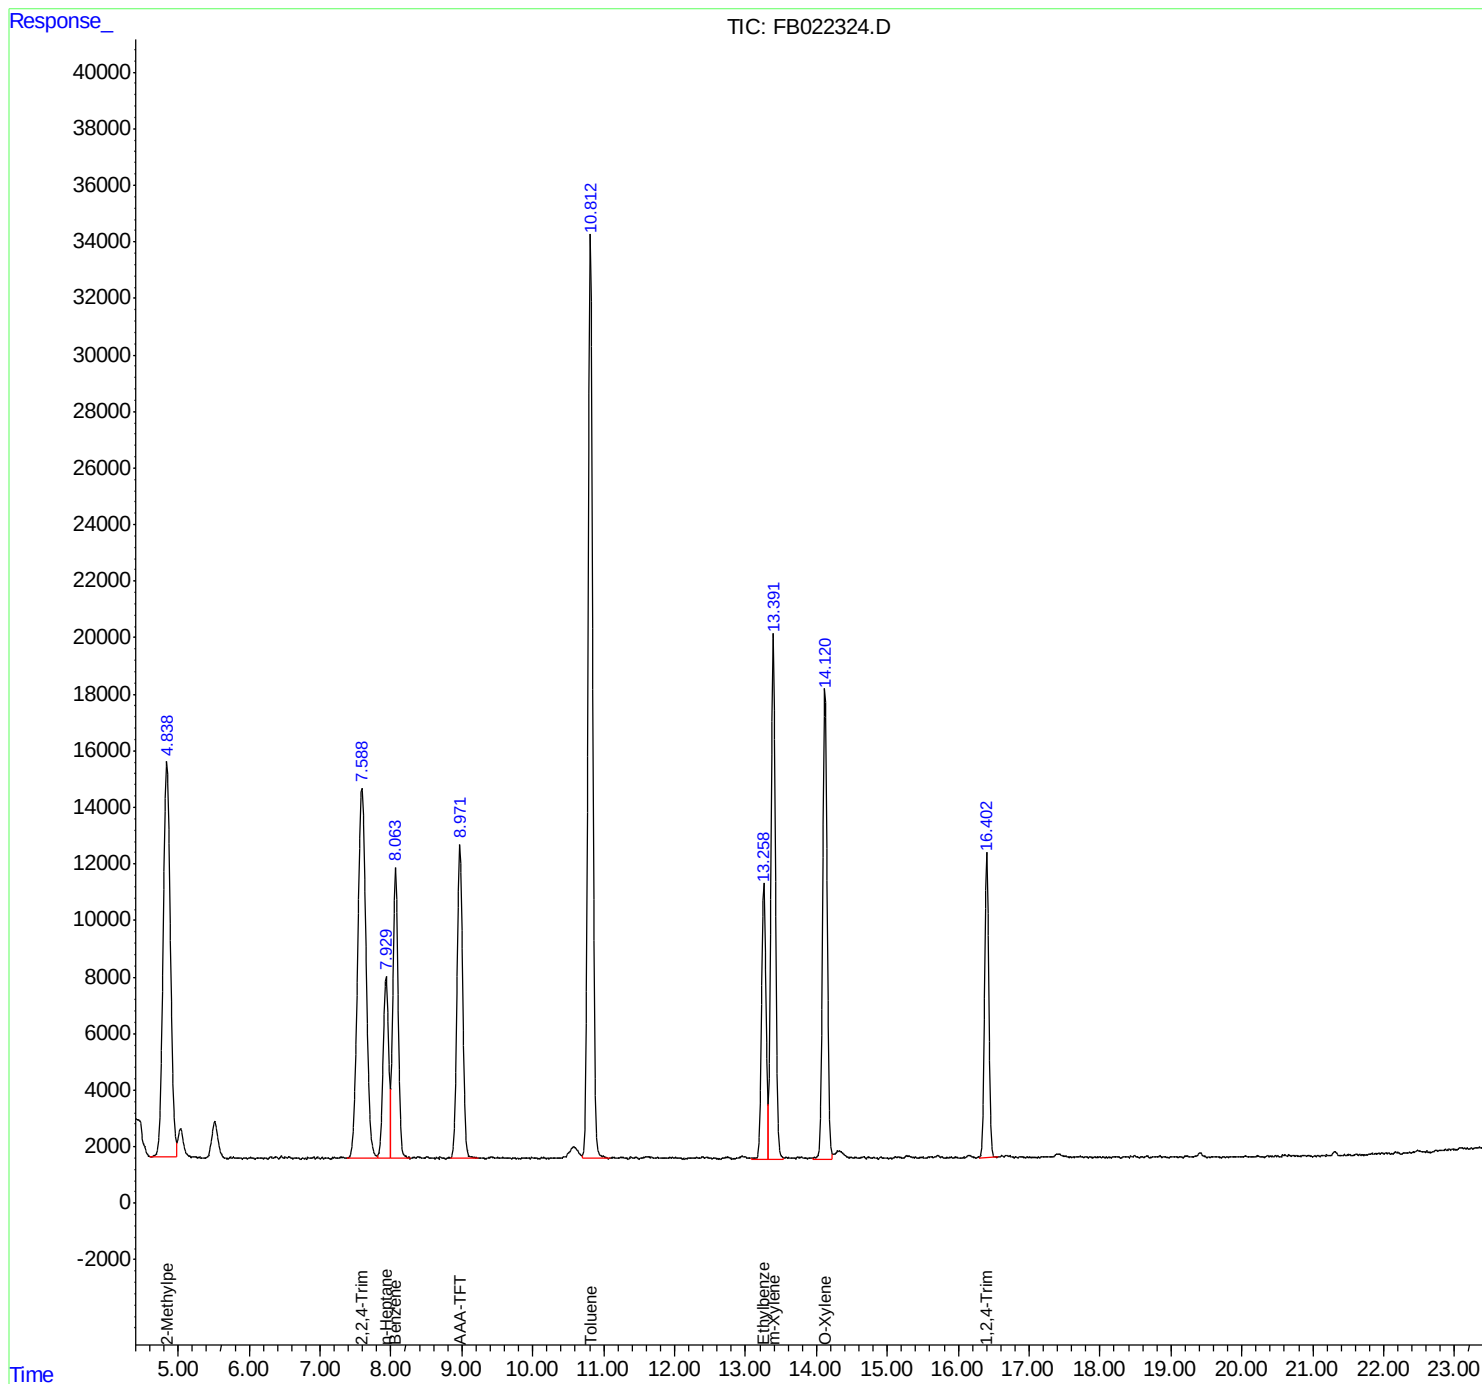


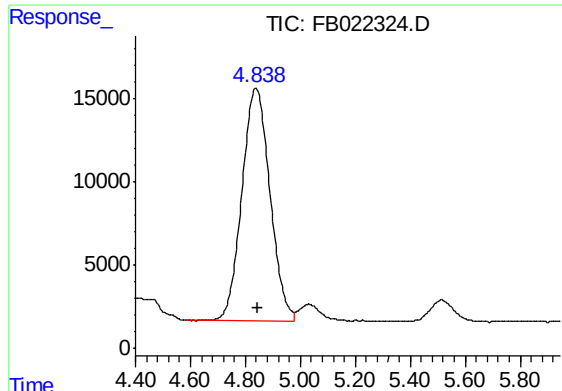

#1 2-Methylpentane


R.T.: 4.839 min
Delta R.T.: -0.008 min
Response: 990816
Conc: 20.17 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-090519MS

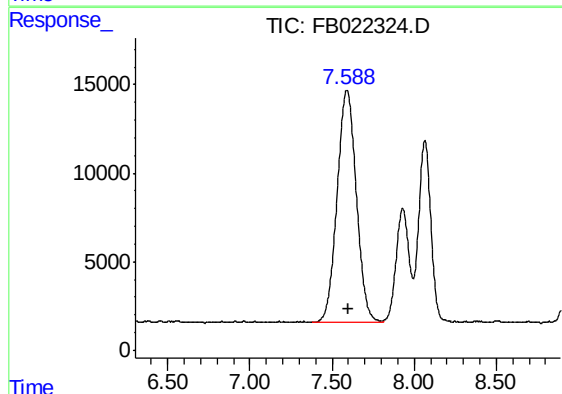


#2 2,2,4-Trimethylpentane

R.T.: 7.590 min
Delta R.T.: -0.007 min
Response: 1073616
Conc: 20.79 ng/ml

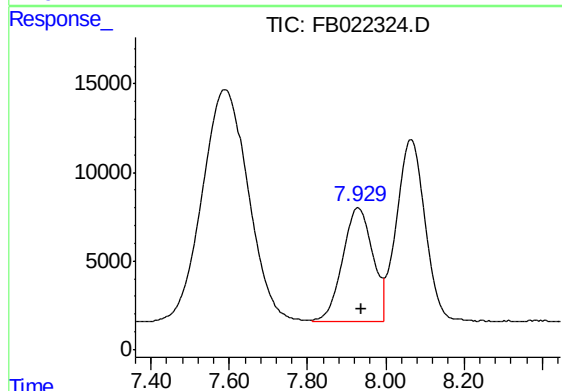


#3 n-Heptane

R.T.: 7.930 min
Delta R.T.: -0.008 min
Response: 347010
Conc: 6.89 ng/ml

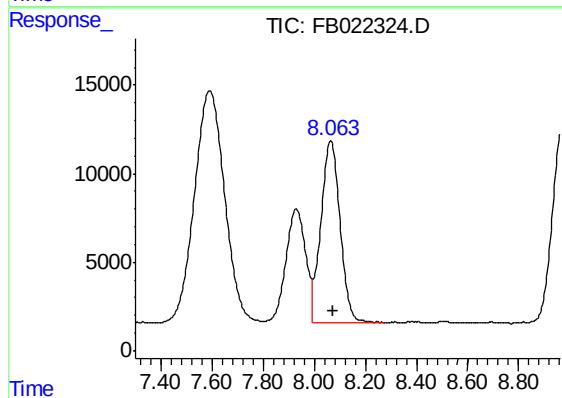

#4 Benzene


R.T.: 8.065 min
Delta R.T.: -0.008 min
Response: 536240
Conc: 9.04 ng/ml

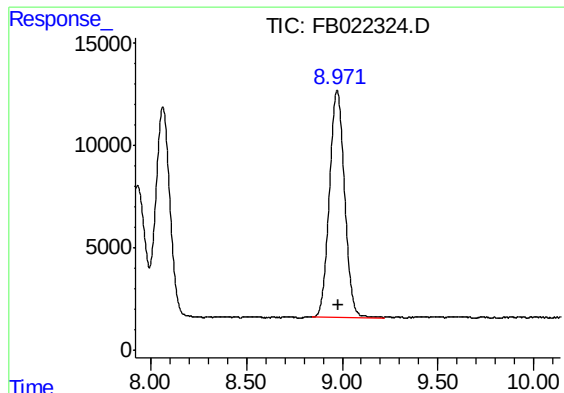

#5 AAA-TFT


R.T.: 8.972 min
Delta R.T.: -0.007 min
Response: 610314
Conc: 20.98 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-090519MS

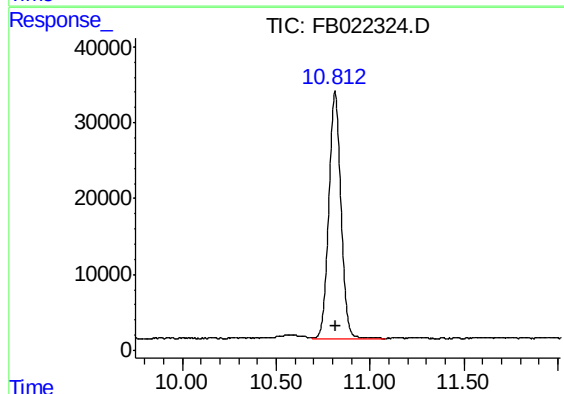


#6 Toluene

R.T.: 10.813 min
Delta R.T.: -0.006 min
Response: 1490024
Conc: 31.32 ng/ml

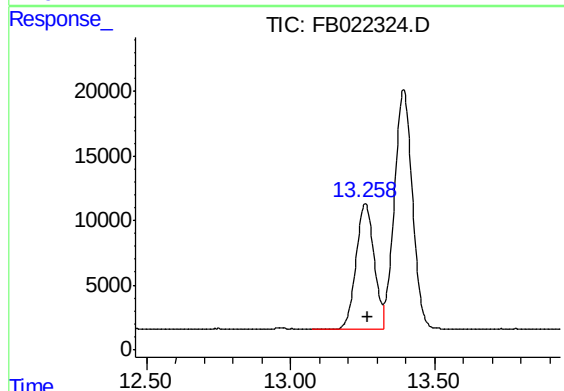


#7 Ethylbenzene

R.T.: 13.259 min
Delta R.T.: -0.006 min
Response: 425055
Conc: 14.18 ng/ml

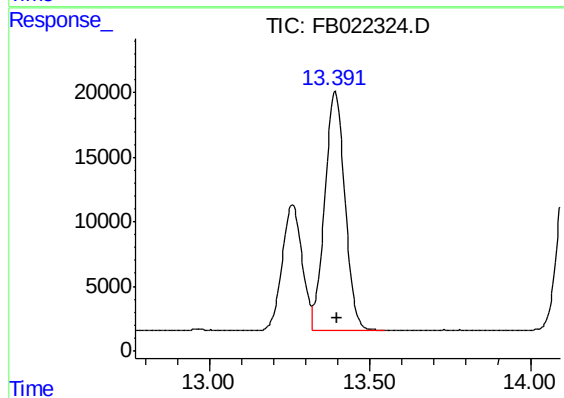

#8 m-Xylene


R.T.: 13.392 min
Delta R.T.: -0.006 min
Response: 812625
Conc: 30.59 ng/ml

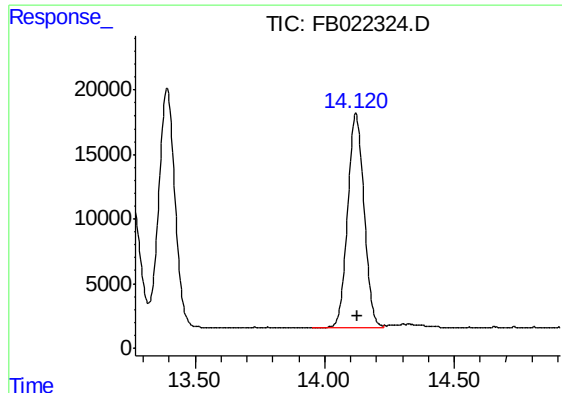

#9 O-Xylene

R.T.: 14.121 min
Delta R.T.: -0.007 min
Response: 728554
Conc: 30.03 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-090519MS

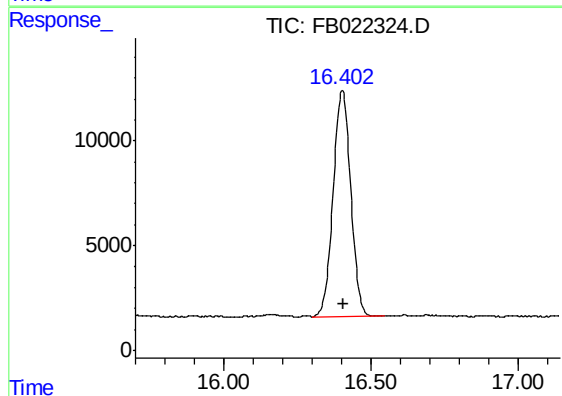

#10 1,2,4-Trimethylbenzene

R.T.: 16.403 min
Delta R.T.: -0.004 min
Response: 449625
Conc: 17.25 ng/ml