

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090619\
 Data File : FB022325.D
 Signal(s) : FID2B.CH
 Acq On : 6 Sep 2019 13:33
 Operator : DD/AJ
 Sample : K4656-02MSD
 Misc : 5.05g/5.00ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AU-06-090519MSD

Integration File: Calibration.e
 Quant Time: Sep 06 22:58:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.972	593970	20.420 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.838	984642	20.040 ng/ml
2) t 2,2,4-Trimethylpentane	7.589	1049782	20.330 ng/ml
3) t n-Heptane	7.930	339959	6.755 ng/ml
4) t Benzene	8.064	525630	8.857 ng/ml
6) t Toluene	10.813	1463580	30.765 ng/ml
7) t Ethylbenzene	13.260	412682	13.766 ng/ml
8) t m-Xylene	13.393	799378	30.090 ng/ml
9) t O-Xylene	14.123	720122	29.684 ng/ml
10) t 1,2,4-Trimethylbenzene	16.404	441879	16.949 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090619\
Data File : FB022325.D
Signal(s) : FID2B.CH
Acq On : 6 Sep 2019 13:33
Operator : DD/AJ
Sample : K4656-02MSD
Misc : 5.05g/5.00ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
AU-06-090519MSD

Integration File: Calibration.e
Quant Time: Sep 06 22:58:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

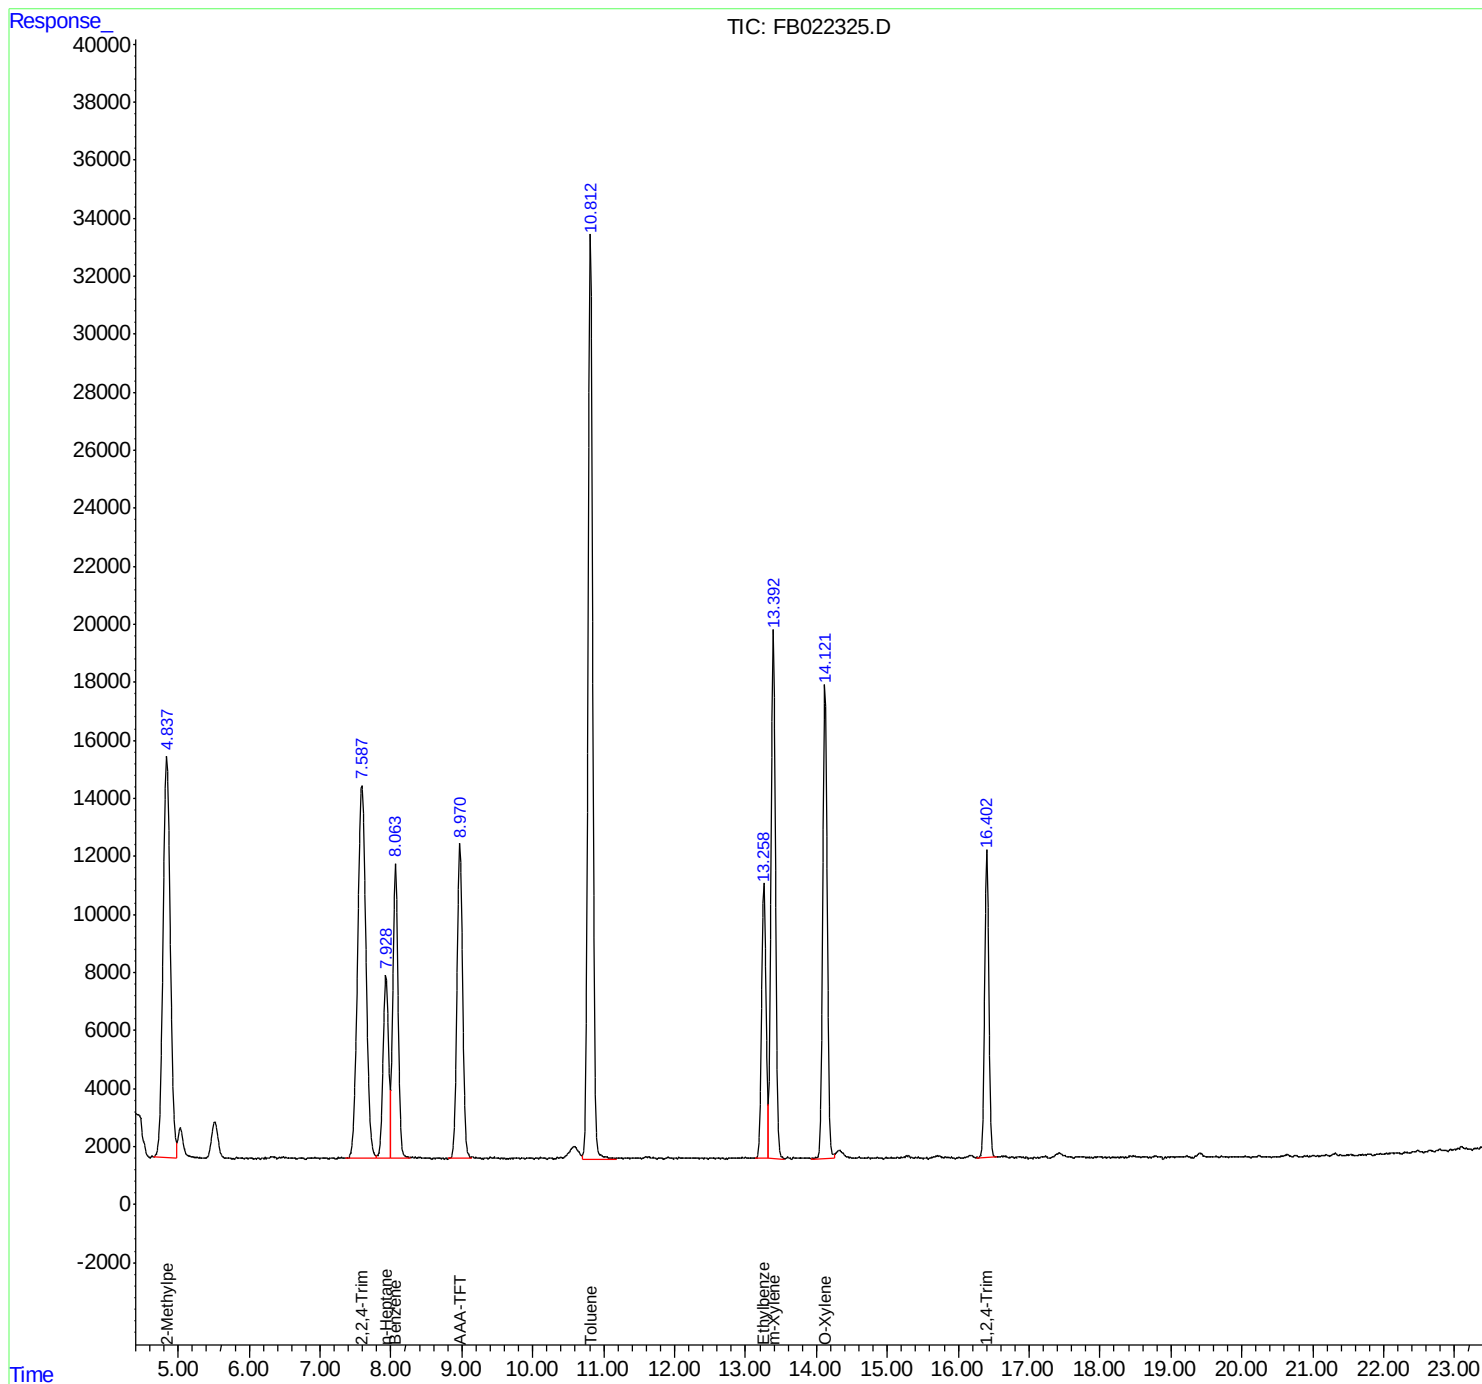


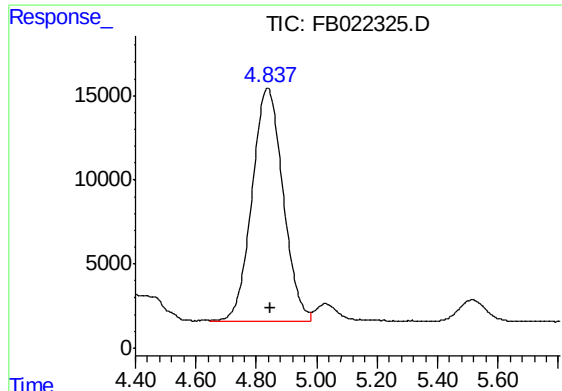

#1 2-Methylpentane


R.T.: 4.838 min
Delta R.T.: -0.009 min
Response: 984642
Conc: 20.04 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-090519MSD

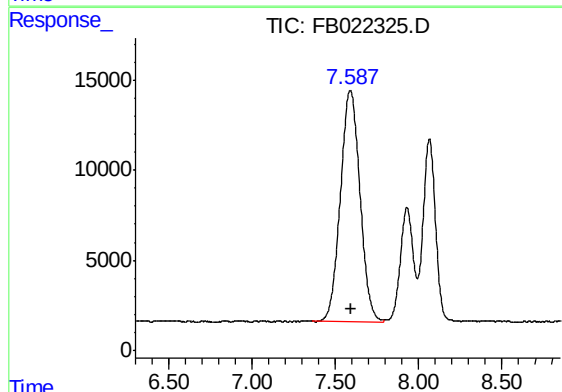


#2 2,2,4-Trimethylpentane

R.T.: 7.589 min
Delta R.T.: -0.008 min
Response: 1049782
Conc: 20.33 ng/ml

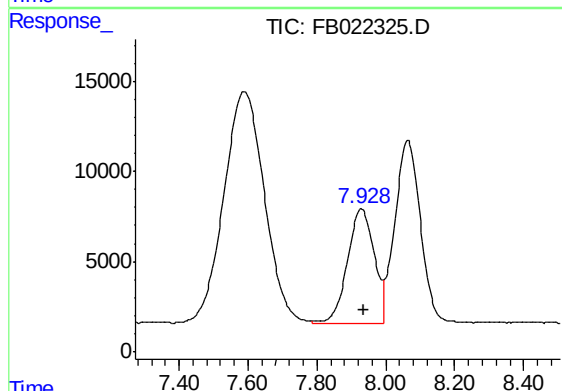


#3 n-Heptane

R.T.: 7.930 min
Delta R.T.: -0.008 min
Response: 339959
Conc: 6.75 ng/ml

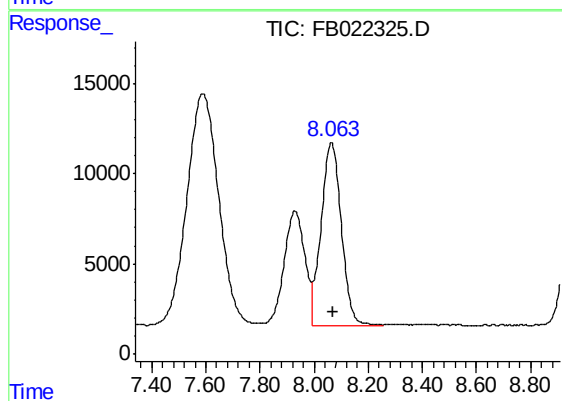

#4 Benzene


R.T.: 8.064 min
Delta R.T.: -0.008 min
Response: 525630
Conc: 8.86 ng/ml

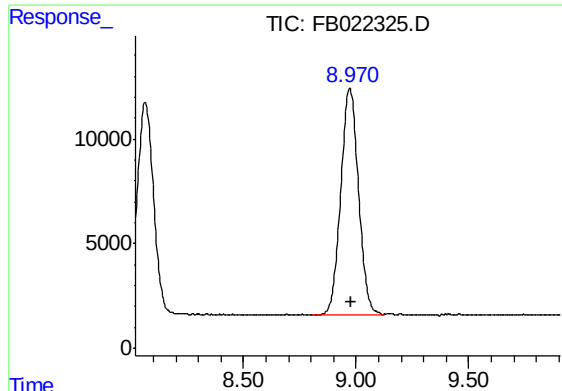

#5 AAA-TFT


R.T.: 8.972 min
Delta R.T.: -0.008 min
Response: 593970
Conc: 20.42 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-090519MSD

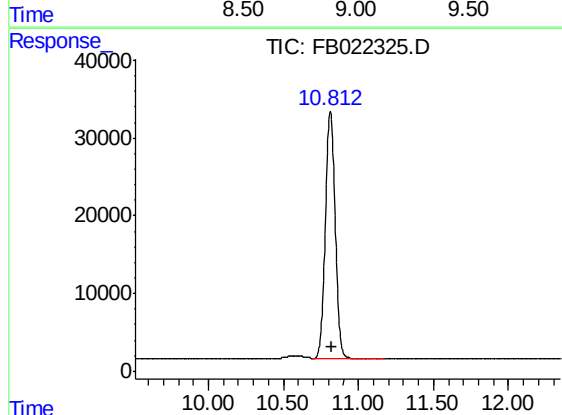


#6 Toluene

R.T.: 10.813 min
Delta R.T.: -0.007 min
Response: 1463580
Conc: 30.76 ng/ml

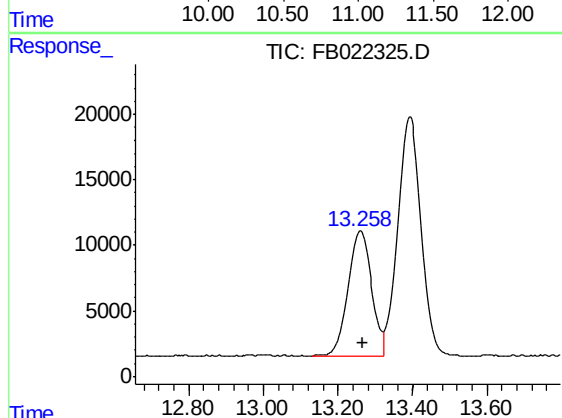


#7 Ethylbenzene

R.T.: 13.260 min
Delta R.T.: -0.005 min
Response: 412682
Conc: 13.77 ng/ml

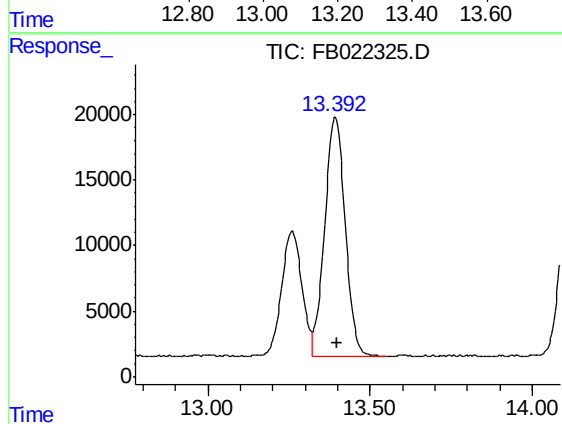

#8 m-Xylene


R.T.: 13.393 min
Delta R.T.: -0.005 min
Response: 799378
Conc: 30.09 ng/ml

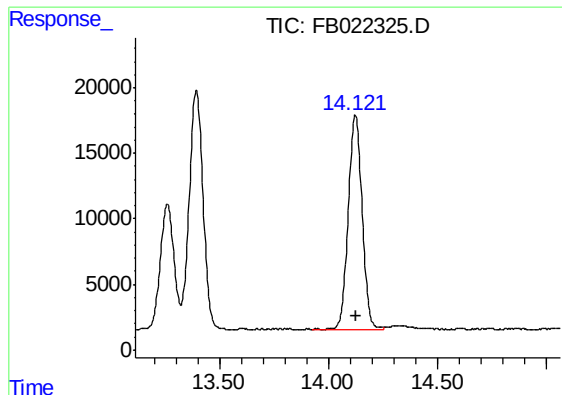

#9 O-Xylene

R.T.: 14.123 min
Delta R.T.: -0.005 min
Response: 720122
Conc: 29.68 ng/ml

Instrument :
FID_B
ClientSampleId :
AU-06-090519MSD

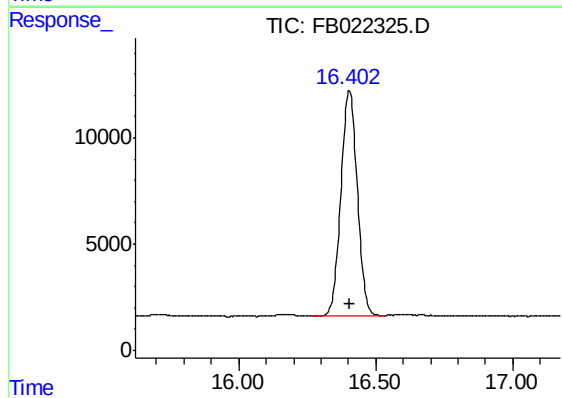

#10 1,2,4-Trimethylbenzene

R.T.: 16.404 min
Delta R.T.: -0.004 min
Response: 441879
Conc: 16.95 ng/ml