

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090622\
 Data File : FB028133.D
 Signal(s) : FID2B.CH
 Acq On : 7 Sep 2022 4:00
 Operator : AJ/MA
 Sample : N4501-02MSD 50X
 Misc : 5.07G/5.00 ML MEOH
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 07 04:50:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	277224	23.921 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	376377	20.805 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	442365	22.558 ng/ml
3) t n-Heptane	7.752	132267	6.866 ng/ml
4) t Benzene	7.890	193545	8.324 ng/ml
6) t Toluene	10.624	541198	24.681 ng/ml
7) t Ethylbenzene	13.060	171142	8.305 ng/ml
8) t m-Xylene	13.193	334274	16.336 ng/ml
9) t O-Xylene	13.920	325140	16.414 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	308037	15.796 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090622\
Data File : FB028133.D
Signal(s) : FID2B.CH
Acq On : 7 Sep 2022 4:00
Operator : AJ/MA
Sample : N4501-02MSD 50X
Misc : 5.07G/5.00 ML MEOH
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 07 04:50:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

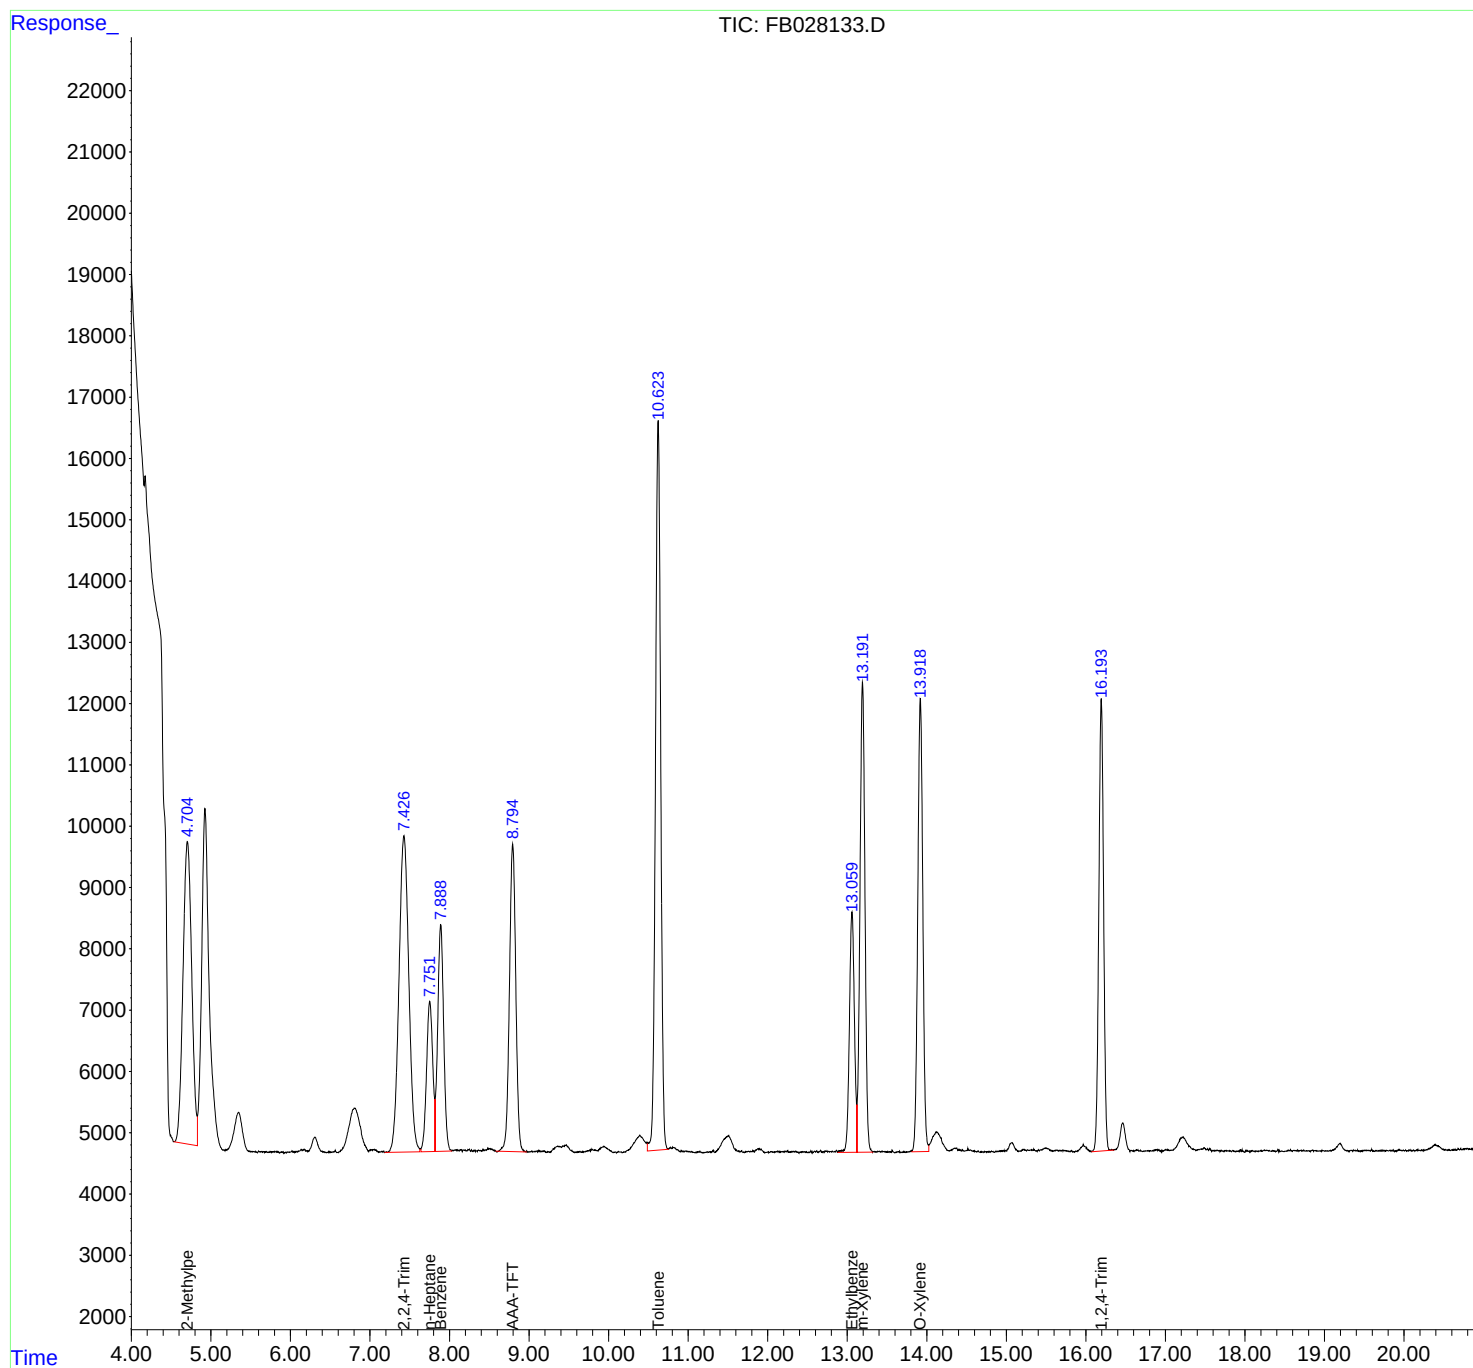


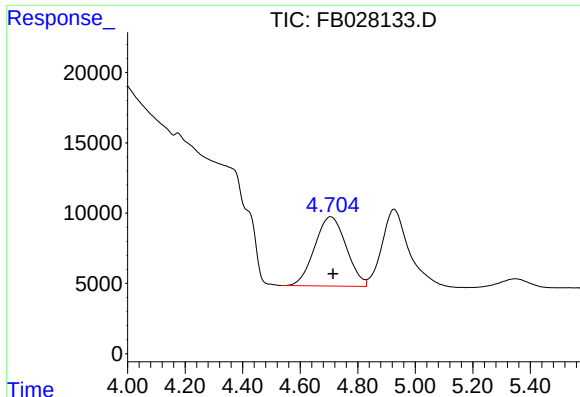

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.010 min
Response: 376377
Conc: 20.80 ng/ml

Instrument :
FID_B
ClientSampleId :

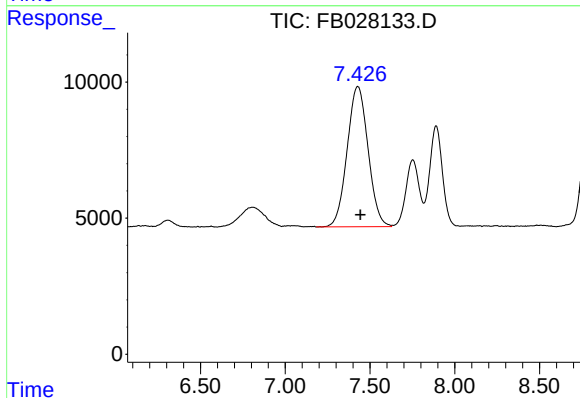


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: -0.016 min
Response: 442365
Conc: 22.56 ng/ml

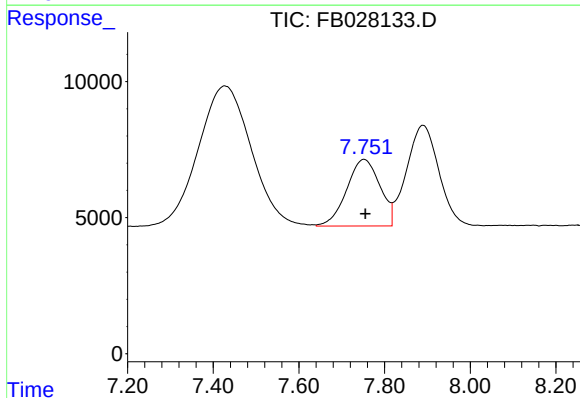


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.003 min
Response: 132267
Conc: 6.87 ng/ml

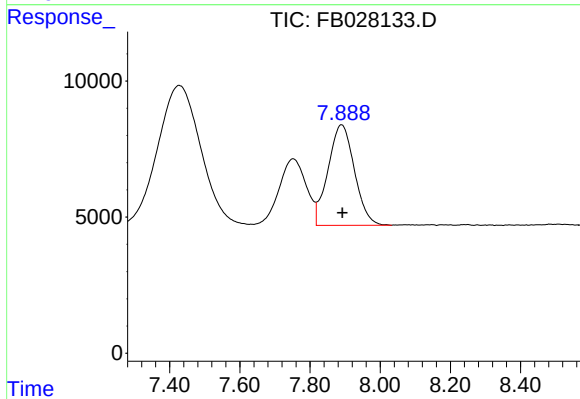

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 193545
Conc: 8.32 ng/ml

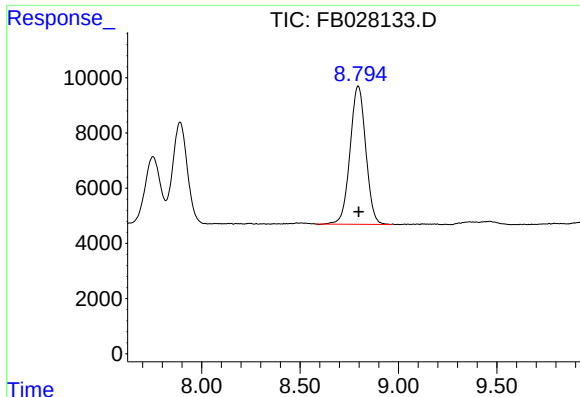

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.003 min
Response: 277224
Conc: 23.92 ng/ml

Instrument :
FID_B
ClientSampleId :

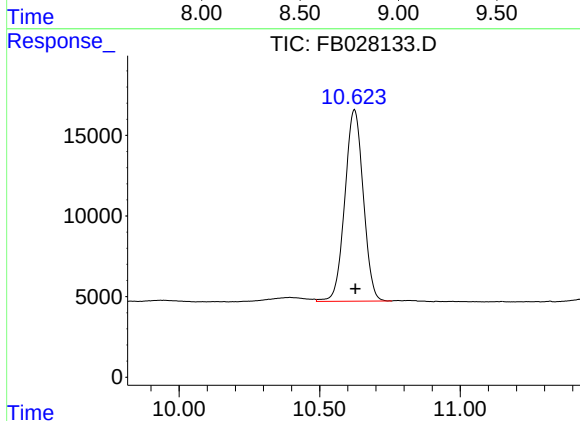


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.003 min
Response: 541198
Conc: 24.68 ng/ml

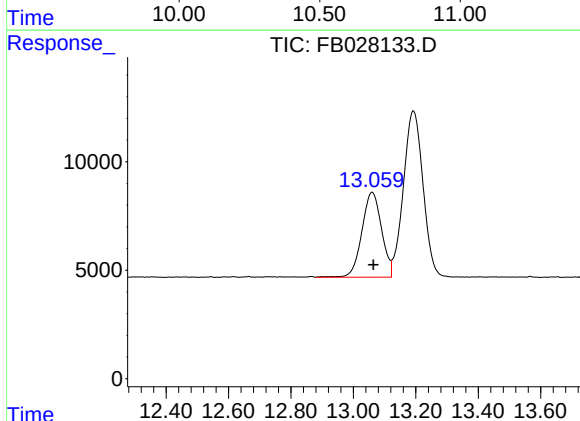


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: -0.004 min
Response: 171142
Conc: 8.31 ng/ml

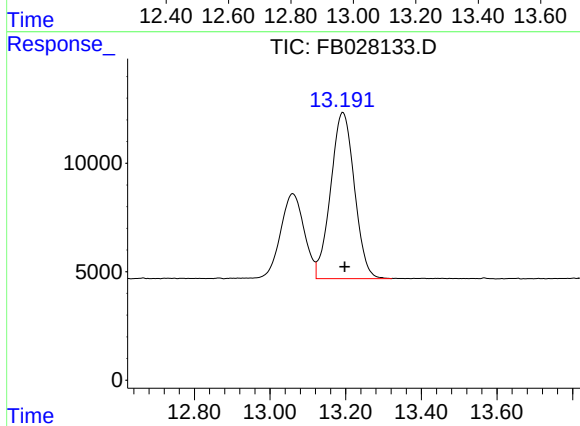

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: -0.004 min
Response: 334274
Conc: 16.34 ng/ml

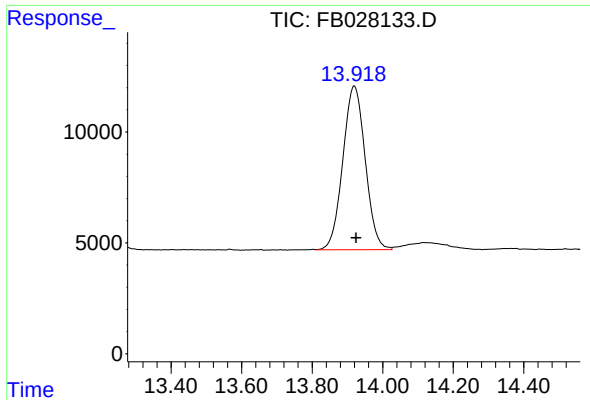

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: -0.005 min
Response: 325140
Conc: 16.41 ng/ml

Instrument :
FID_B
ClientSampleId :

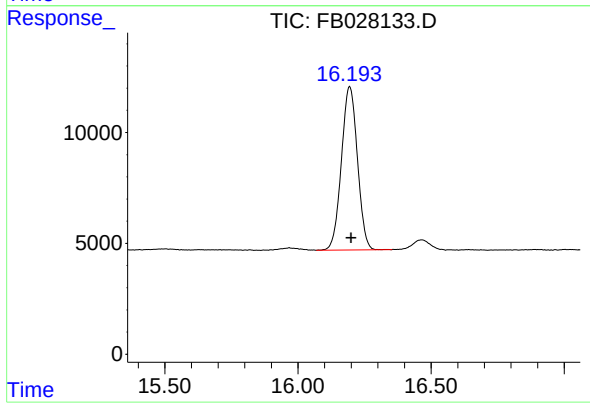

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.005 min
Response: 308037
Conc: 15.80 ng/ml