

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090622\
 Data File : FB028112.D
 Signal(s) : FID2B.CH
 Acq On : 6 Sep 2022 12:21
 Operator : AJ/MA
 Sample : BSF0906S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0906S1

Integration File: Calibration.e
 Quant Time: Sep 07 04:48:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	187508	16.179 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.720	400000	22.111 ng/ml
2) t 2,2,4-Trimethylpentane	7.436	506417	25.824 ng/ml
3) t n-Heptane	7.757	131114	6.806 ng/ml
4) t Benzene	7.893	177020	7.613 ng/ml
6) t Toluene	10.628	526178	23.996 ng/ml
7) t Ethylbenzene	13.064	169072	8.205 ng/ml
8) t m-Xylene	13.197	341206	16.675 ng/ml
9) t O-Xylene	13.923	344211	17.376 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	366192	18.778 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090622\
Data File : FB028112.D
Signal(s) : FID2B.CH
Acq On : 6 Sep 2022 12:21
Operator : AJ/MA
Sample : BSF0906S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0906S1

Integration File: Calibration.e
Quant Time: Sep 07 04:48:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

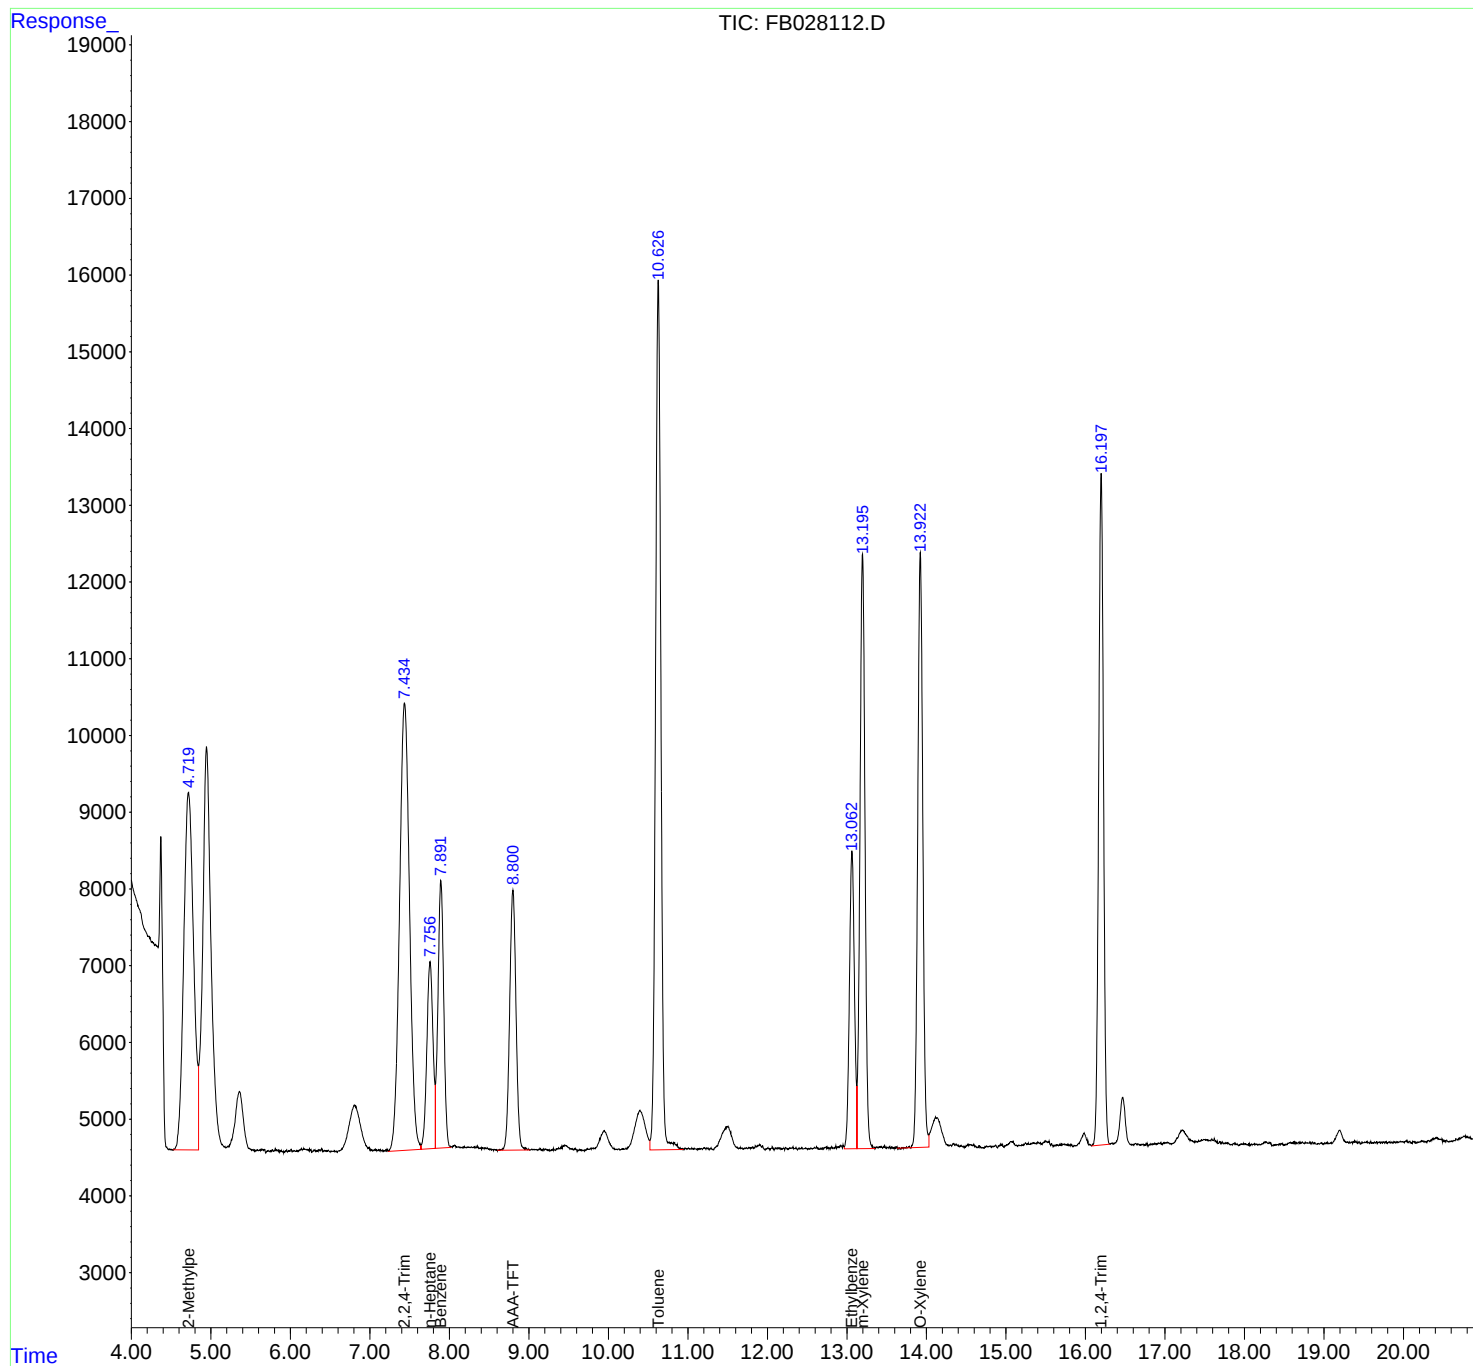


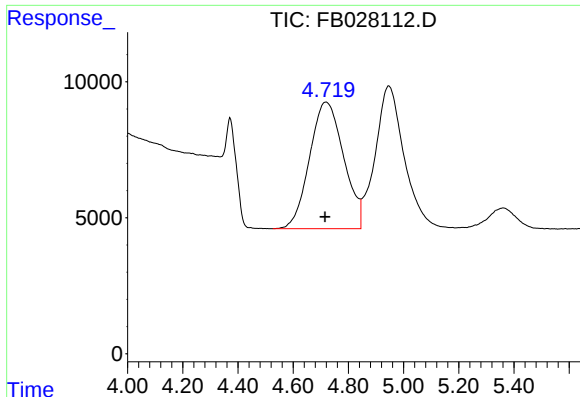

#1 2-Methylpentane


R.T.: 4.720 min
Delta R.T.: 0.005 min
Response: 400000
Conc: 22.11 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0906S1

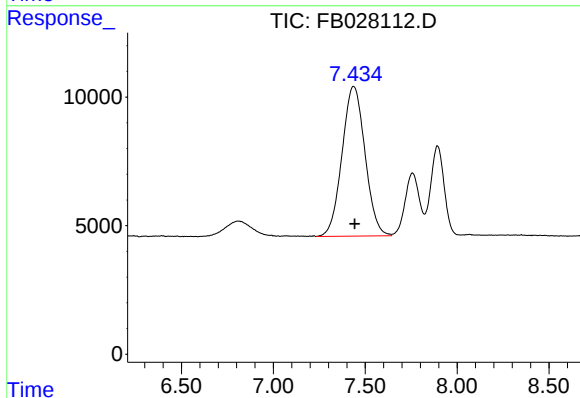


#2 2,2,4-Trimethylpentane

R.T.: 7.436 min
Delta R.T.: -0.007 min
Response: 506417
Conc: 25.82 ng/ml

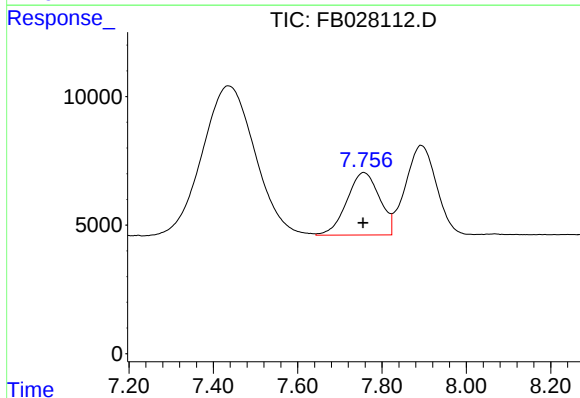


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.002 min
Response: 131114
Conc: 6.81 ng/ml

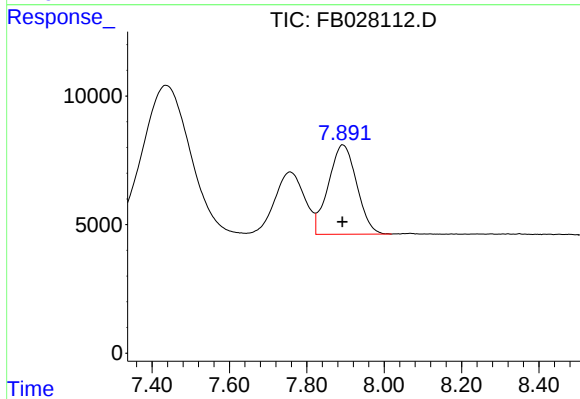

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.001 min
Response: 177020
Conc: 7.61 ng/ml

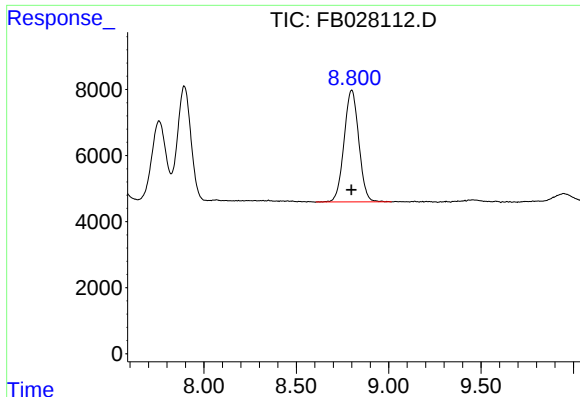

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.002 min
Response: 187508
Conc: 16.18 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0906S1

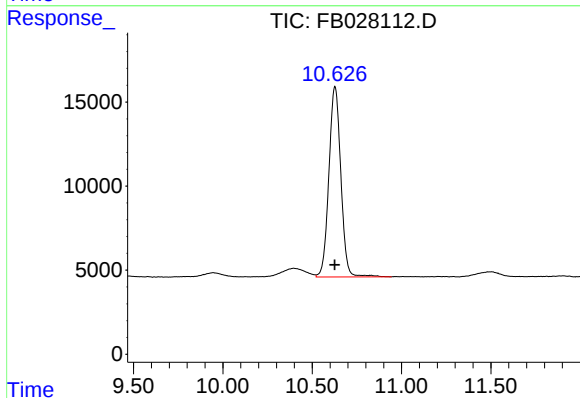


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 526178
Conc: 24.00 ng/ml

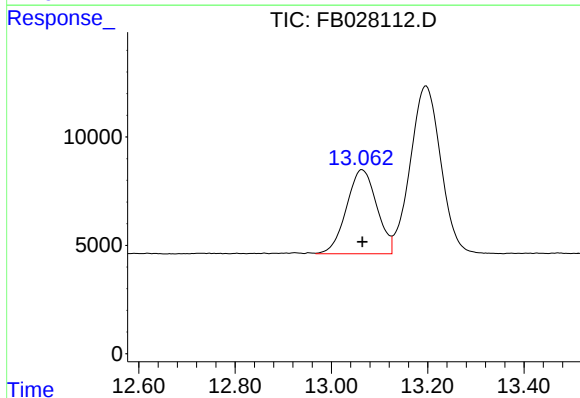


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.000 min
Response: 169072
Conc: 8.20 ng/ml

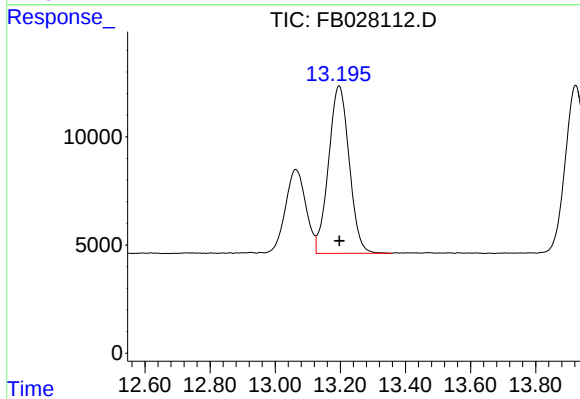

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.000 min
Response: 341206
Conc: 16.67 ng/ml

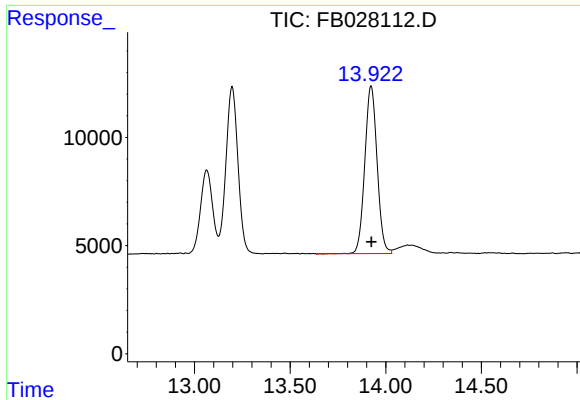

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.000 min
Response: 344211
Conc: 17.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0906S1

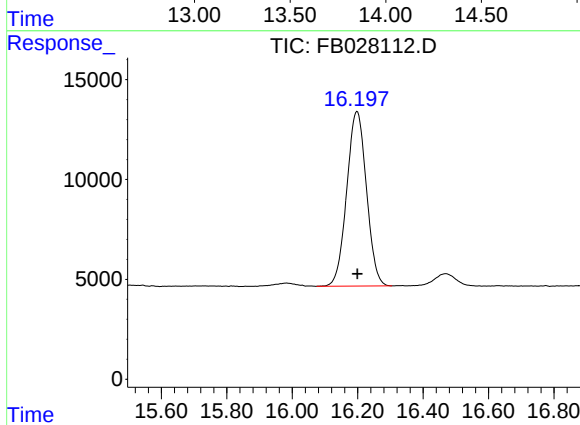

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: -0.001 min
Response: 366192
Conc: 18.78 ng/ml