

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090622\
 Data File : FB028132.D
 Signal(s) : FID2B.CH
 Acq On : 7 Sep 2022 3:23
 Operator : AJ/MA
 Sample : N4501-02MS 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-07-COMPMS

Integration File: Calibration.e
 Quant Time: Sep 07 05:10:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	166416	14.359 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	268216	14.826 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	330264	16.841 ng/ml
3) t n-Heptane	7.754	88880	4.613 ng/ml
4) t Benzene	7.892	130826	5.627 ng/ml
6) t Toluene	10.625	370878	16.913 ng/ml
7) t Ethylbenzene	13.061	118233	5.738 ng/ml
8) t m-Xylene	13.194	233563	11.414 ng/ml
9) t O-Xylene	13.921	236913	11.960 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	238392	12.225 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090622\
Data File : FB028132.D
Signal(s) : FID2B.CH
Acq On : 7 Sep 2022 3:23
Operator : AJ/MA
Sample : N4501-02MS 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMS

Integration File: Calibration.e
Quant Time: Sep 07 05:10:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

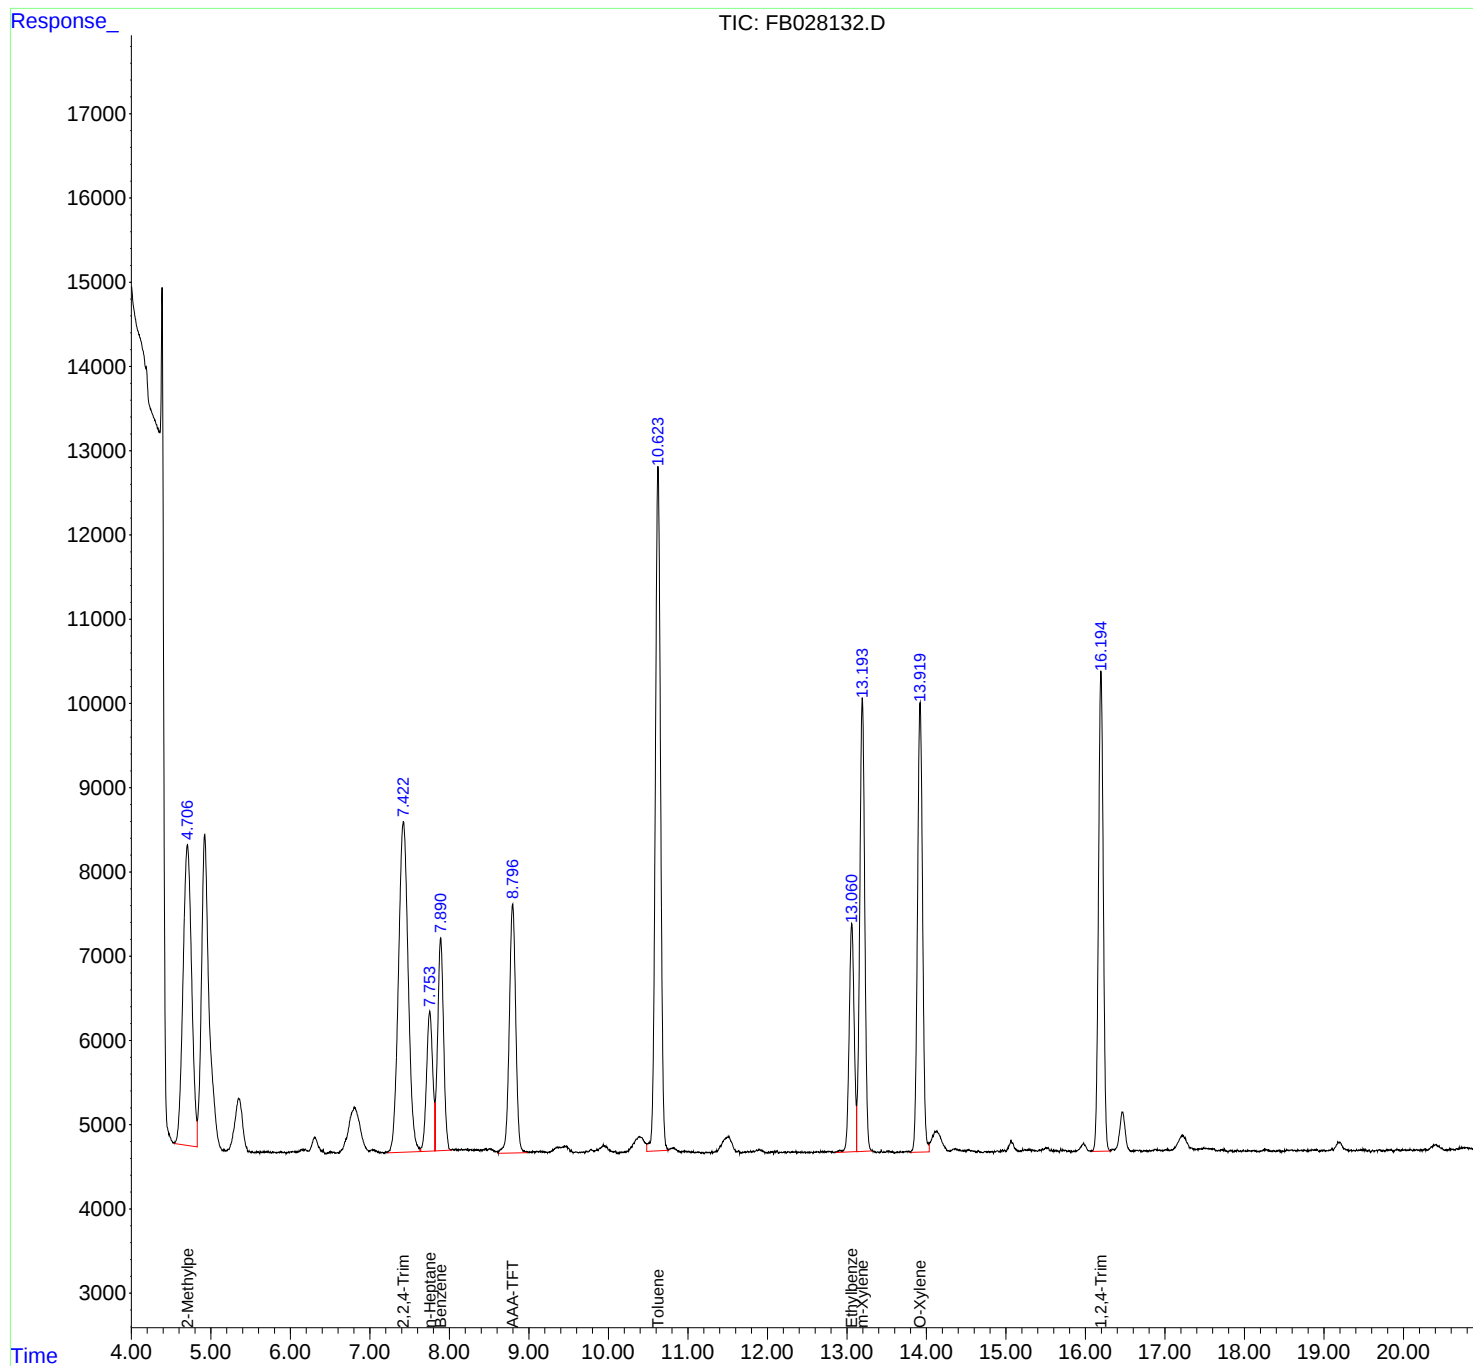


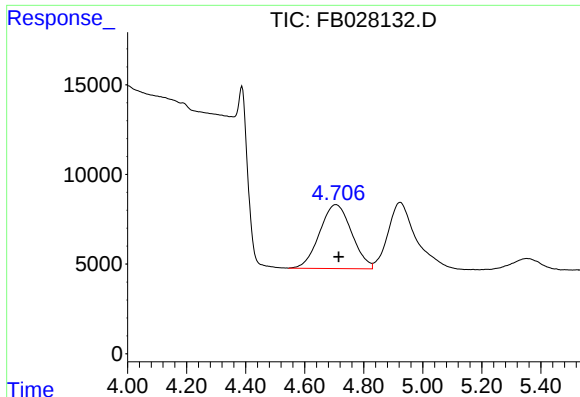

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: -0.008 min
Response: 268216
Conc: 14.83 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMS

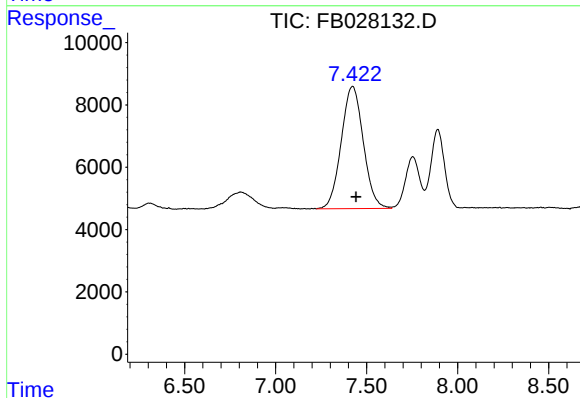


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: -0.019 min
Response: 330264
Conc: 16.84 ng/ml

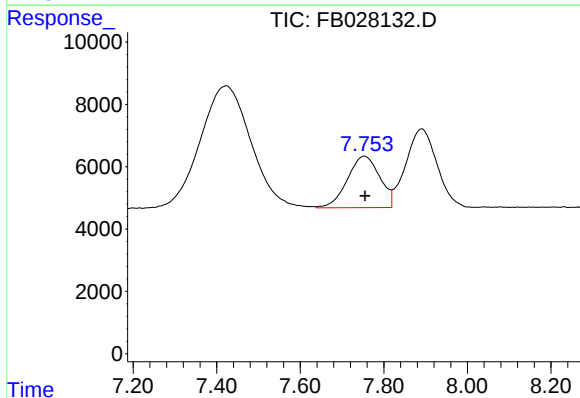


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.000 min
Response: 88880
Conc: 4.61 ng/ml

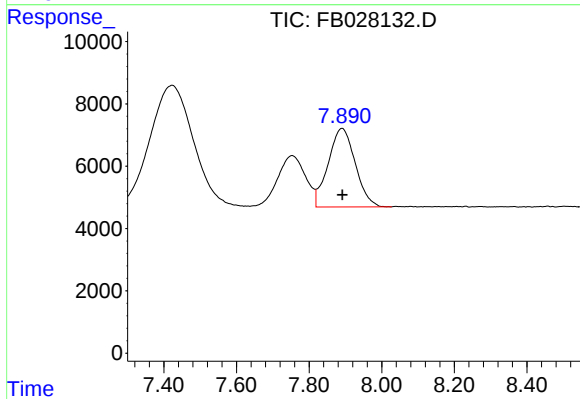

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 130826
Conc: 5.63 ng/ml

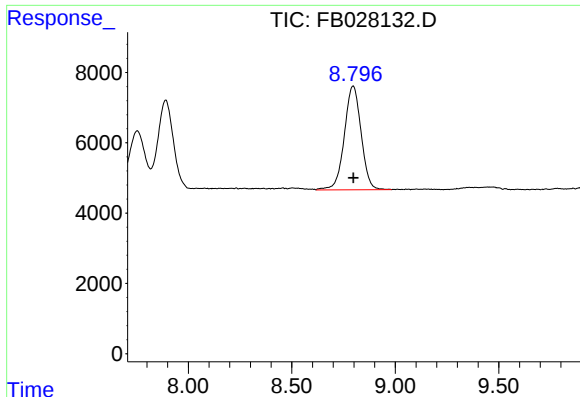

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 166416
Conc: 14.36 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMS

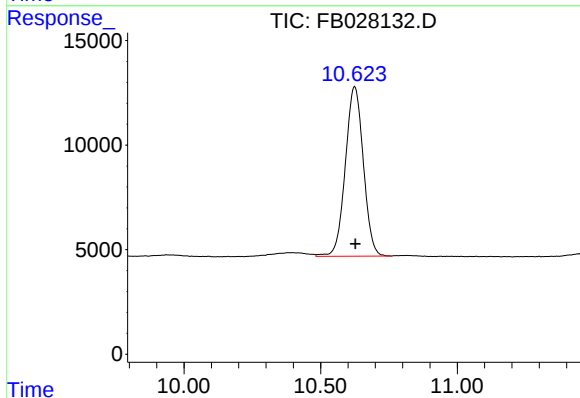


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.003 min
Response: 370878
Conc: 16.91 ng/ml

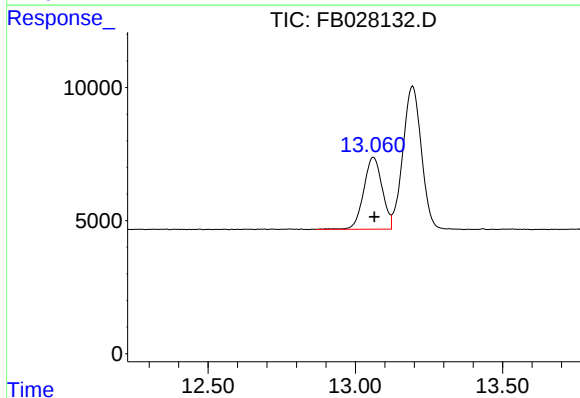


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: -0.003 min
Response: 118233
Conc: 5.74 ng/ml

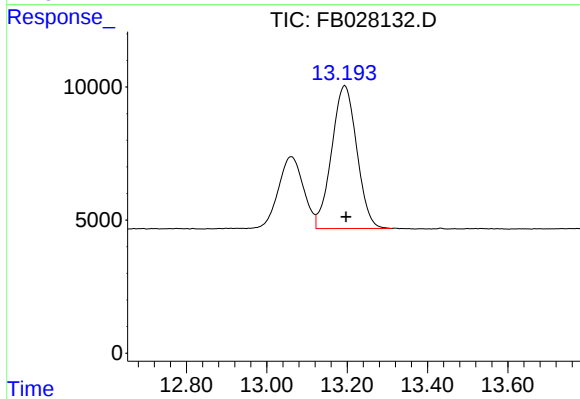

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: -0.003 min
Response: 233563
Conc: 11.41 ng/ml

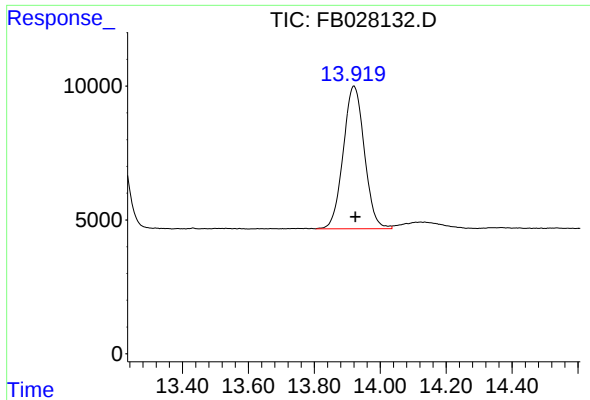

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: -0.004 min
Response: 236913
Conc: 11.96 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMS

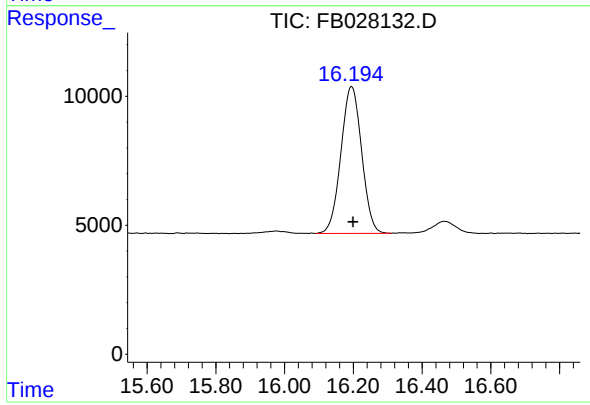

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.004 min
Response: 238392
Conc: 12.22 ng/ml