

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090623\
 Data File : FB030318.D
 Signal(s) : FID2B.CH
 Acq On : 6 Sep 2023 14:55
 Operator : YP/AJ
 Sample : 04299-06
 Misc : 5.08G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 07 01:13:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082223.M
 Quant Title :
 QLast Update : Tue Aug 22 18:06:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	157279	13.215 ng/ml
Target Compounds			
4) t Benzene	7.892	29031	1.169 ng/ml
6) t Toluene	10.628	20038	0.836 ng/ml
7) t Ethylbenzene	13.065	6231	0.278 ng/ml
8) t m-Xylene	13.189	5692	0.255 ng/ml
9) t O-Xylene	13.931	10047	0.471 ng/ml
10) t 1,2,4-Trimethylbenzene	16.233	22965	1.084 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090623\
Data File : FB030318.D
Signal(s) : FID2B.CH
Acq On : 6 Sep 2023 14:55
Operator : YP/AJ
Sample : 04299-06
Misc : 5.08G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 07 01:13:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082223.M
Quant Title :
QLast Update : Tue Aug 22 18:06:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

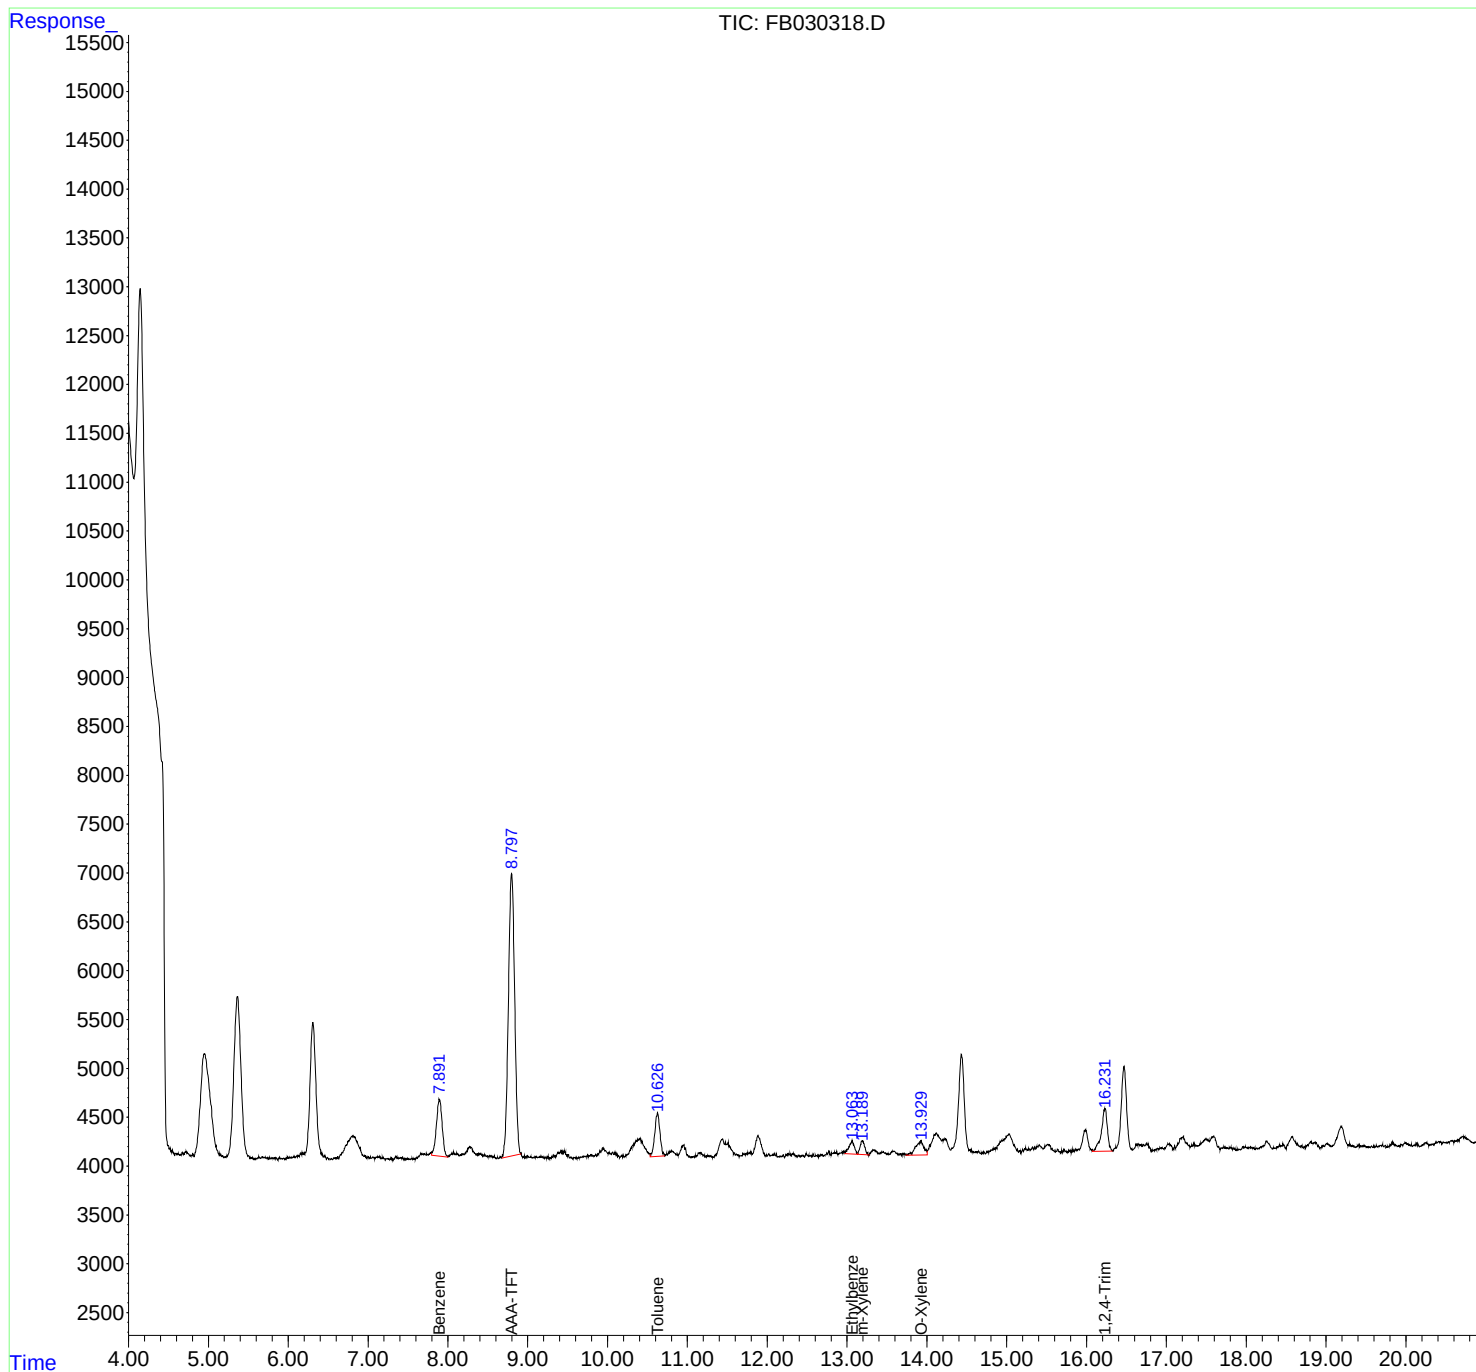


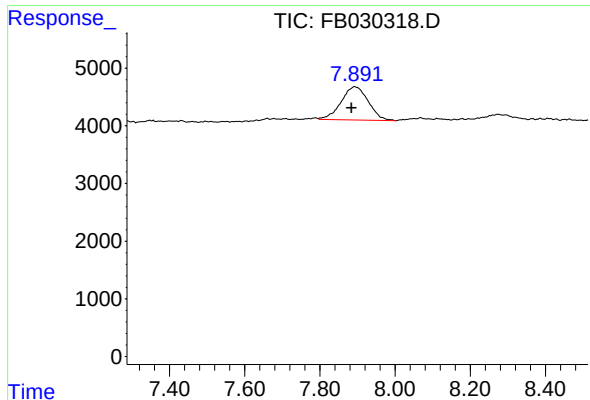

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.008 min
Response: 29031
Conc: 1.17 ng/ml

Instrument :
FID_B
ClientSampleId :

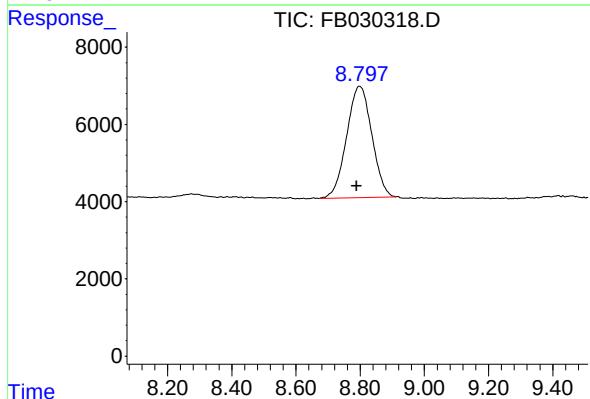


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.009 min
Response: 157279
Conc: 13.22 ng/ml

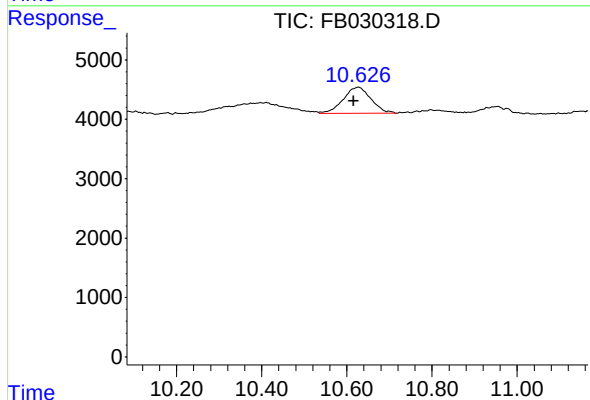


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.011 min
Response: 20038
Conc: 0.84 ng/ml

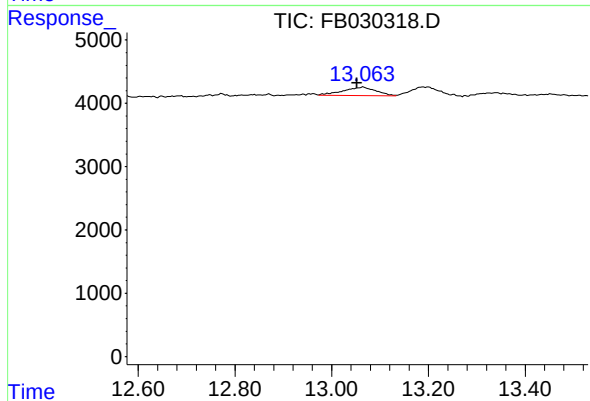

#7 Ethylbenzene


R.T.: 13.065 min
Delta R.T.: 0.013 min
Response: 6231
Conc: 0.28 ng/ml

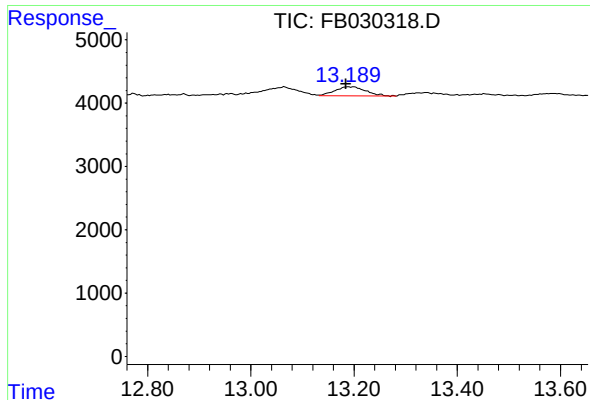

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.005 min
Response: 5692
Conc: 0.26 ng/ml

Instrument :
FID_B
ClientSampleId :

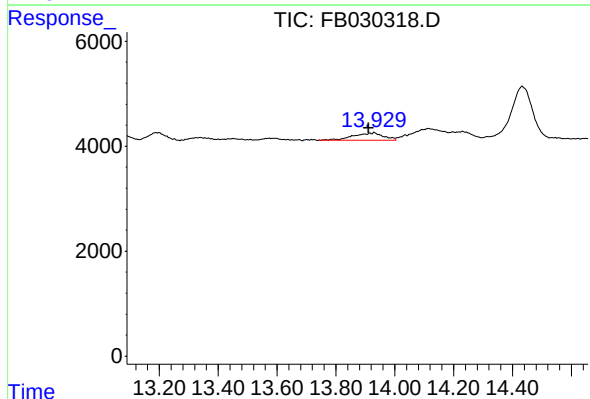

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.020 min
Response: 10047
Conc: 0.47 ng/ml

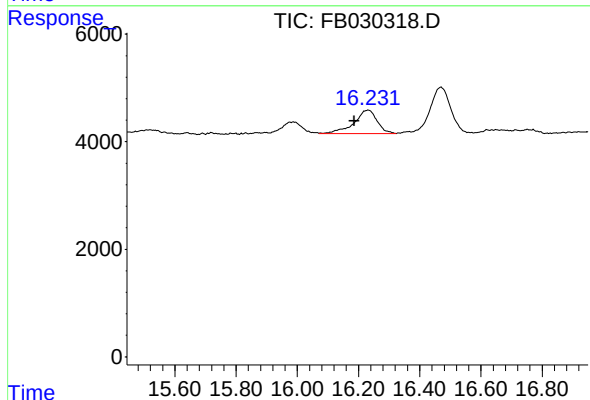

#10 1,2,4-Trimethylbenzene

R.T.: 16.233 min
Delta R.T.: 0.047 min
Response: 22965
Conc: 1.08 ng/ml