

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090623\
 Data File : FB030327.D
 Signal(s) : FID2B.CH
 Acq On : 6 Sep 2023 21:35
 Operator : YP/AJ
 Sample : 04299-08 50X
 Misc : 5.08G/5.00 ML MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 07 01:13:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082223.M
 Quant Title :
 QLast Update : Tue Aug 22 18:06:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	192344	16.161 ng/ml
Target Compounds			
4) t Benzene	7.893	283977	11.432 ng/ml
6) t Toluene	10.628	40920	1.706 ng/ml
7) t Ethylbenzene	13.063	960056	42.825 ng/ml
8) t m-Xylene	13.192	909117	40.775 ng/ml
9) t O-Xylene	13.922	605813	28.404 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	624756	29.483 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090623\
Data File : FB030327.D
Signal(s) : FID2B.CH
Acq On : 6 Sep 2023 21:35
Operator : YP/AJ
Sample : 04299-08 50X
Misc : 5.08G/5.00 ML MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 07 01:13:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082223.M
Quant Title :
QLast Update : Tue Aug 22 18:06:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

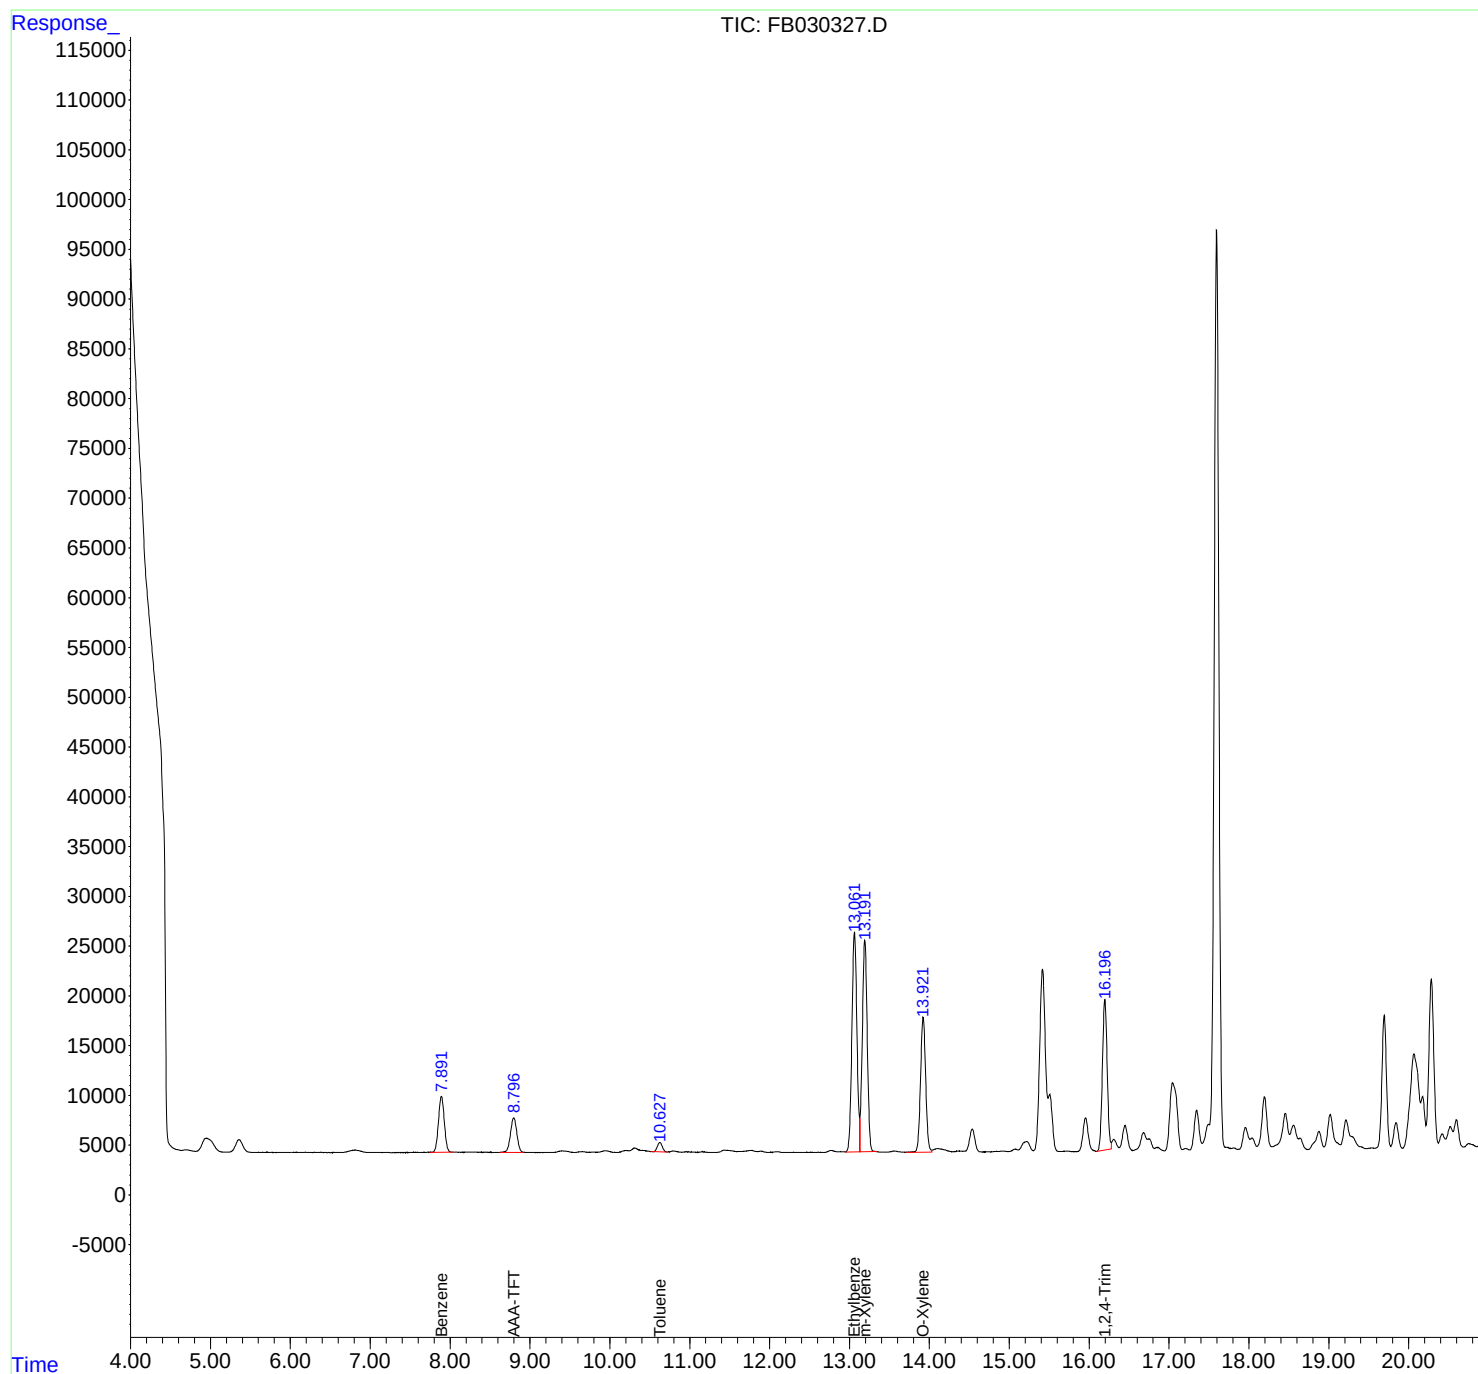


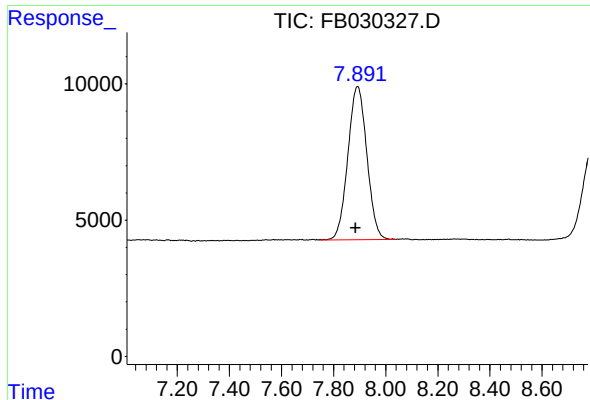

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.008 min
Response: 283977
Conc: 11.43 ng/ml

Instrument : FID_B
ClientSampleId :

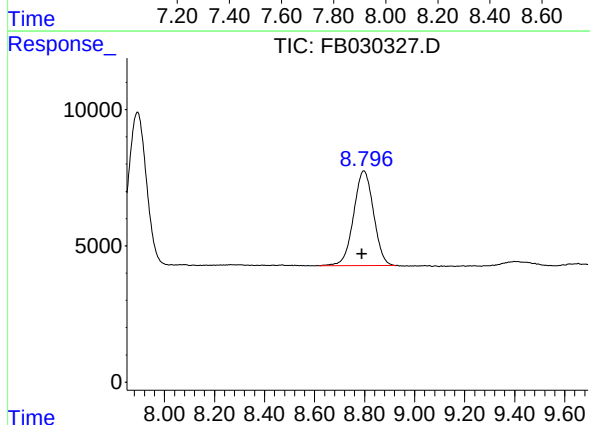


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.009 min
Response: 192344
Conc: 16.16 ng/ml

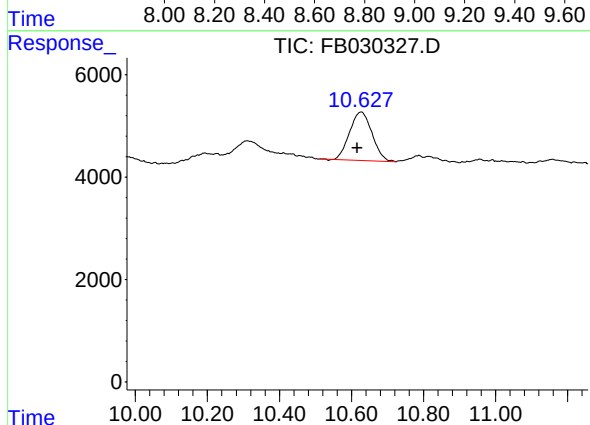


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.012 min
Response: 40920
Conc: 1.71 ng/ml

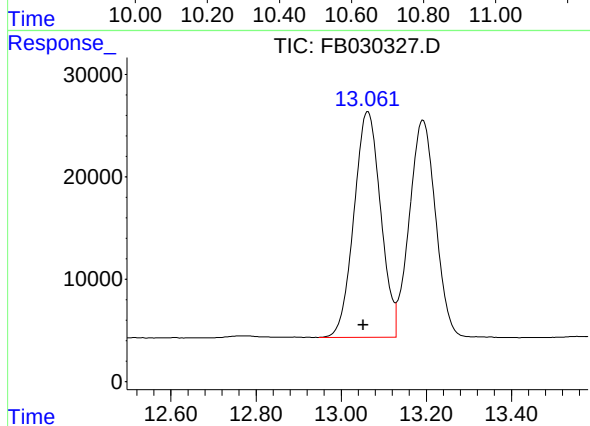

#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.011 min
Response: 960056
Conc: 42.82 ng/ml

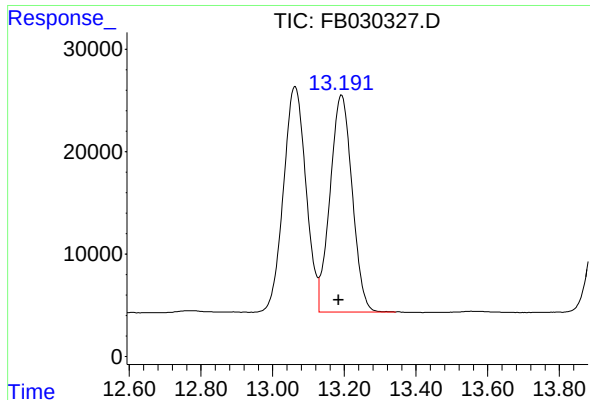


#8 m-Xylene

R.T.: 13.192 min
Delta R.T.: 0.008 min
Response: 909117
Conc: 40.78 ng/ml

Instrument :


FID_B

ClientSampleId :

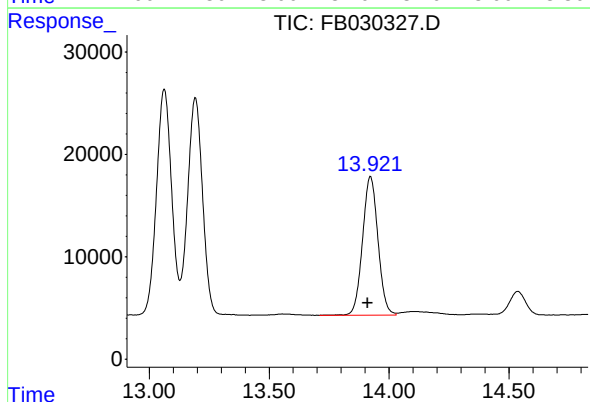

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.011 min
Response: 605813
Conc: 28.40 ng/ml

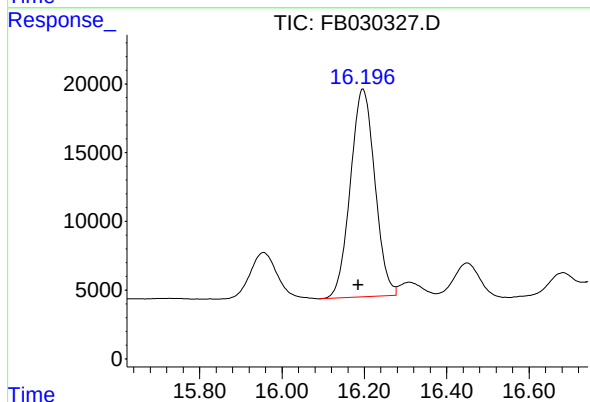

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.011 min
Response: 624756
Conc: 29.48 ng/ml