

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090623\
Data File : FB030320.D
Signal(s) : FID2B.CH
Acq On : 6 Sep 2023 16:15
Operator : YP/AJ
Sample : 04299-02
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-01-COMP

Integration File: Calibration.e
Quant Time: Sep 07 01:13:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082223.M
Quant Title :
QLast Update : Tue Aug 22 18:06:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	866	0.073 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090623\
Data File : FB030320.D
Signal(s) : FID2B.CH
Acq On : 6 Sep 2023 16:15
Operator : YP/AJ
Sample : 04299-02
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-01-COMP

Integration File: Calibration.e
Quant Time: Sep 07 01:13:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082223.M
Quant Title :
QLast Update : Tue Aug 22 18:06:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

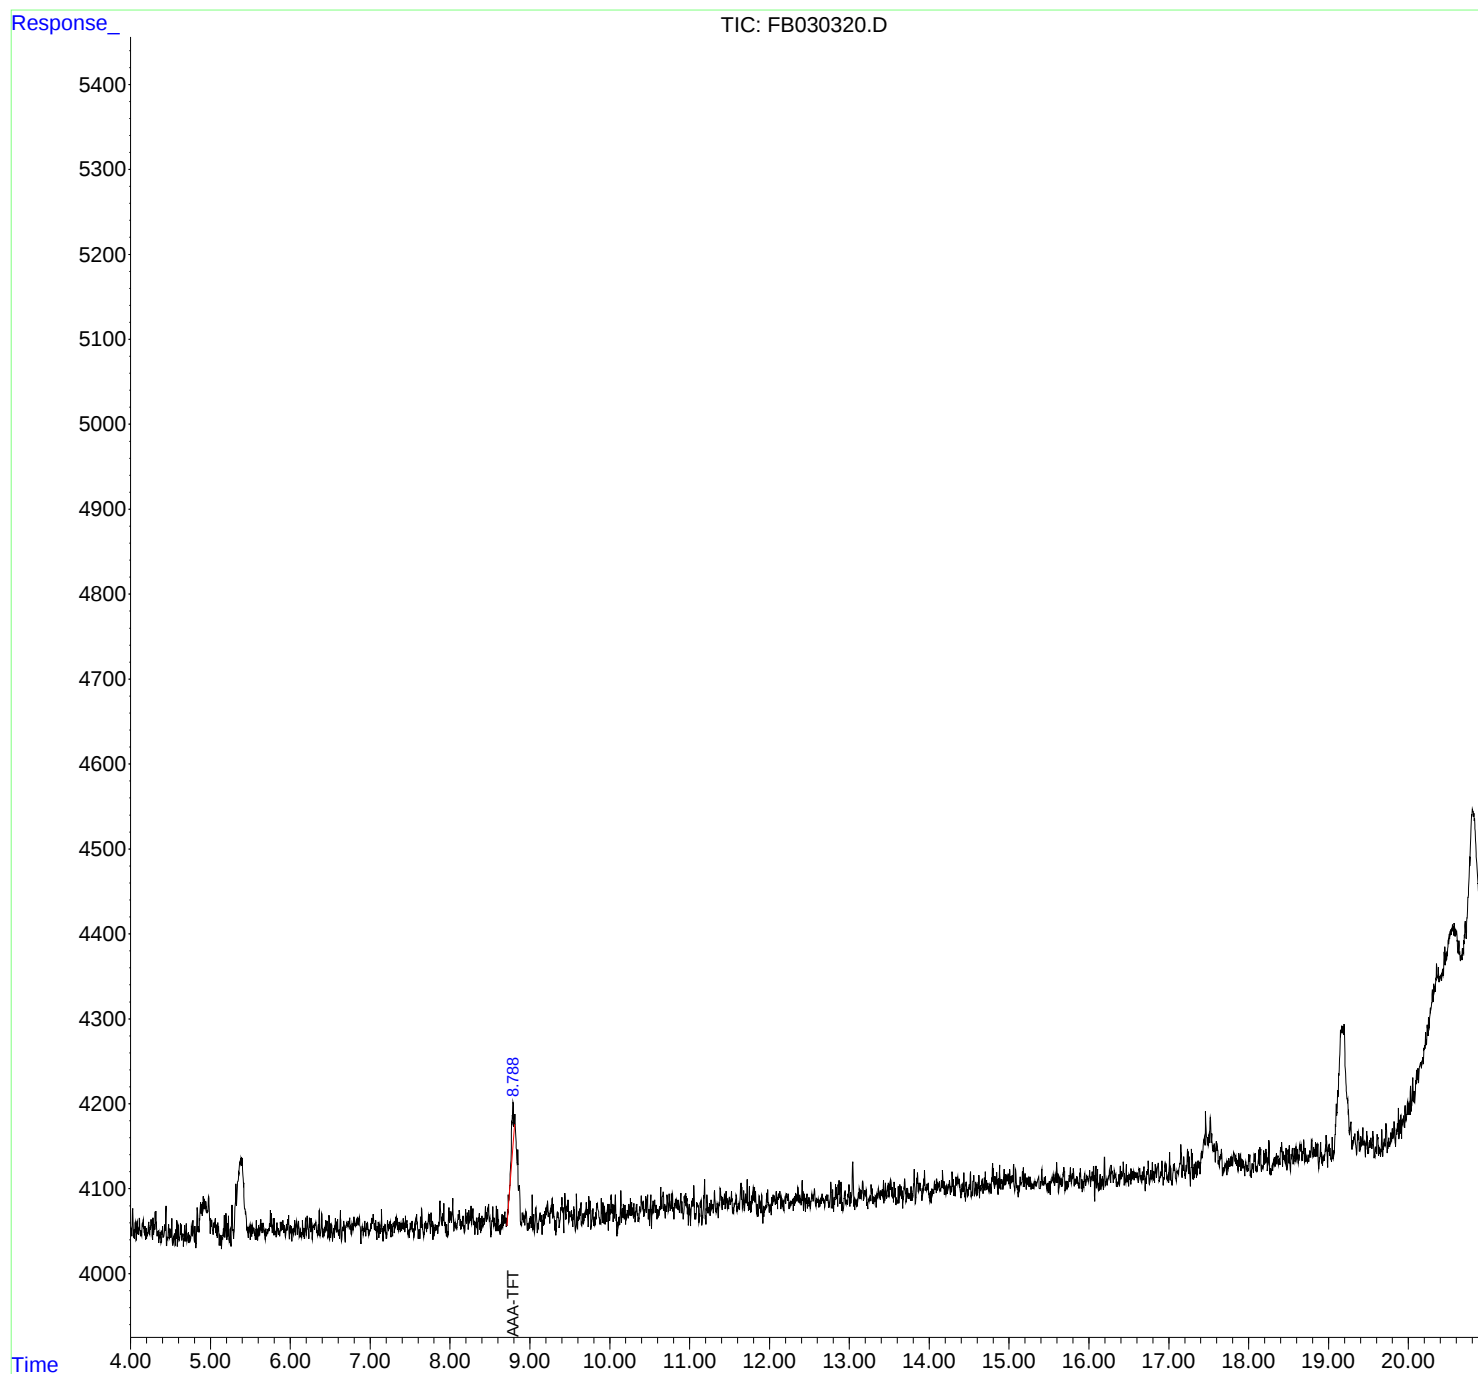

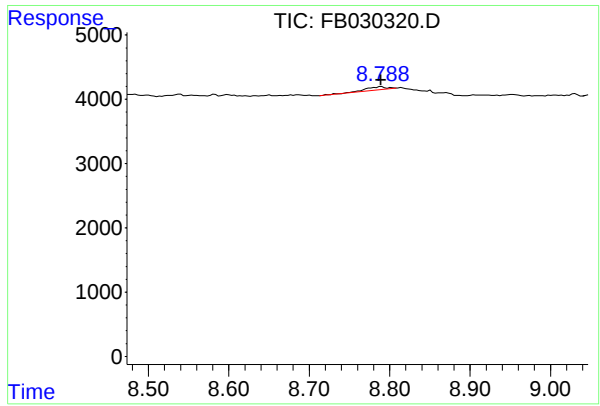

#5 AAA-TFT

R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 866
Conc: 0.07 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-01-COMP