

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090719\
Data File : FB022382.D
Signal(s) : FID2B.CH
Acq On : 7 Sep 2019 23:37
Operator : DD/AJ
Sample : K4636-10
Misc : 5.06g/5.00ML DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 09 00:48:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.972	476406	16.378 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.537	3995	0.077 ng/ml
4) t Benzene	8.070	10163	0.171 ng/ml
6) t Toluene	10.822	18937	0.398 ng/ml
8) t m-Xylene	13.389	19442	0.732 ng/ml
9) t O-Xylene	14.132	7186	0.296 ng/ml
10) t 1,2,4-Trimethylbenzene	16.436	15780	0.605 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090719\
Data File : FB022382.D
Signal(s) : FID2B.CH
Acq On : 7 Sep 2019 23:37
Operator : DD/AJ
Sample : K4636-10
Misc : 5.06g/5.00ML DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 09 00:48:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

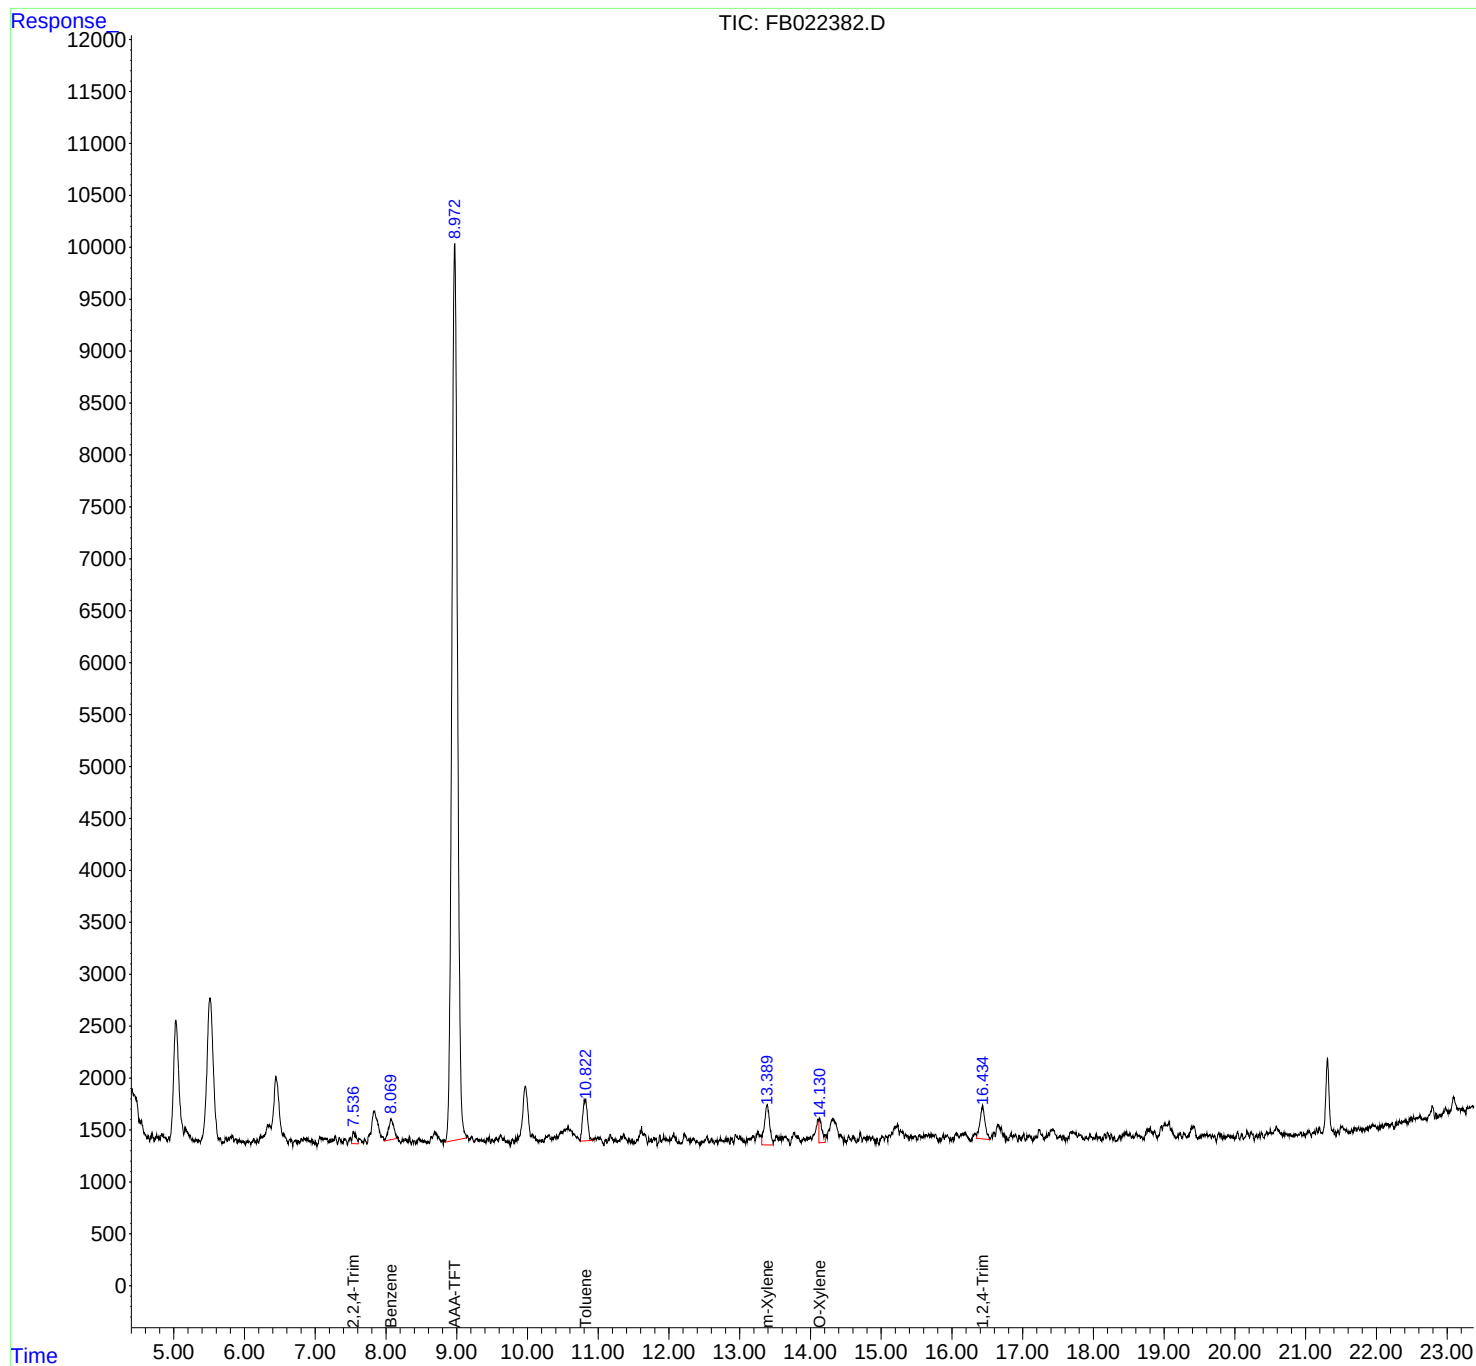


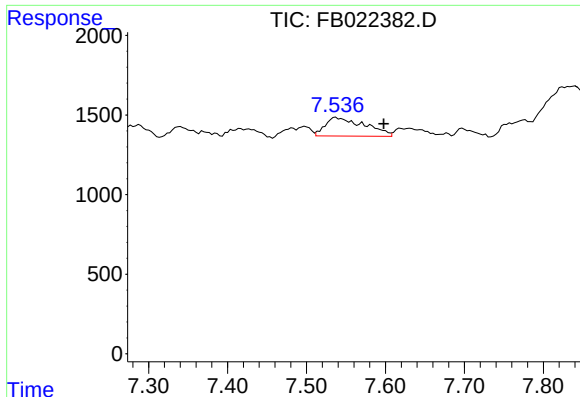

#2 2,2,4-Trimethylpentane


R.T.: 7.537 min
Delta R.T.: -0.060 min
Response: 3995
Conc: 0.08 ng/ml

Instrument :
FID_B
ClientSampleId :

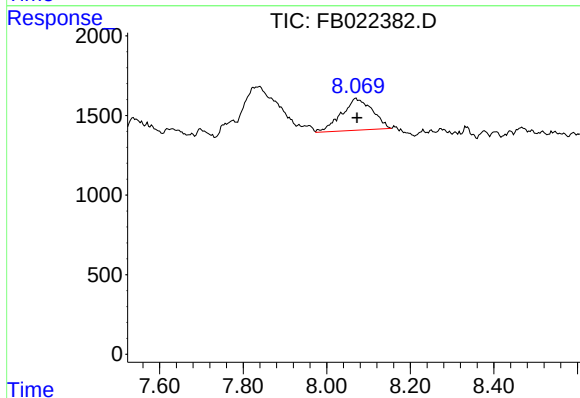


#4 Benzene

R.T.: 8.070 min
Delta R.T.: -0.003 min
Response: 10163
Conc: 0.17 ng/ml

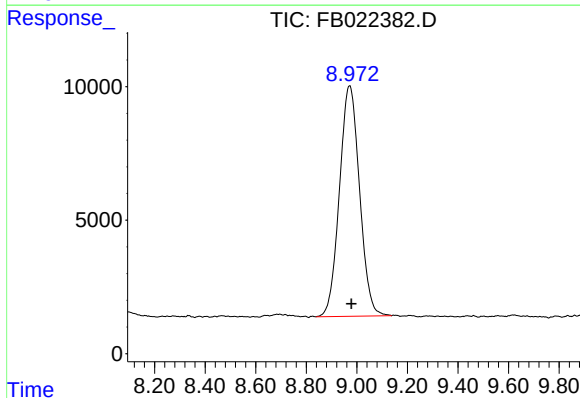


#5 AAA-TFT

R.T.: 8.972 min
Delta R.T.: -0.007 min
Response: 476406
Conc: 16.38 ng/ml

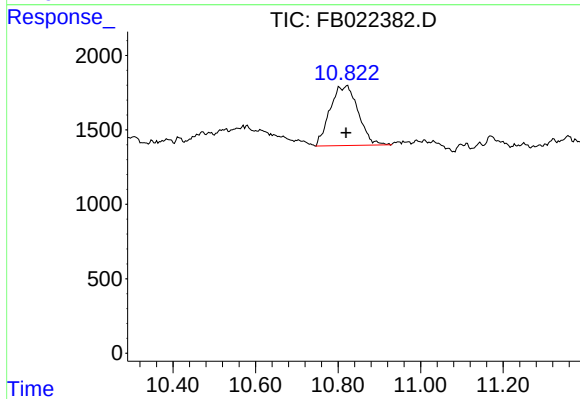

#6 Toluene


R.T.: 10.822 min
Delta R.T.: 0.003 min
Response: 18937
Conc: 0.40 ng/ml

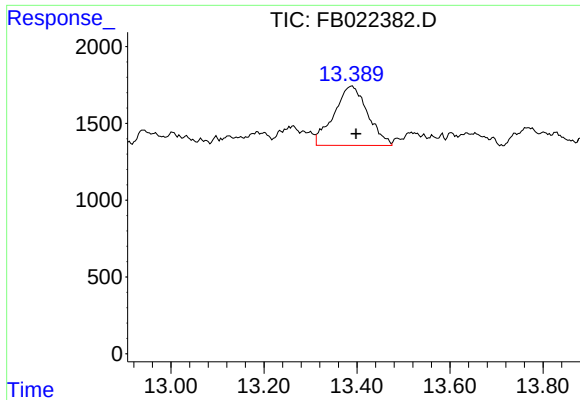

#8 m-Xylene


R.T.: 13.389 min
Delta R.T.: -0.009 min
Response: 19442
Conc: 0.73 ng/ml

Instrument :
FID_B
ClientSampleId :

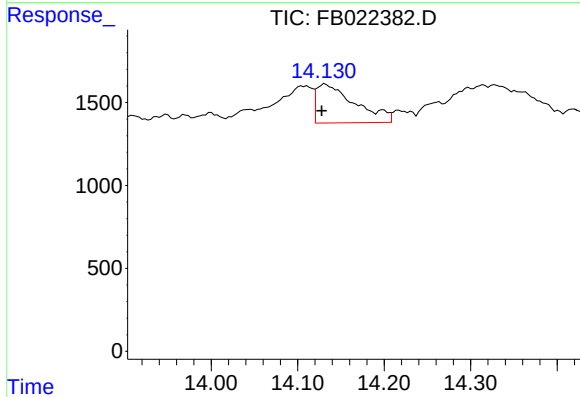

#9 O-Xylene

R.T.: 14.132 min
Delta R.T.: 0.004 min
Response: 7186
Conc: 0.30 ng/ml

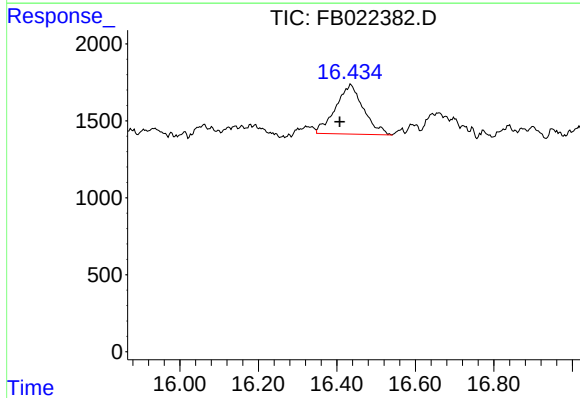

#10 1,2,4-Trimethylbenzene

R.T.: 16.436 min
Delta R.T.: 0.029 min
Response: 15780
Conc: 0.61 ng/ml