

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090719\
 Data File : FB022385.D
 Signal(s) : FID2B.CH
 Acq On : 8 Sep 2019 1:09
 Operator : DD/AJ
 Sample : K4636-16
 Misc : 5.08g/5.00ML DI WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Sep 09 00:49:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.968	418147	14.375 ng/ml
Target Compounds			
3) t n-Heptane	7.921	6055	0.120 ng/ml
4) t Benzene	8.054	10602	0.179 ng/ml
6) t Toluene	10.787	3528	0.074 ng/ml
7) t Ethylbenzene	13.213	8808	0.294 ng/ml
9) t O-Xylene	14.129	3527	0.145 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090719\
Data File : FB022385.D
Signal(s) : FID2B.CH
Acq On : 8 Sep 2019 1:09
Operator : DD/AJ
Sample : K4636-16
Misc : 5.08g/5.00ML DI WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 09 00:49:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

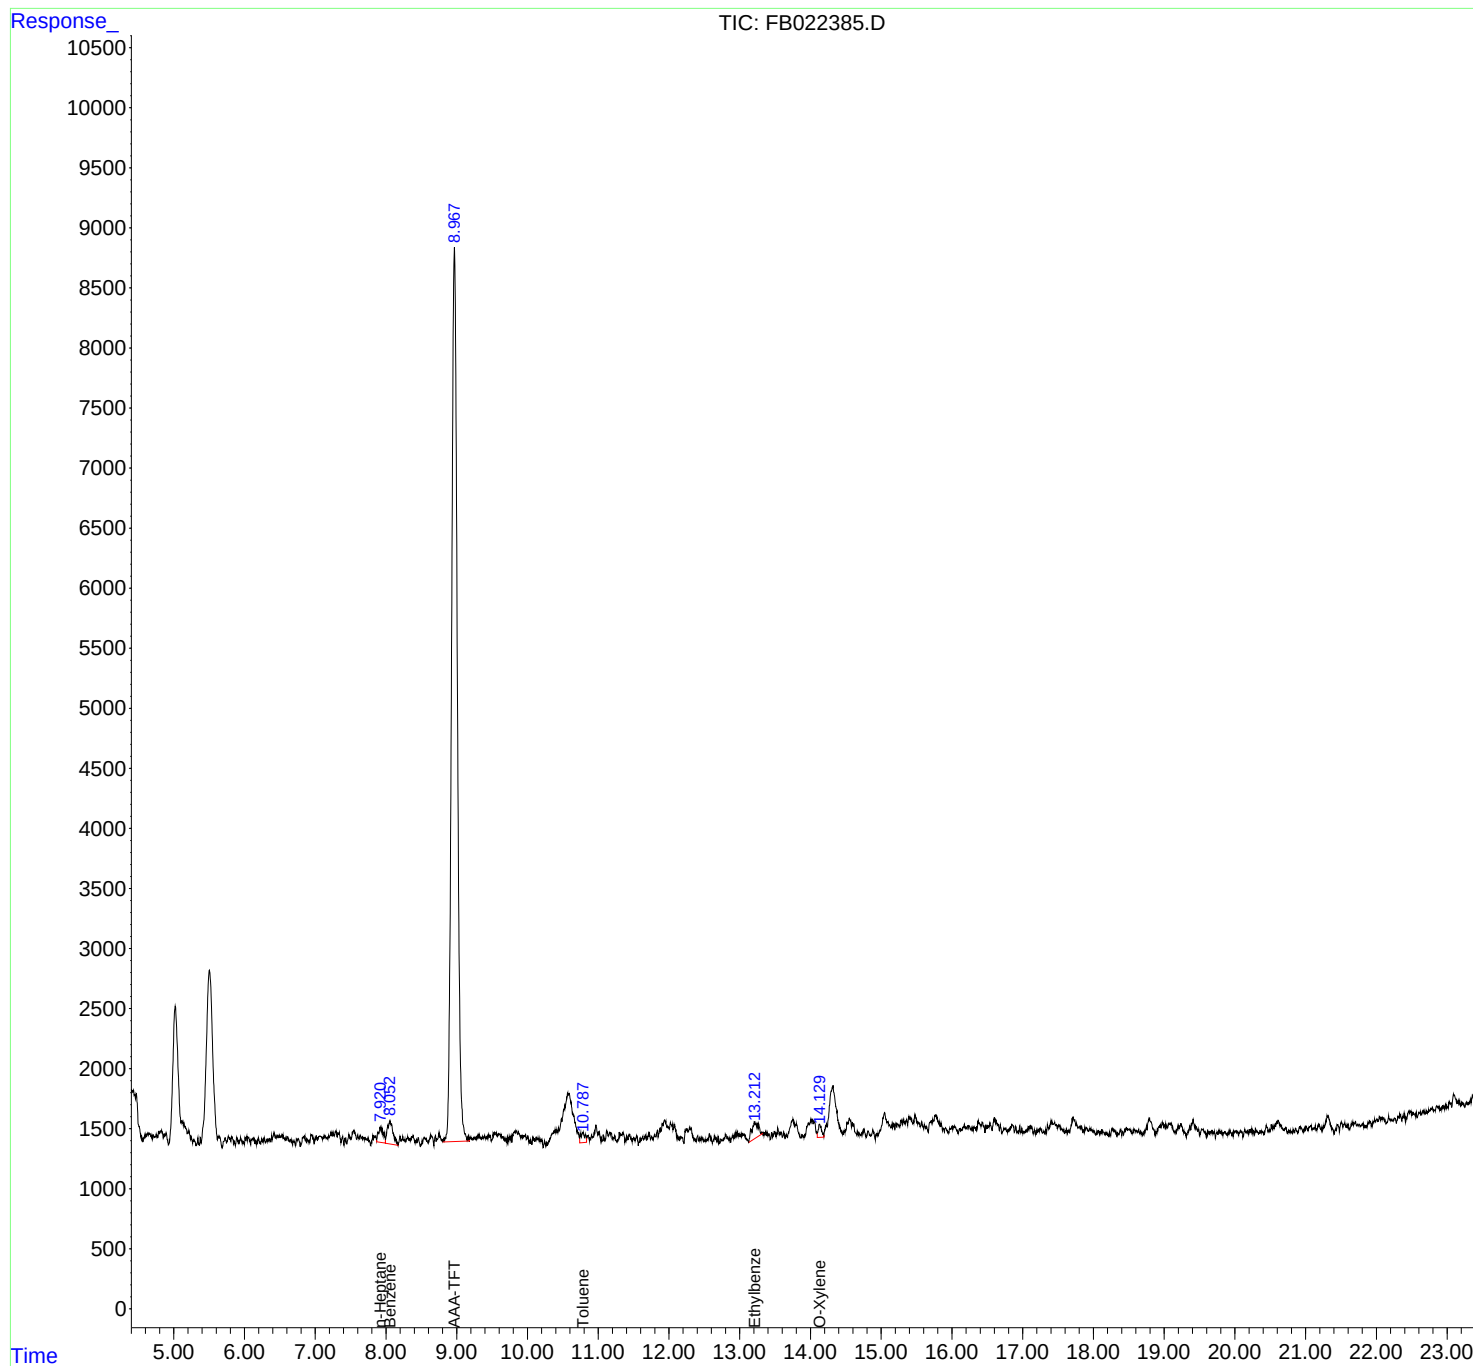


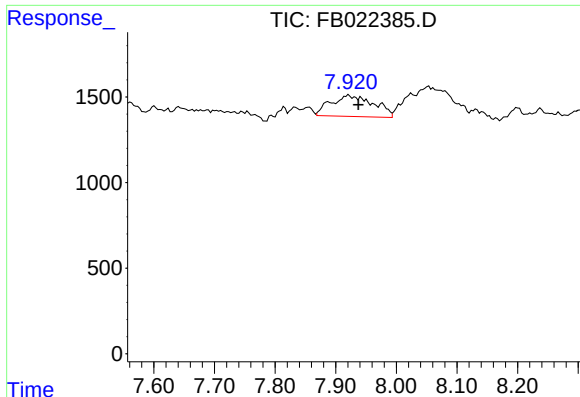

#3 n-Heptane


R.T.: 7.921 min
Delta R.T.: -0.016 min
Response: 6055
Conc: 0.12 ng/ml

Instrument :
FID_B
ClientSampleId :

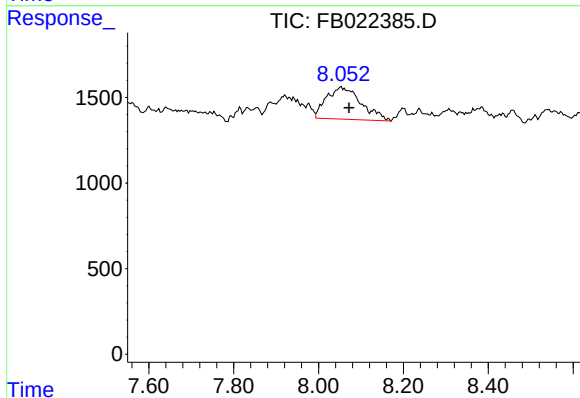


#4 Benzene

R.T.: 8.054 min
Delta R.T.: -0.018 min
Response: 10602
Conc: 0.18 ng/ml

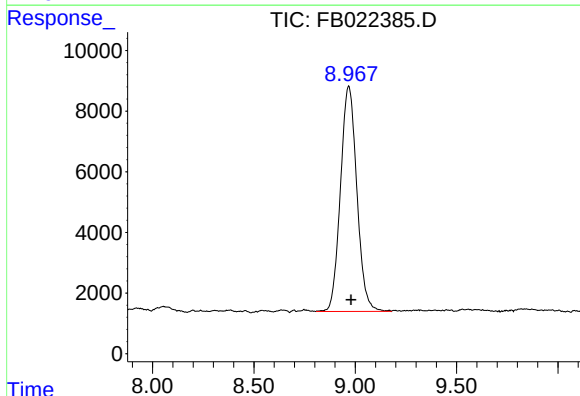


#5 AAA-TFT

R.T.: 8.968 min
Delta R.T.: -0.011 min
Response: 418147
Conc: 14.38 ng/ml

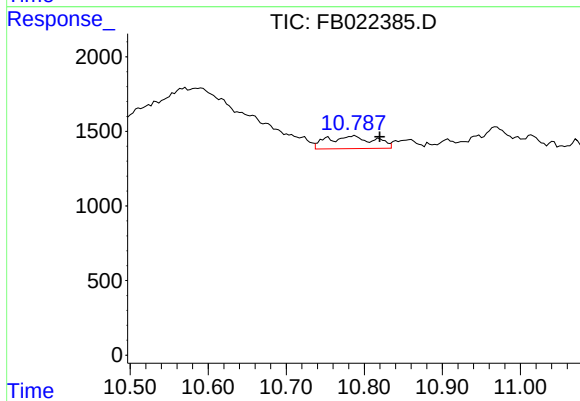

#6 Toluene


R.T.: 10.787 min
Delta R.T.: -0.033 min
Response: 3528
Conc: 0.07 ng/ml

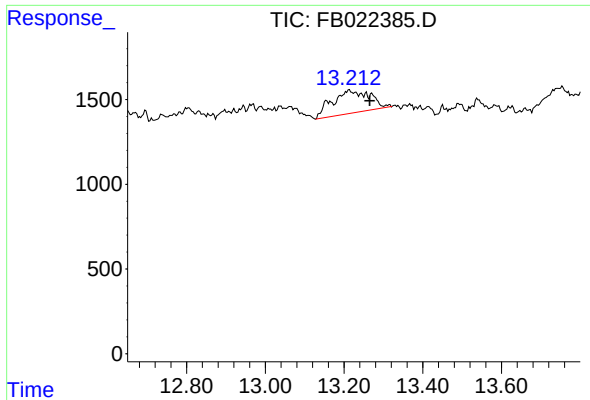

#7 Ethylbenzene

R.T.: 13.213 min
Delta R.T.: -0.052 min
Response: 8808
Conc: 0.29 ng/ml

Instrument :
FID_B
ClientSampleId :

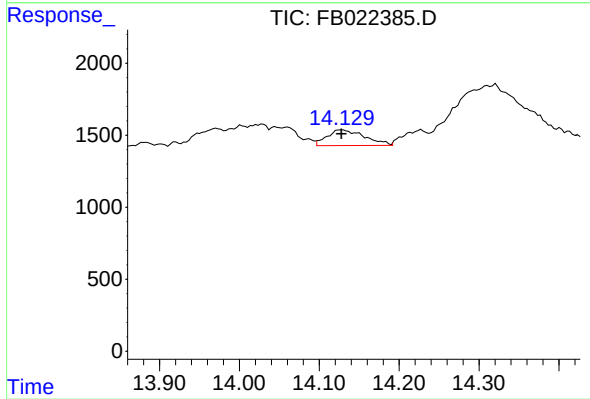

#9 O-Xylene

R.T.: 14.129 min
Delta R.T.: 0.001 min
Response: 3527
Conc: 0.15 ng/ml