

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090719\
Data File : FB022387.D
Signal(s) : FID2B.CH
Acq On : 8 Sep 2019 2:09
Operator : DD/AJ
Sample : K4662-02
Misc : 5.04g/5.00ML DI WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 09 00:50:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.971	452784	15.566 ng/ml
Target Compounds			
6) t Toluene	10.808	5803	0.122 ng/ml
7) t Ethylbenzene	13.238	4450	0.148 ng/ml
8) t m-Xylene	13.388	16377	0.616 ng/ml
9) t O-Xylene	14.114	6793	0.280 ng/ml
10) t 1,2,4-Trimethylbenzene	16.397	4371	0.168 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090719\
Data File : FB022387.D
Signal(s) : FID2B.CH
Acq On : 8 Sep 2019 2:09
Operator : DD/AJ
Sample : K4662-02
Misc : 5.04g/5.00ML DI WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 09 00:50:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

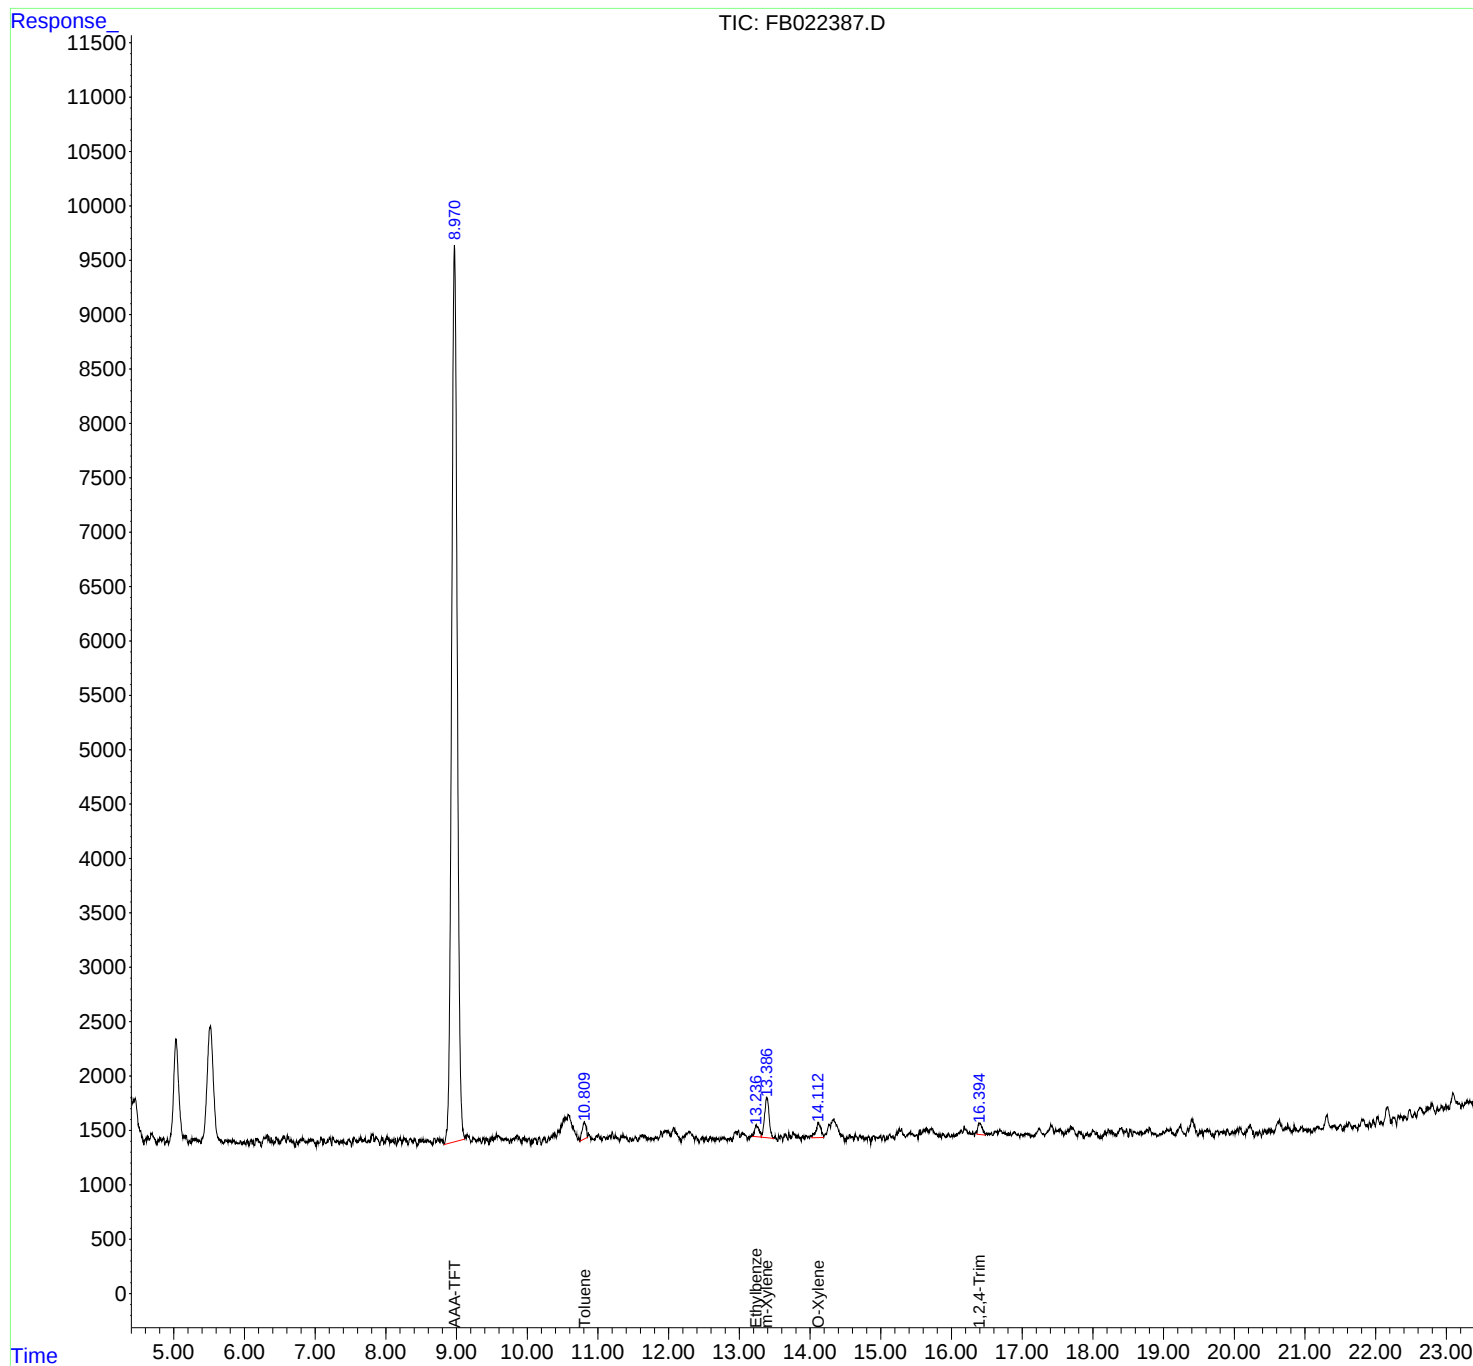


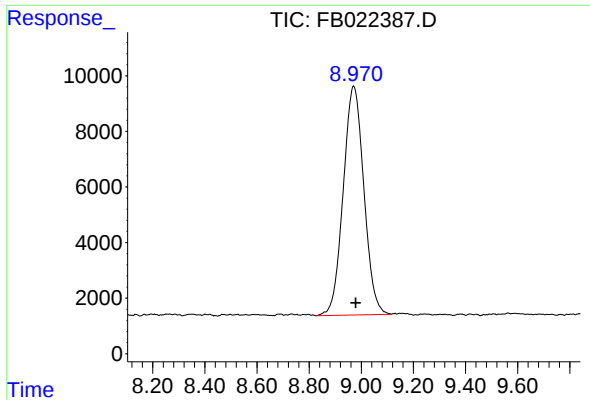

#5 AAA-TFT


R.T.: 8.971 min
Delta R.T.: -0.008 min
Response: 452784
Conc: 15.57 ng/ml

Instrument :
FID_B
ClientSampleId :

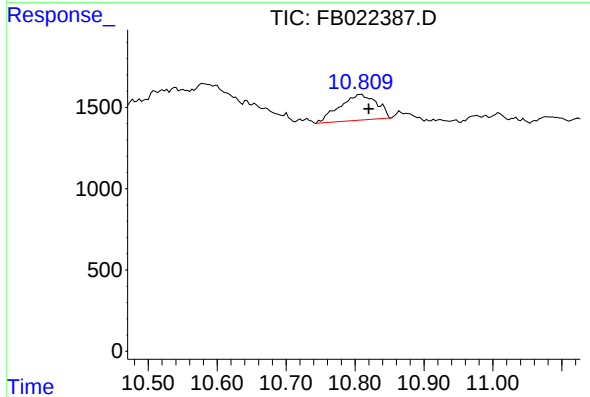


#6 Toluene

R.T.: 10.808 min
Delta R.T.: -0.011 min
Response: 5803
Conc: 0.12 ng/ml

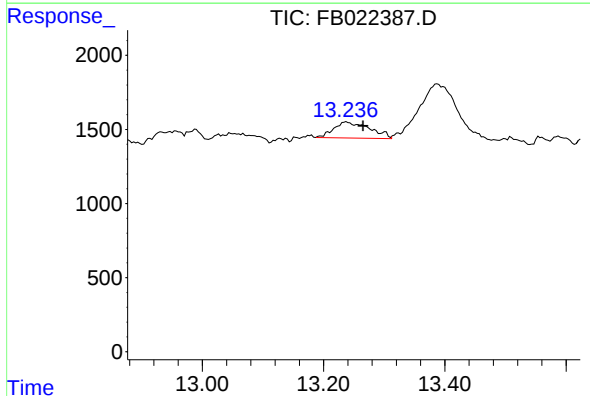


#7 Ethylbenzene

R.T.: 13.238 min
Delta R.T.: -0.027 min
Response: 4450
Conc: 0.15 ng/ml

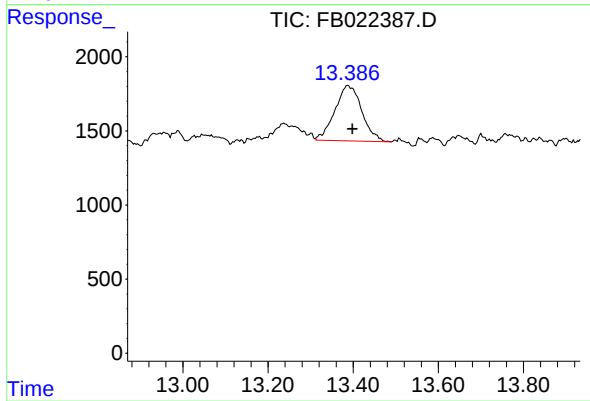

#8 m-Xylene


R.T.: 13.388 min
Delta R.T.: -0.010 min
Response: 16377
Conc: 0.62 ng/ml

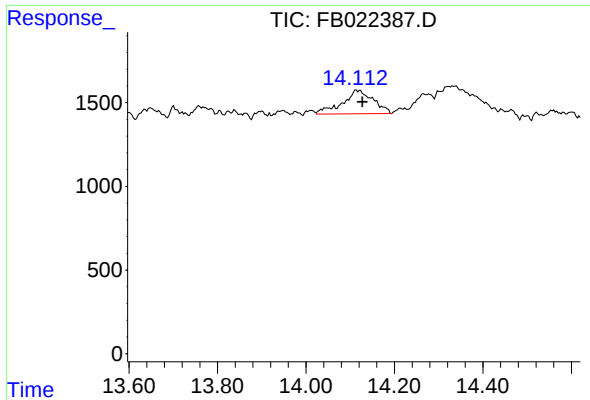

#9 O-Xylene

R.T.: 14.114 min
Delta R.T.: -0.014 min
Response: 6793
Conc: 0.28 ng/ml

Instrument :
FID_B
ClientSampleId :

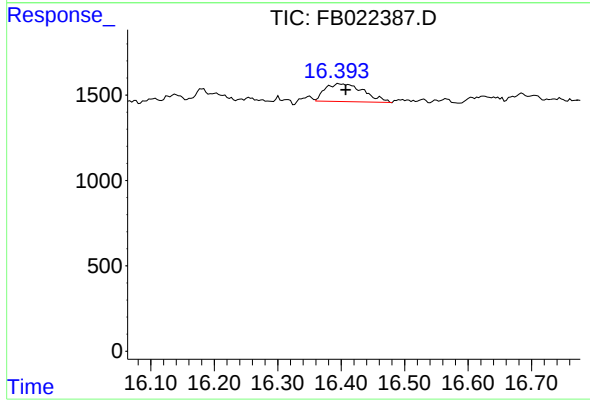

#10 1,2,4-Trimethylbenzene

R.T.: 16.397 min
Delta R.T.: -0.010 min
Response: 4371
Conc: 0.17 ng/ml