

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090719\
 Data File : FB022364.D
 Signal(s) : FID2B.CH
 Acq On : 7 Sep 2019 13:15
 Operator : DD/AJ
 Sample : BSF0907S1
 Misc : 5.01g/5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0907S1

Integration File: Calibration.e
 Quant Time: Sep 09 00:43:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.971	586222	20.154 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.838	1195030	24.322 ng/ml
2) t 2,2,4-Trimethylpentane	7.589	1319911	25.561 ng/ml
3) t n-Heptane	7.928	435192	8.647 ng/ml
4) t Benzene	8.064	552599	9.311 ng/ml
6) t Toluene	10.812	1527391	32.106 ng/ml
7) t Ethylbenzene	13.259	453634	15.132 ng/ml
8) t m-Xylene	13.392	865945	32.596 ng/ml
9) t O-Xylene	14.122	775676	31.973 ng/ml
10) t 1,2,4-Trimethylbenzene	16.403	498112	19.106 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090719\
Data File : FB022364.D
Signal(s) : FID2B.CH
Acq On : 7 Sep 2019 13:15
Operator : DD/AJ
Sample : BSF0907S1
Misc : 5.01g/5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0907S1

Integration File: Calibration.e
Quant Time: Sep 09 00:43:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

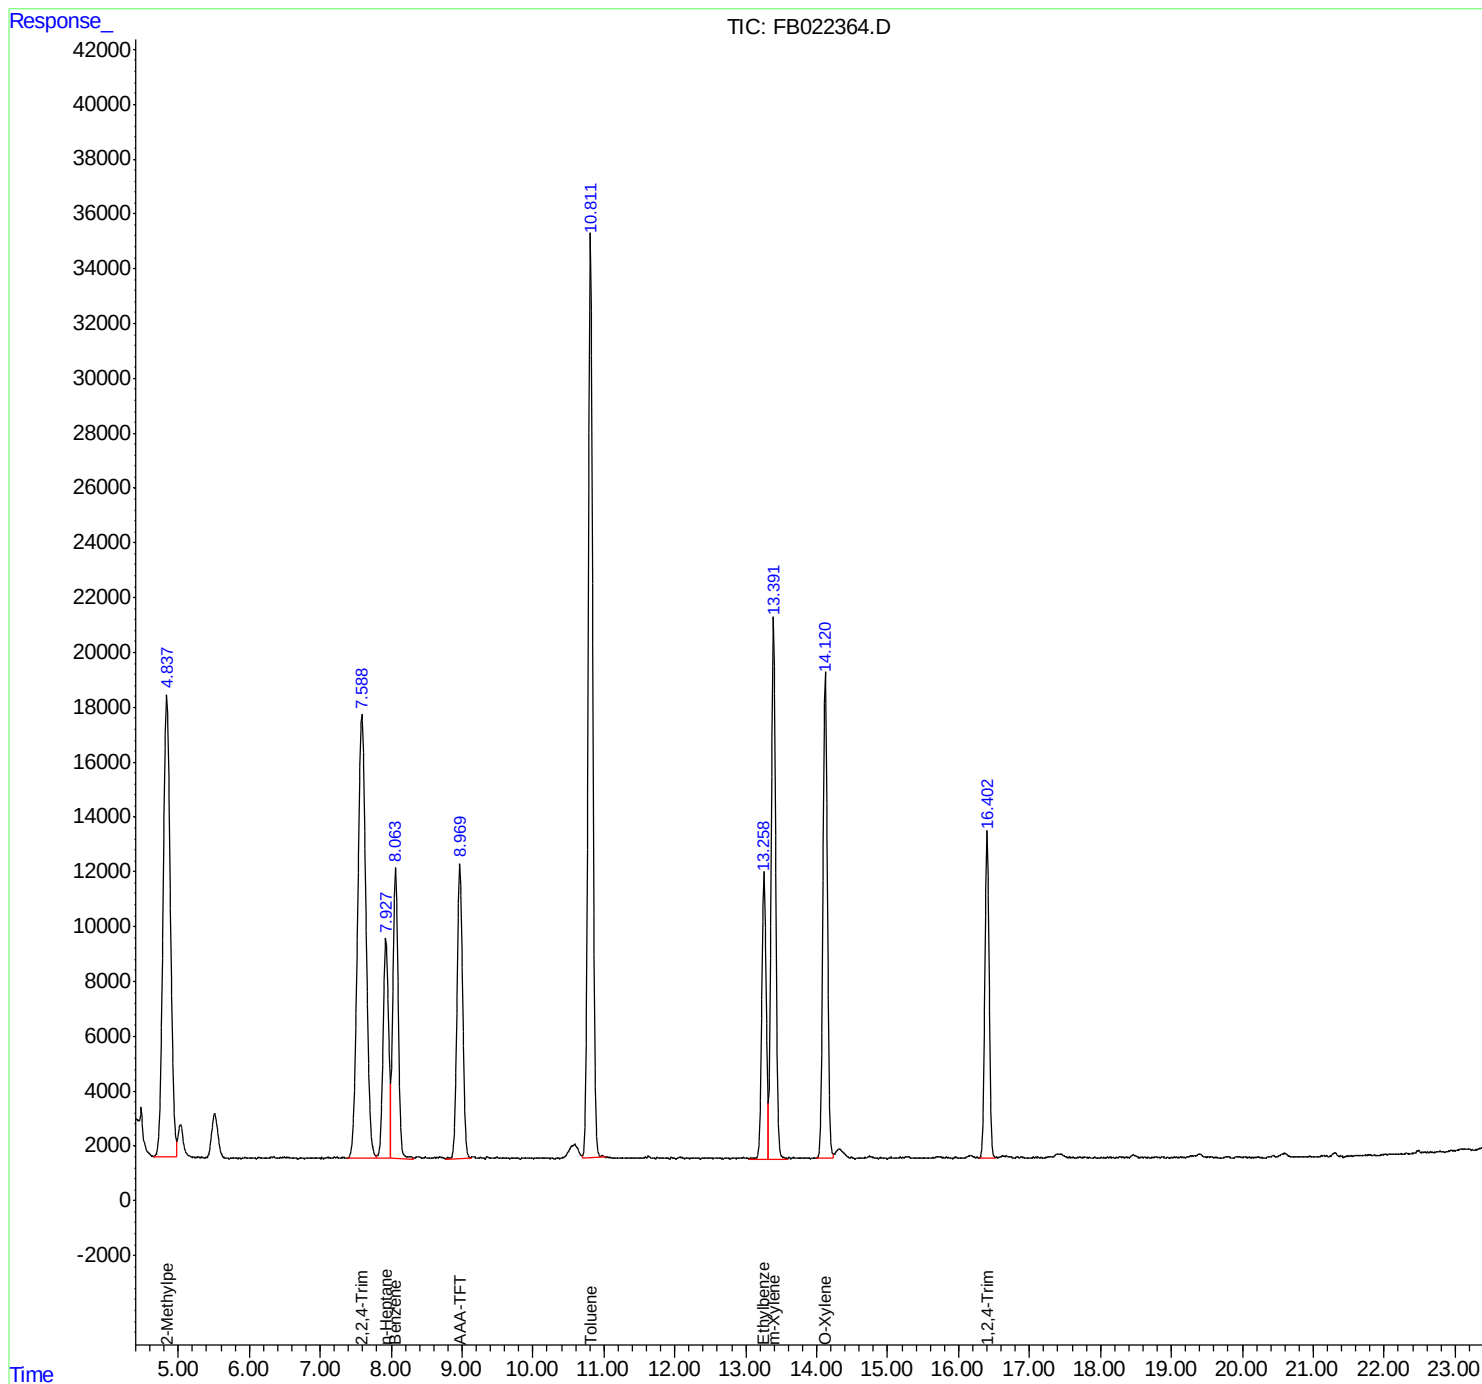


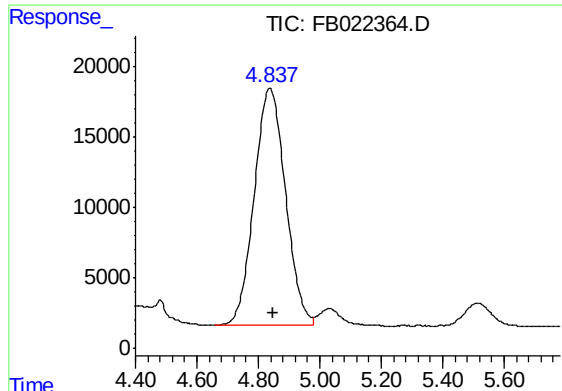

#1 2-Methylpentane


R.T.: 4.838 min
Delta R.T.: -0.009 min
Response: 1195030
Conc: 24.32 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0907S1

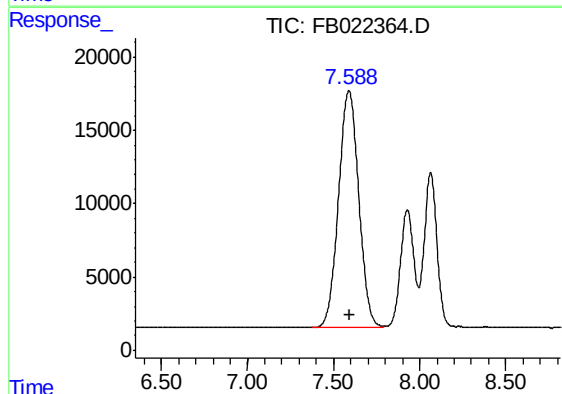


#2 2,2,4-Trimethylpentane

R.T.: 7.589 min
Delta R.T.: -0.008 min
Response: 1319911
Conc: 25.56 ng/ml

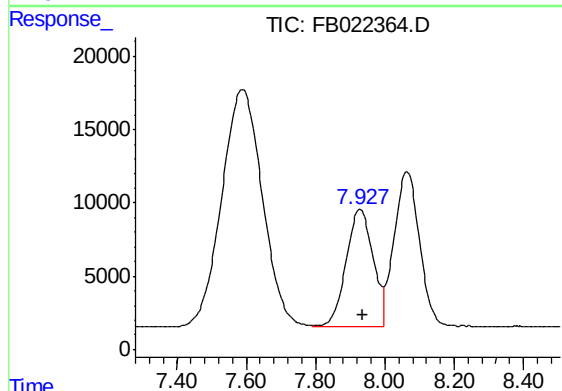


#3 n-Heptane

R.T.: 7.928 min
Delta R.T.: -0.009 min
Response: 435192
Conc: 8.65 ng/ml

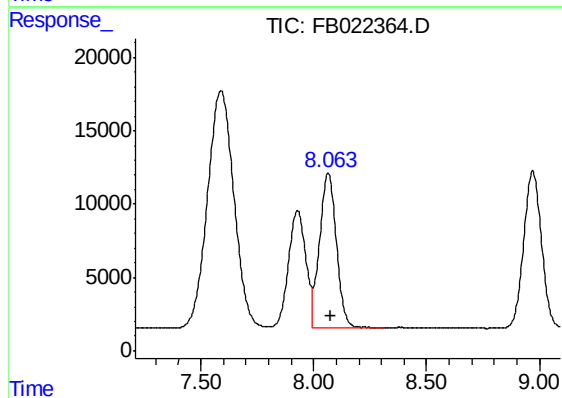

#4 Benzene


R.T.: 8.064 min
Delta R.T.: -0.008 min
Response: 552599
Conc: 9.31 ng/ml

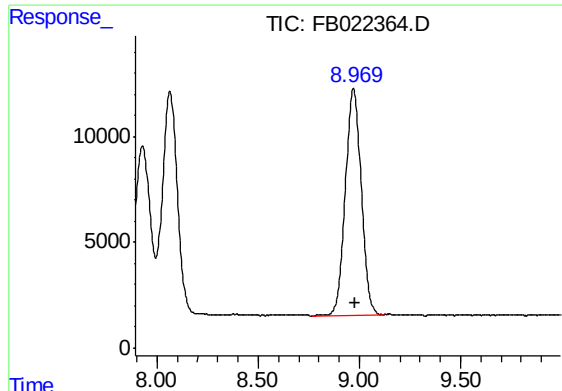

#5 AAA-TFT


R.T.: 8.971 min
Delta R.T.: -0.008 min
Response: 586222
Conc: 20.15 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0907S1

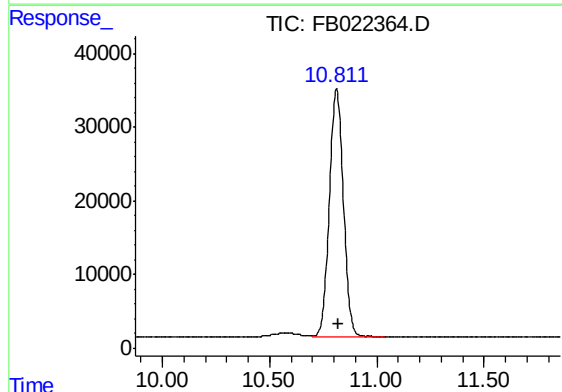


#6 Toluene

R.T.: 10.812 min
Delta R.T.: -0.007 min
Response: 1527391
Conc: 32.11 ng/ml

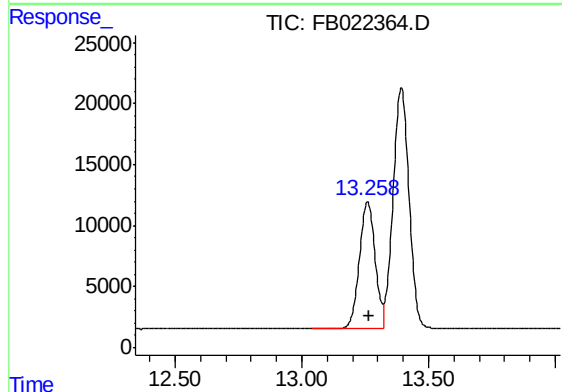


#7 Ethylbenzene

R.T.: 13.259 min
Delta R.T.: -0.006 min
Response: 453634
Conc: 15.13 ng/ml

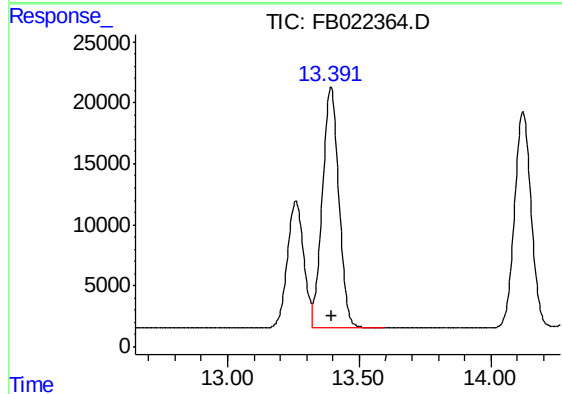

#8 m-Xylene


R.T.: 13.392 min
Delta R.T.: -0.006 min
Response: 865945
Conc: 32.60 ng/ml

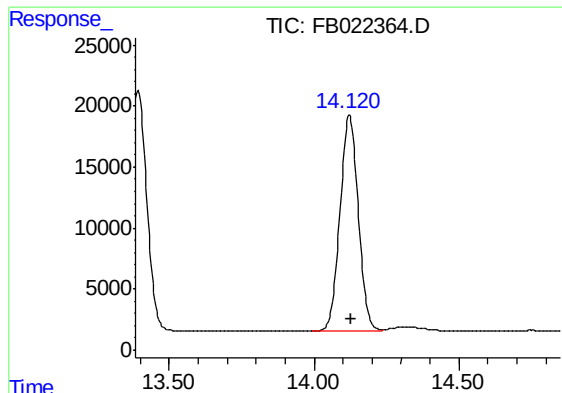

#9 O-Xylene

R.T.: 14.122 min
Delta R.T.: -0.006 min
Response: 775676
Conc: 31.97 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0907S1

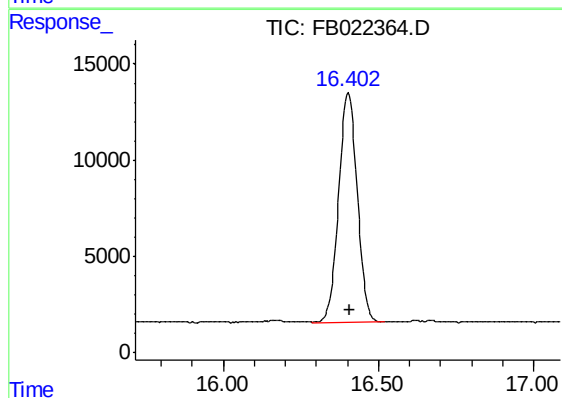

#10 1,2,4-Trimethylbenzene

R.T.: 16.403 min
Delta R.T.: -0.004 min
Response: 498112
Conc: 19.11 ng/ml