

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090719\
 Data File : FB022375.D
 Signal(s) : FID2B.CH
 Acq On : 7 Sep 2019 19:05
 Operator : DD/AJ
 Sample : K4752-02MS
 Misc : 5.01g/5.00ML DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-07-COMPMS

Integration File: Calibration.e
 Quant Time: Sep 09 00:46:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.972	491331	16.891 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.835	997268	20.297 ng/ml
2) t 2,2,4-Trimethylpentane	7.589	1149983	22.270 ng/ml
3) t n-Heptane	7.929	369320	7.338 ng/ml
4) t Benzene	8.064	453542	7.642 ng/ml
6) t Toluene	10.813	1299853	27.323 ng/ml
7) t Ethylbenzene	13.260	392541	13.094 ng/ml
8) t m-Xylene	13.392	763061	28.723 ng/ml
9) t O-Xylene	14.122	711576	29.331 ng/ml
10) t 1,2,4-Trimethylbenzene	16.403	456254	17.500 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090719\
Data File : FB022375.D
Signal(s) : FID2B.CH
Acq On : 7 Sep 2019 19:05
Operator : DD/AJ
Sample : K4752-02MS
Misc : 5.01g/5.00ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMS

Integration File: Calibration.e
Quant Time: Sep 09 00:46:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

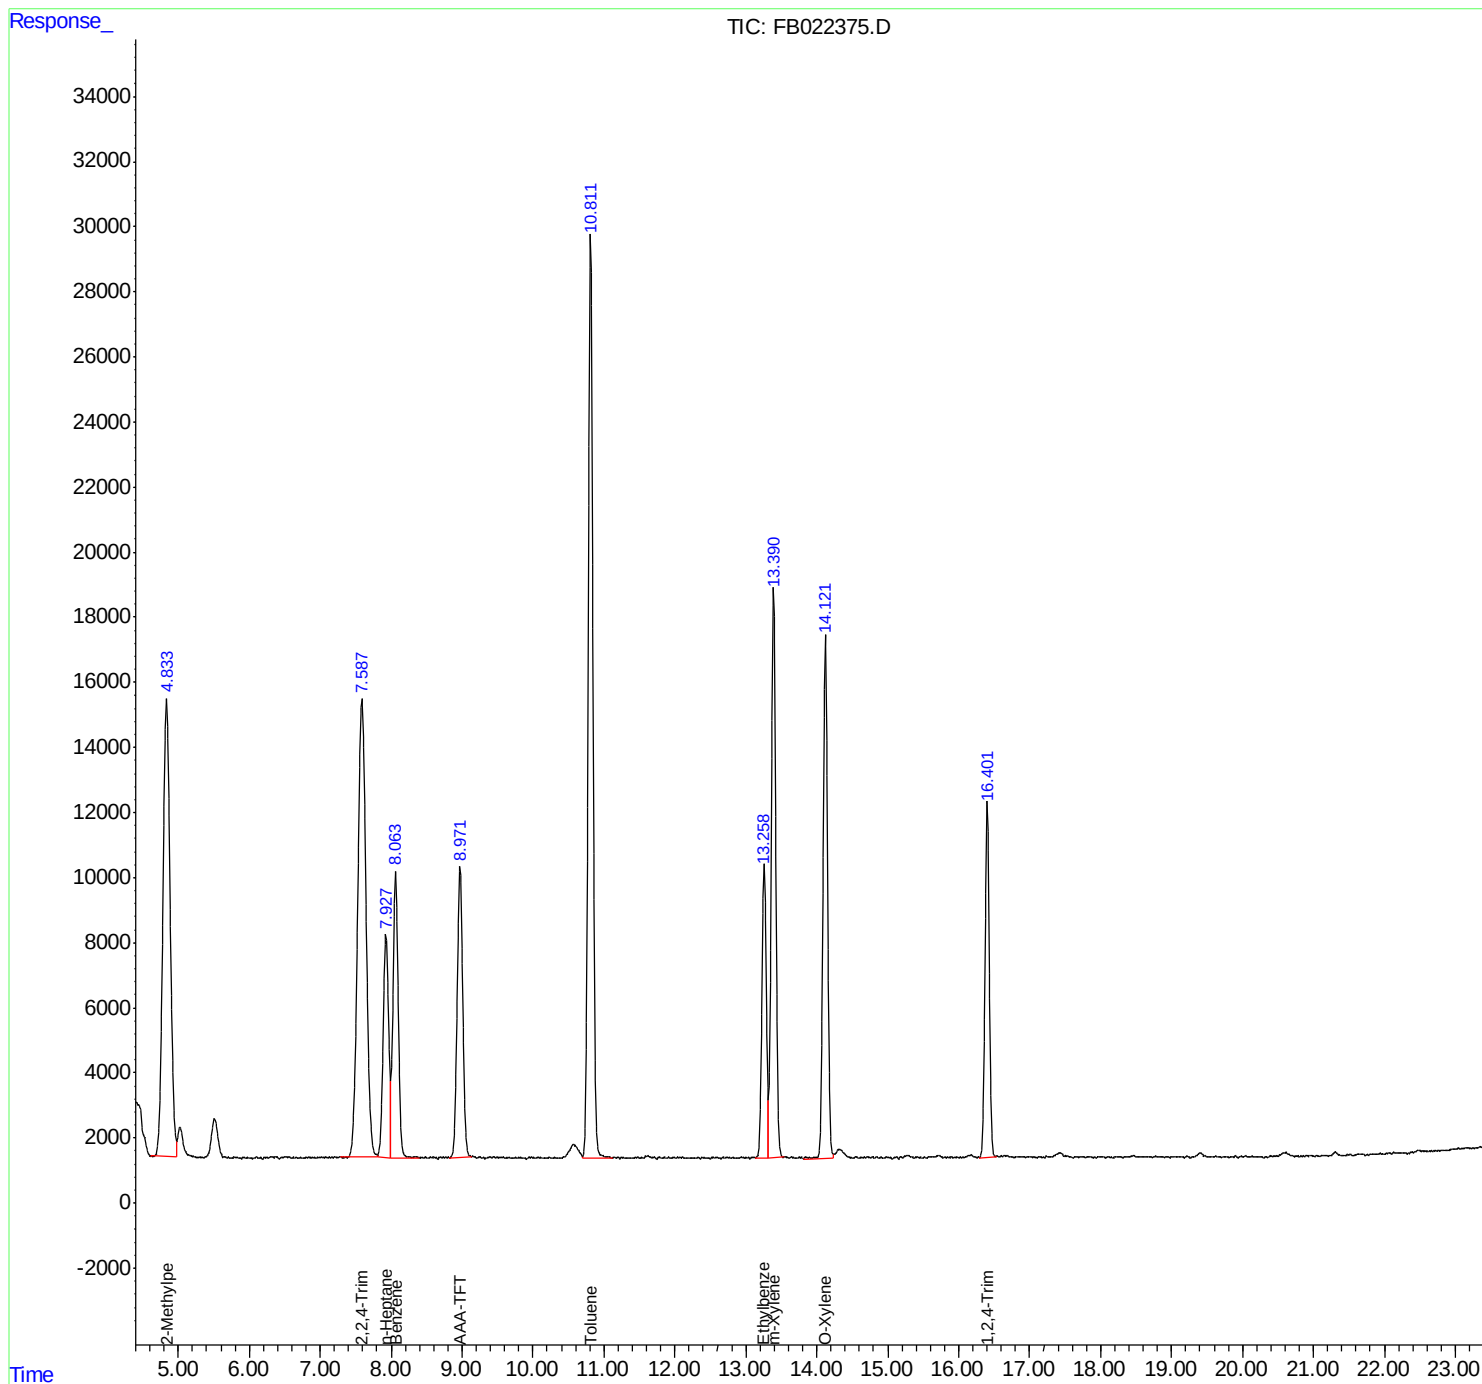


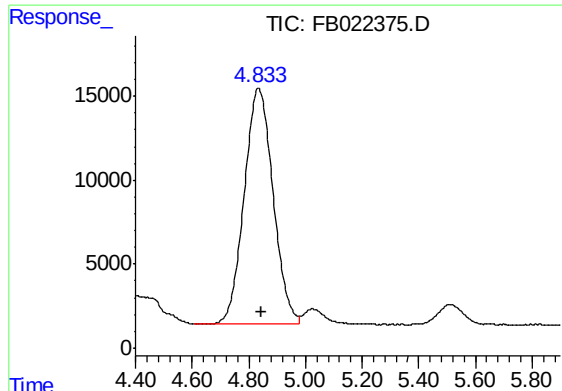

#1 2-Methylpentane


R.T.: 4.835 min
Delta R.T.: -0.012 min
Response: 997268
Conc: 20.30 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMS

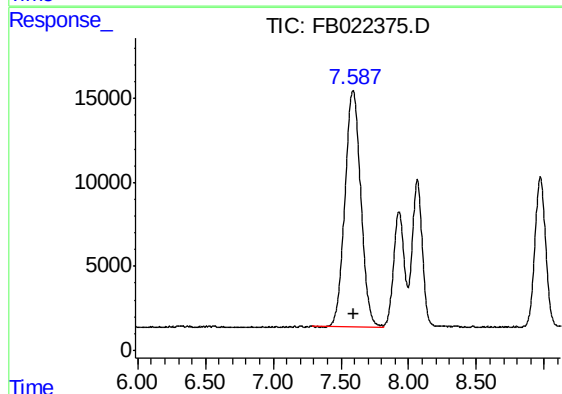


#2 2,2,4-Trimethylpentane

R.T.: 7.589 min
Delta R.T.: -0.009 min
Response: 1149983
Conc: 22.27 ng/ml

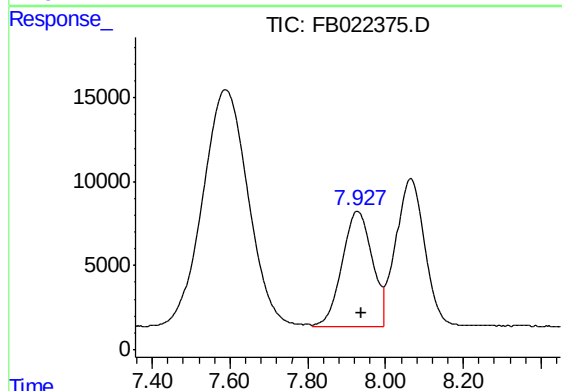


#3 n-Heptane

R.T.: 7.929 min
Delta R.T.: -0.009 min
Response: 369320
Conc: 7.34 ng/ml

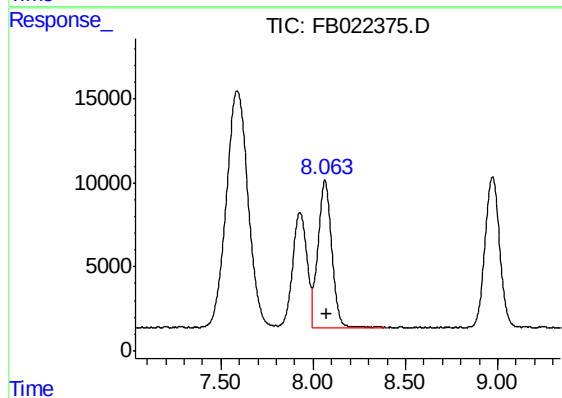

#4 Benzene


R.T.: 8.064 min
Delta R.T.: -0.008 min
Response: 453542
Conc: 7.64 ng/ml

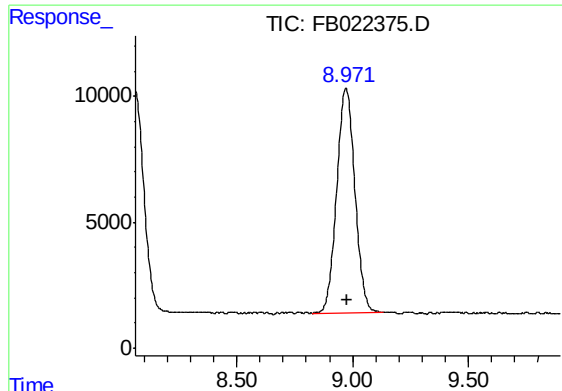

#5 AAA-TFT


R.T.: 8.972 min
Delta R.T.: -0.007 min
Response: 491331
Conc: 16.89 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMS

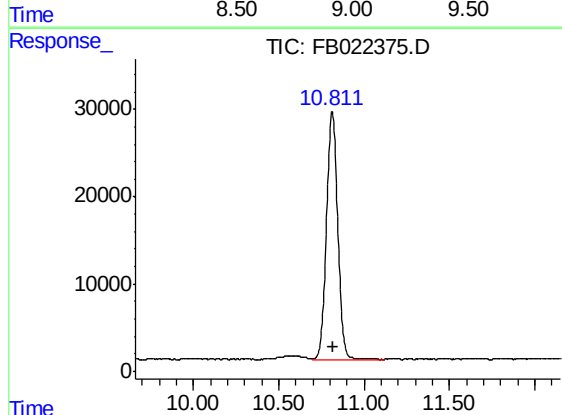


#6 Toluene

R.T.: 10.813 min
Delta R.T.: -0.007 min
Response: 1299853
Conc: 27.32 ng/ml

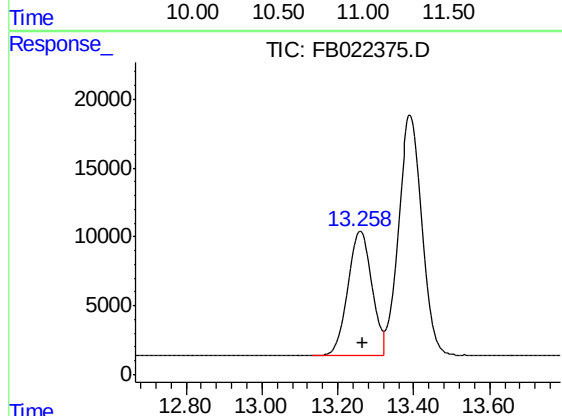


#7 Ethylbenzene

R.T.: 13.260 min
Delta R.T.: -0.005 min
Response: 392541
Conc: 13.09 ng/ml

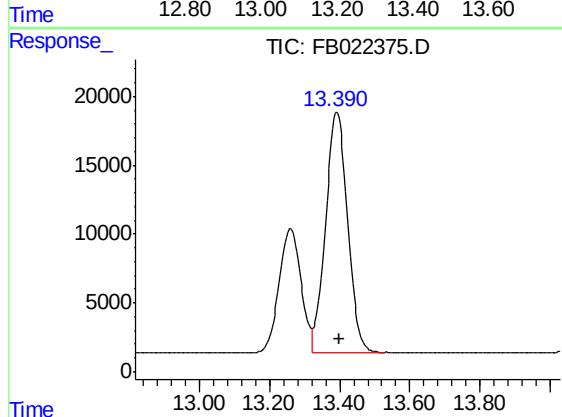

#8 m-Xylene


R.T.: 13.392 min
Delta R.T.: -0.006 min
Response: 763061
Conc: 28.72 ng/ml

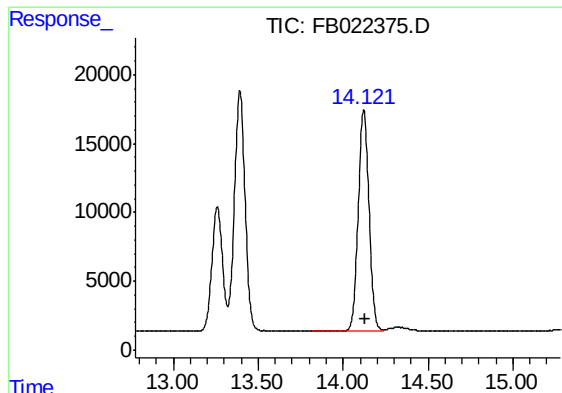

#9 O-Xylene

R.T.: 14.122 min
Delta R.T.: -0.006 min
Response: 711576
Conc: 29.33 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMS

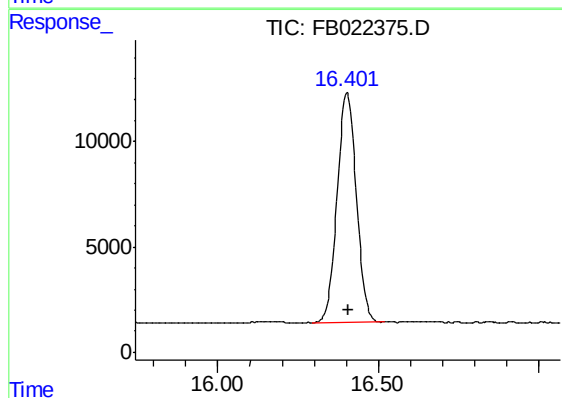

#10 1,2,4-Trimethylbenzene

R.T.: 16.403 min
Delta R.T.: -0.005 min
Response: 456254
Conc: 17.50 ng/ml