

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090719\
 Data File : FB022376.D
 Signal(s) : FID2B.CH
 Acq On : 7 Sep 2019 19:35
 Operator : DD/AJ
 Sample : K4752-02MSD
 Misc : 5.02g/5.00ML DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-07-COMPMSD

Integration File: Calibration.e
 Quant Time: Sep 09 00:47:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
 Quant Title :
 QLast Update : Wed Sep 04 17:01:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.973	522056	17.948 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.837	998624	20.325 ng/ml
2) t 2,2,4-Trimethylpentane	7.590	1148409	22.240 ng/ml
3) t n-Heptane	7.930	372262	7.396 ng/ml
4) t Benzene	8.065	461804	7.781 ng/ml
6) t Toluene	10.814	1298526	27.295 ng/ml
7) t Ethylbenzene	13.260	403295	13.452 ng/ml
8) t m-Xylene	13.393	778467	29.303 ng/ml
9) t O-Xylene	14.122	720942	29.717 ng/ml
10) t 1,2,4-Trimethylbenzene	16.402	456948	17.527 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090719\
Data File : FB022376.D
Signal(s) : FID2B.CH
Acq On : 7 Sep 2019 19:35
Operator : DD/AJ
Sample : K4752-02MSD
Misc : 5.02g/5.00ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMSD

Integration File: Calibration.e
Quant Time: Sep 09 00:47:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090419.M
Quant Title :
QLast Update : Wed Sep 04 17:01:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

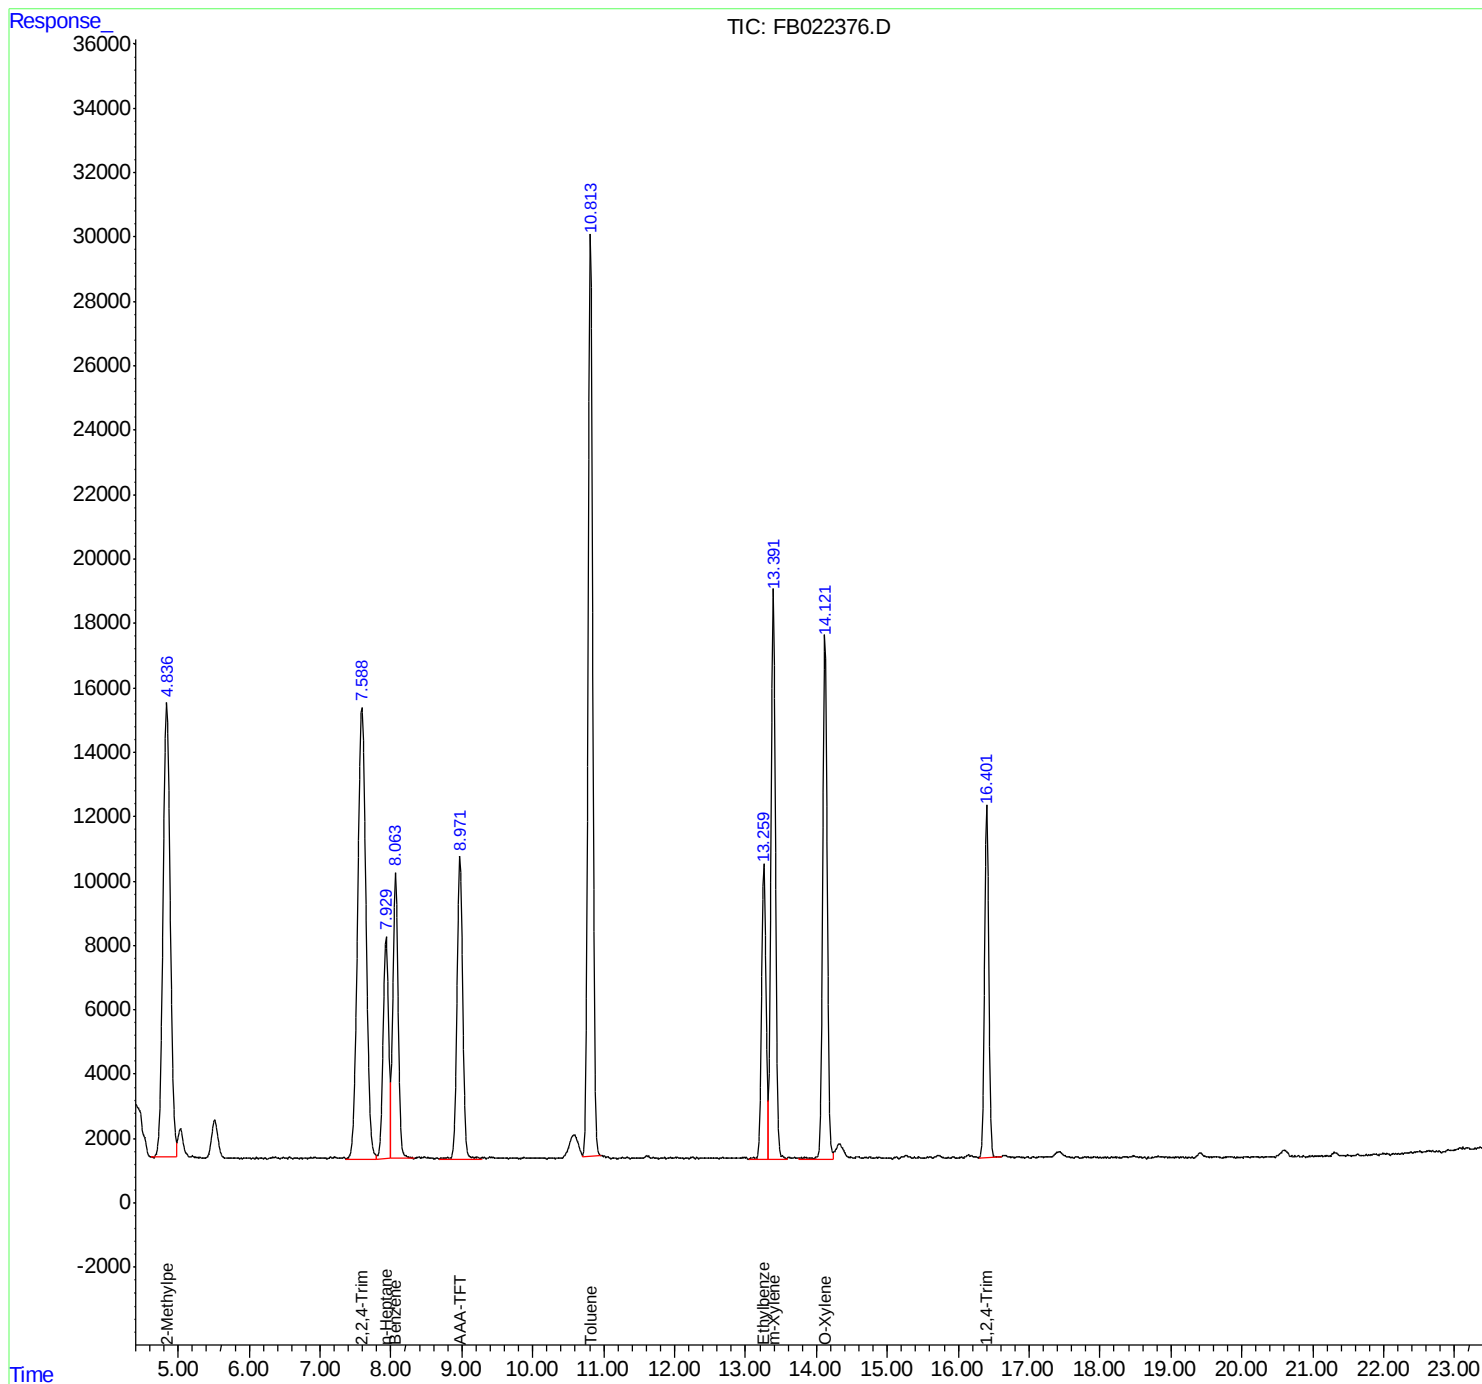


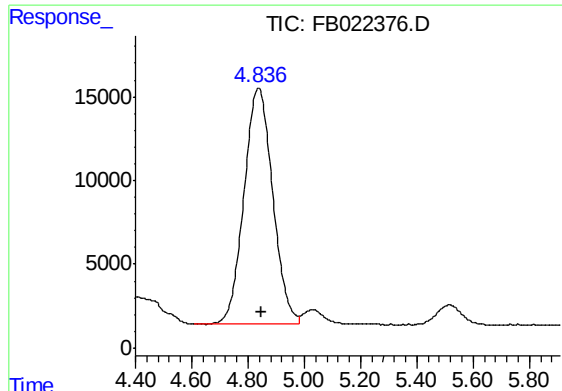

#1 2-Methylpentane


R.T.: 4.837 min
Delta R.T.: -0.010 min
Response: 998624
Conc: 20.32 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMSD

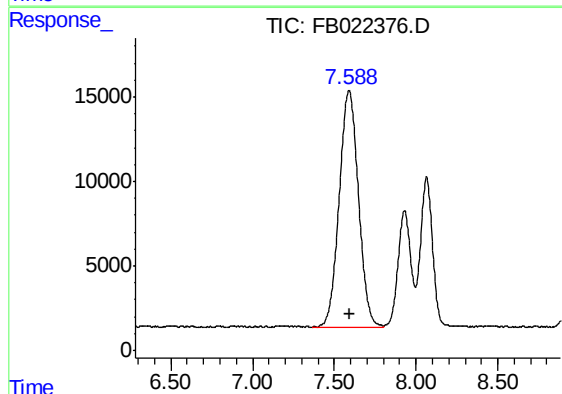


#2 2,2,4-Trimethylpentane

R.T.: 7.590 min
Delta R.T.: -0.008 min
Response: 1148409
Conc: 22.24 ng/ml

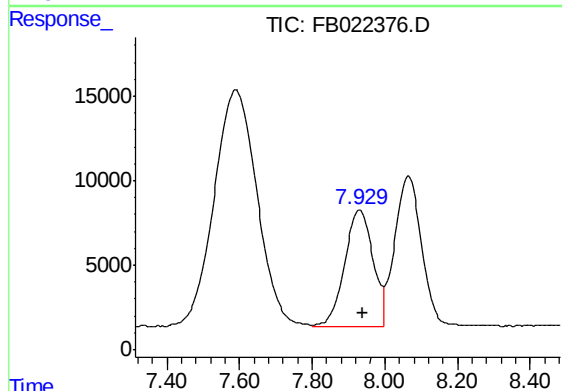


#3 n-Heptane

R.T.: 7.930 min
Delta R.T.: -0.007 min
Response: 372262
Conc: 7.40 ng/ml

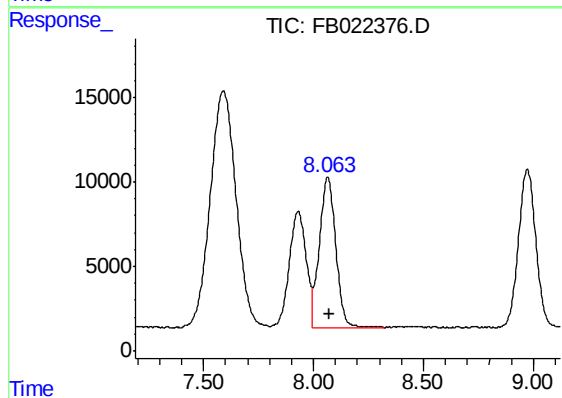

#4 Benzene


R.T.: 8.065 min
Delta R.T.: -0.007 min
Response: 461804
Conc: 7.78 ng/ml

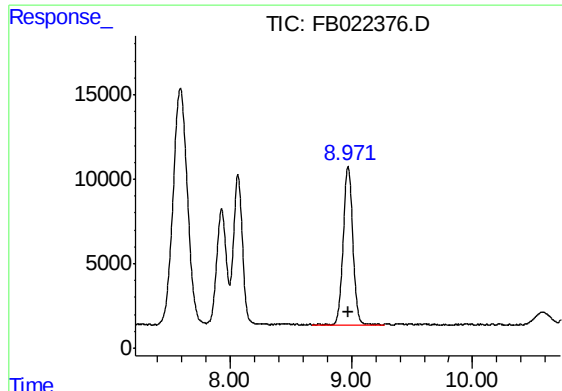

#5 AAA-TFT


R.T.: 8.973 min
Delta R.T.: -0.006 min
Response: 522056
Conc: 17.95 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMSD

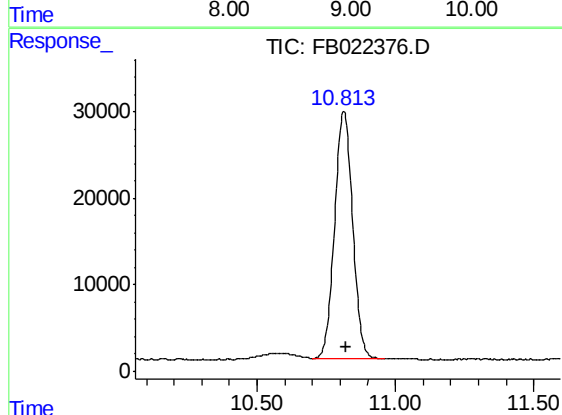


#6 Toluene

R.T.: 10.814 min
Delta R.T.: -0.006 min
Response: 1298526
Conc: 27.30 ng/ml

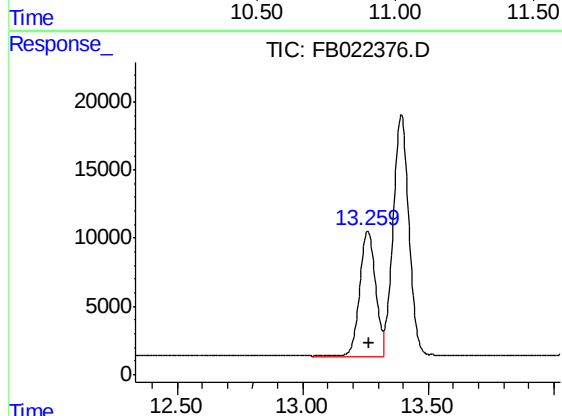


#7 Ethylbenzene

R.T.: 13.260 min
Delta R.T.: -0.005 min
Response: 403295
Conc: 13.45 ng/ml

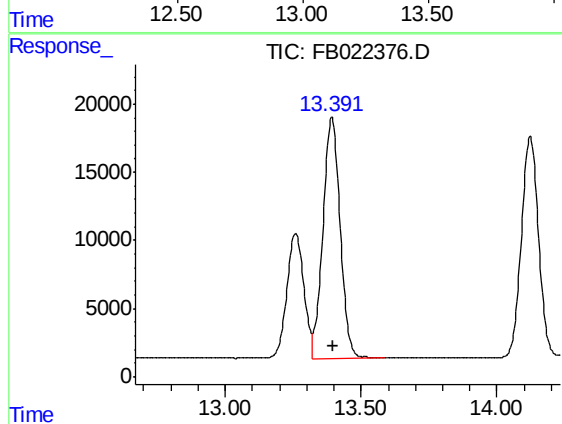

#8 m-Xylene


R.T.: 13.393 min
Delta R.T.: -0.005 min
Response: 778467
Conc: 29.30 ng/ml

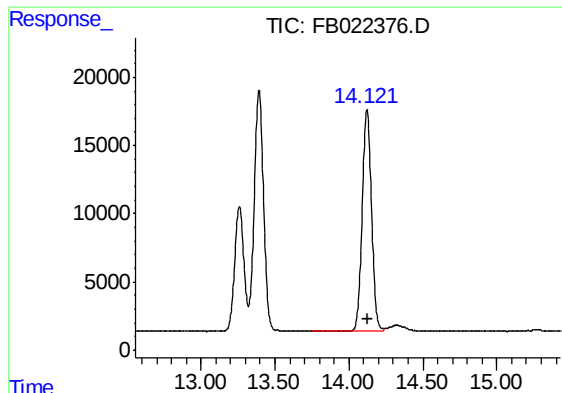

#9 O-Xylene

R.T.: 14.122 min
Delta R.T.: -0.006 min
Response: 720942
Conc: 29.72 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-07-COMPMSD

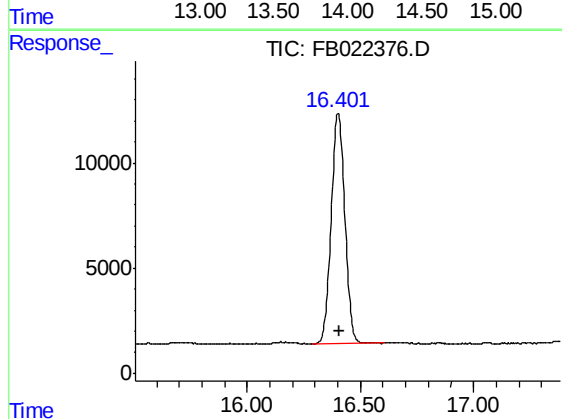

#10 1,2,4-Trimethylbenzene

R.T.: 16.402 min
Delta R.T.: -0.005 min
Response: 456948
Conc: 17.53 ng/ml