

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090722\
Data File : FB028146.D
Signal(s) : FID2B.CH
Acq On : 7 Sep 2022 12:04
Operator : AJ/MA
Sample : BSF0907S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0907S1

Integration File: Calibration.e
Quant Time: Sep 08 04:43:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	228735	19.737 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.715	415587	22.972 ng/ml
2) t 2,2,4-Trimethylpentane	7.433	486067	24.786 ng/ml
3) t n-Heptane	7.756	138806	7.205 ng/ml
4) t Benzene	7.893	191385	8.231 ng/ml
6) t Toluene	10.626	548264	25.003 ng/ml
7) t Ethylbenzene	13.062	176115	8.546 ng/ml
8) t m-Xylene	13.195	343446	16.784 ng/ml
9) t O-Xylene	13.922	336803	17.002 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	317979	16.306 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090722\
Data File : FB028146.D
Signal(s) : FID2B.CH
Acq On : 7 Sep 2022 12:04
Operator : AJ/MA
Sample : BSF0907S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0907S1

Integration File: Calibration.e
Quant Time: Sep 08 04:43:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

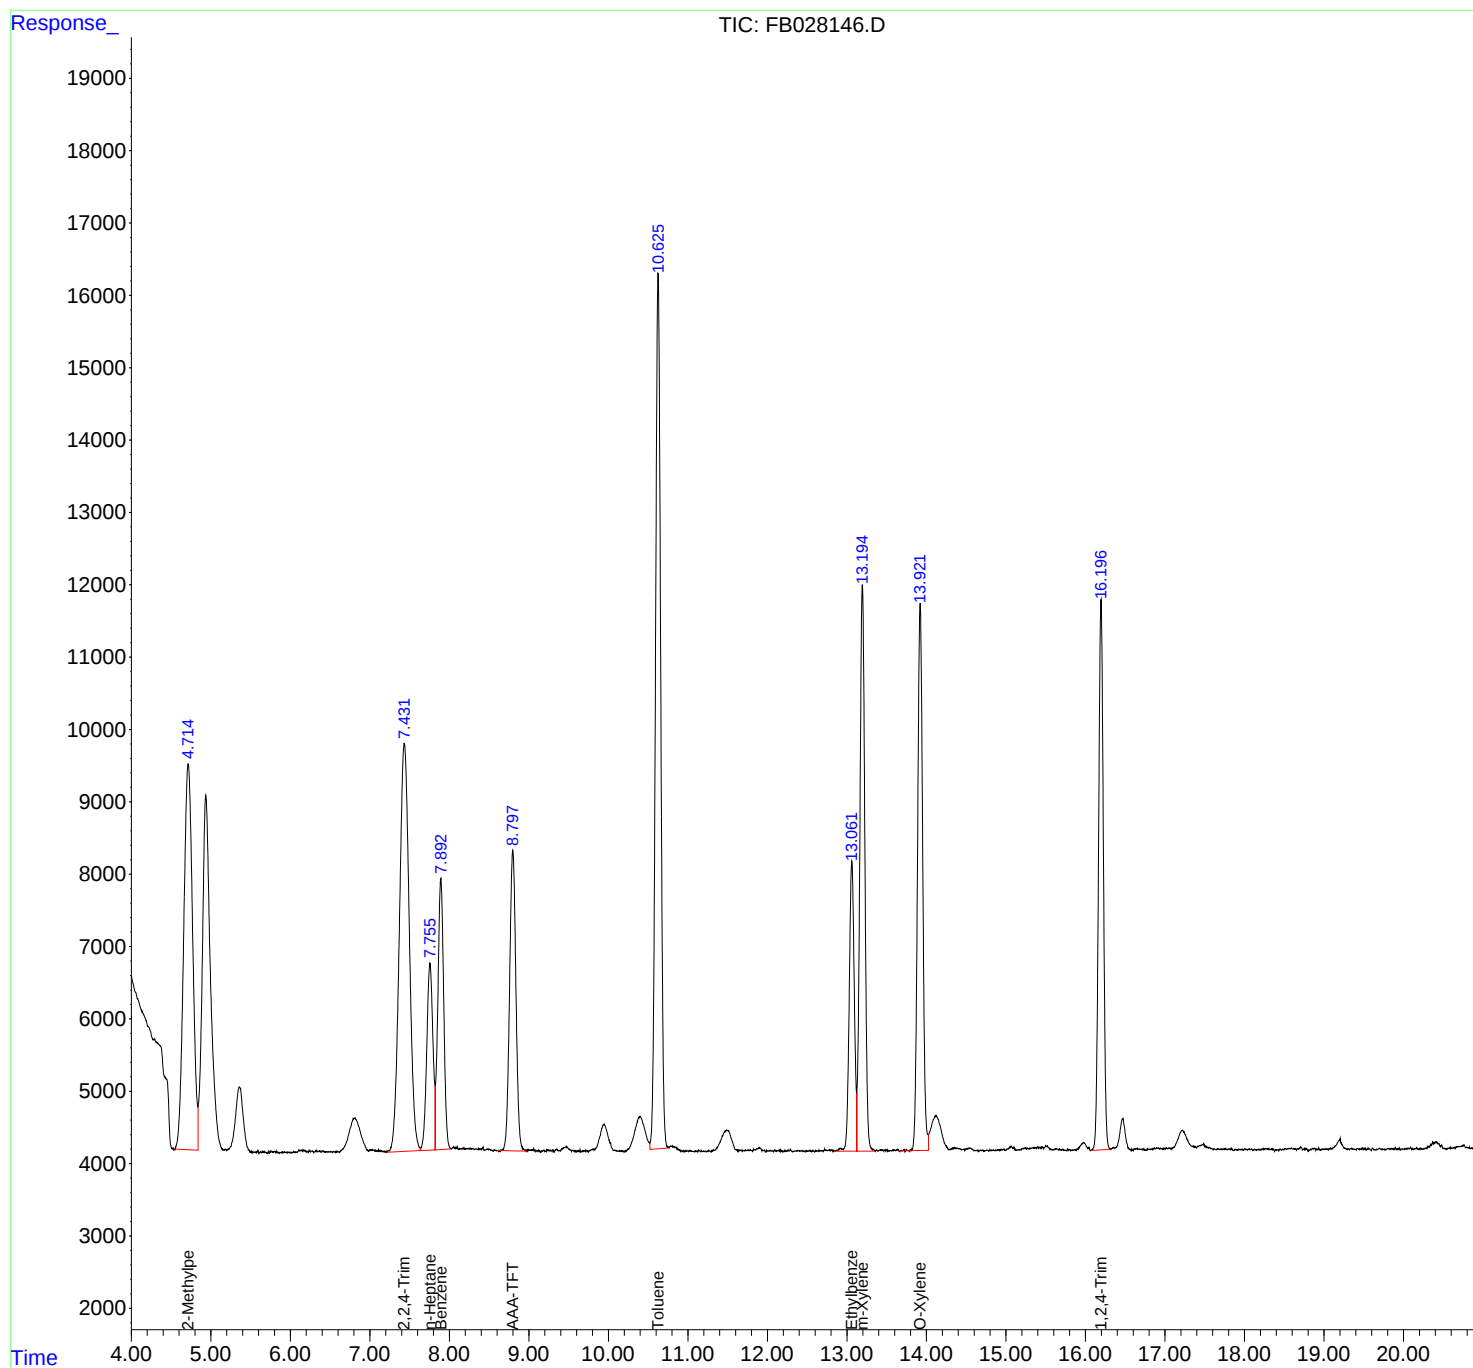


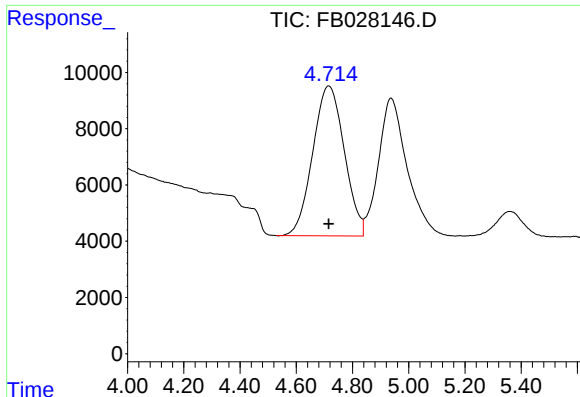

#1 2-Methylpentane


R.T.: 4.715 min
Delta R.T.: 0.000 min
Response: 415587
Conc: 22.97 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0907S1

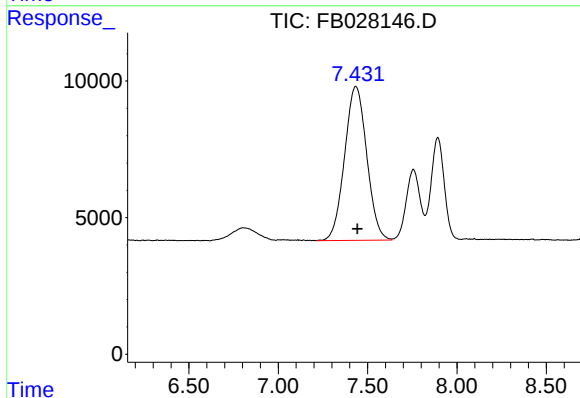


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
Delta R.T.: -0.010 min
Response: 486067
Conc: 24.79 ng/ml

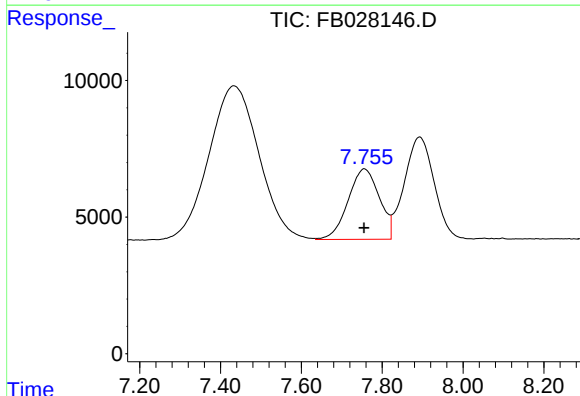


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.001 min
Response: 138806
Conc: 7.21 ng/ml

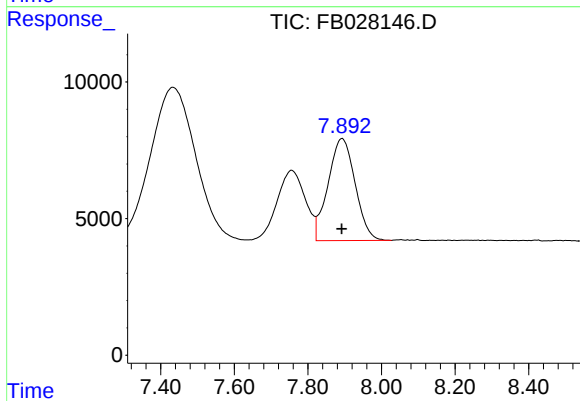

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.001 min
Response: 191385
Conc: 8.23 ng/ml

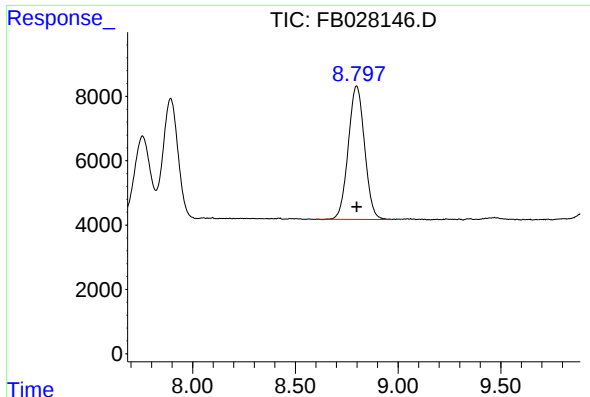

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 228735
Conc: 19.74 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0907S1

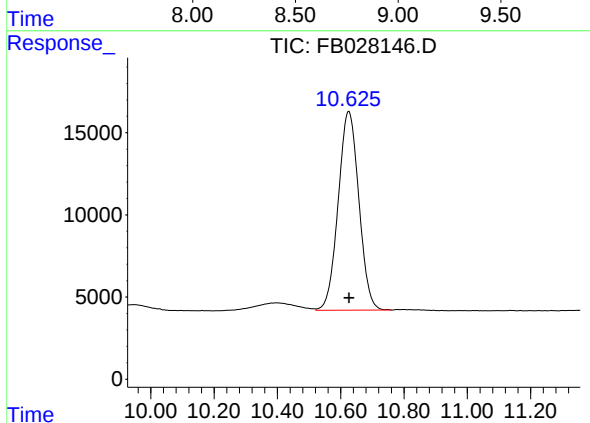


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.001 min
Response: 548264
Conc: 25.00 ng/ml

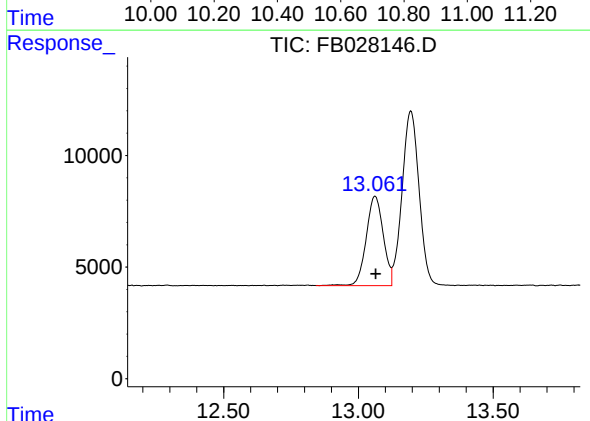


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: -0.002 min
Response: 176115
Conc: 8.55 ng/ml

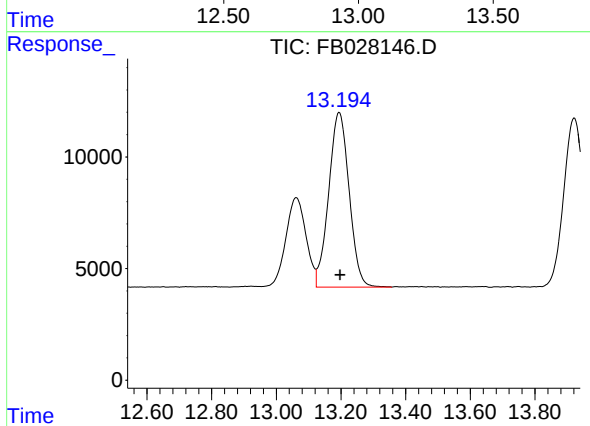

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: -0.002 min
Response: 343446
Conc: 16.78 ng/ml

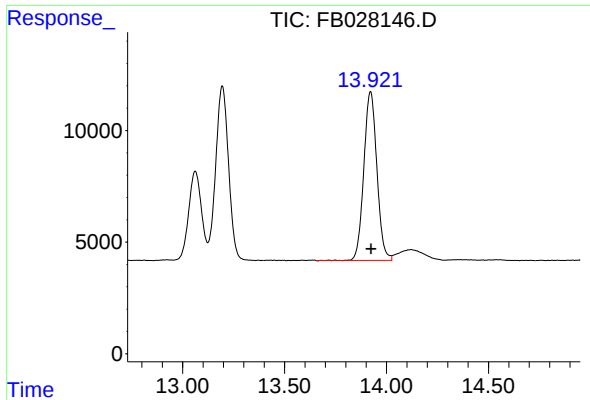

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.002 min
Response: 336803
Conc: 17.00 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0907S1

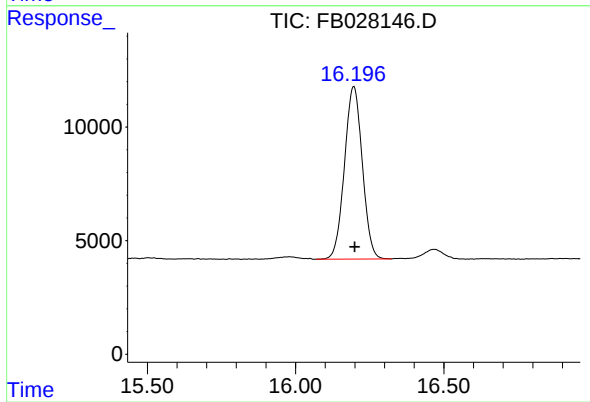

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: -0.003 min
Response: 317979
Conc: 16.31 ng/ml