

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090722\
 Data File : FB028147.D
 Signal(s) : FID2B.CH
 Acq On : 7 Sep 2022 12:41
 Operator : AJ/MA
 Sample : BSF0907W1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0907W1

Integration File: Calibration.e
 Quant Time: Sep 08 04:44:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	188577	16.272 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	456560	25.237 ng/ml
2) t 2,2,4-Trimethylpentane	7.434	513293	26.175 ng/ml
3) t n-Heptane	7.756	147359	7.649 ng/ml
4) t Benzene	7.894	192540	8.281 ng/ml
6) t Toluene	10.627	553424	25.238 ng/ml
7) t Ethylbenzene	13.063	175331	8.508 ng/ml
8) t m-Xylene	13.196	345857	16.902 ng/ml
9) t O-Xylene	13.922	336775	17.001 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	318148	16.314 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB090722\
Data File : FB028147.D
Signal(s) : FID2B.CH
Acq On : 7 Sep 2022 12:41
Operator : AJ/MA
Sample : BSF0907W1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0907W1

Integration File: Calibration.e
Quant Time: Sep 08 04:44:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

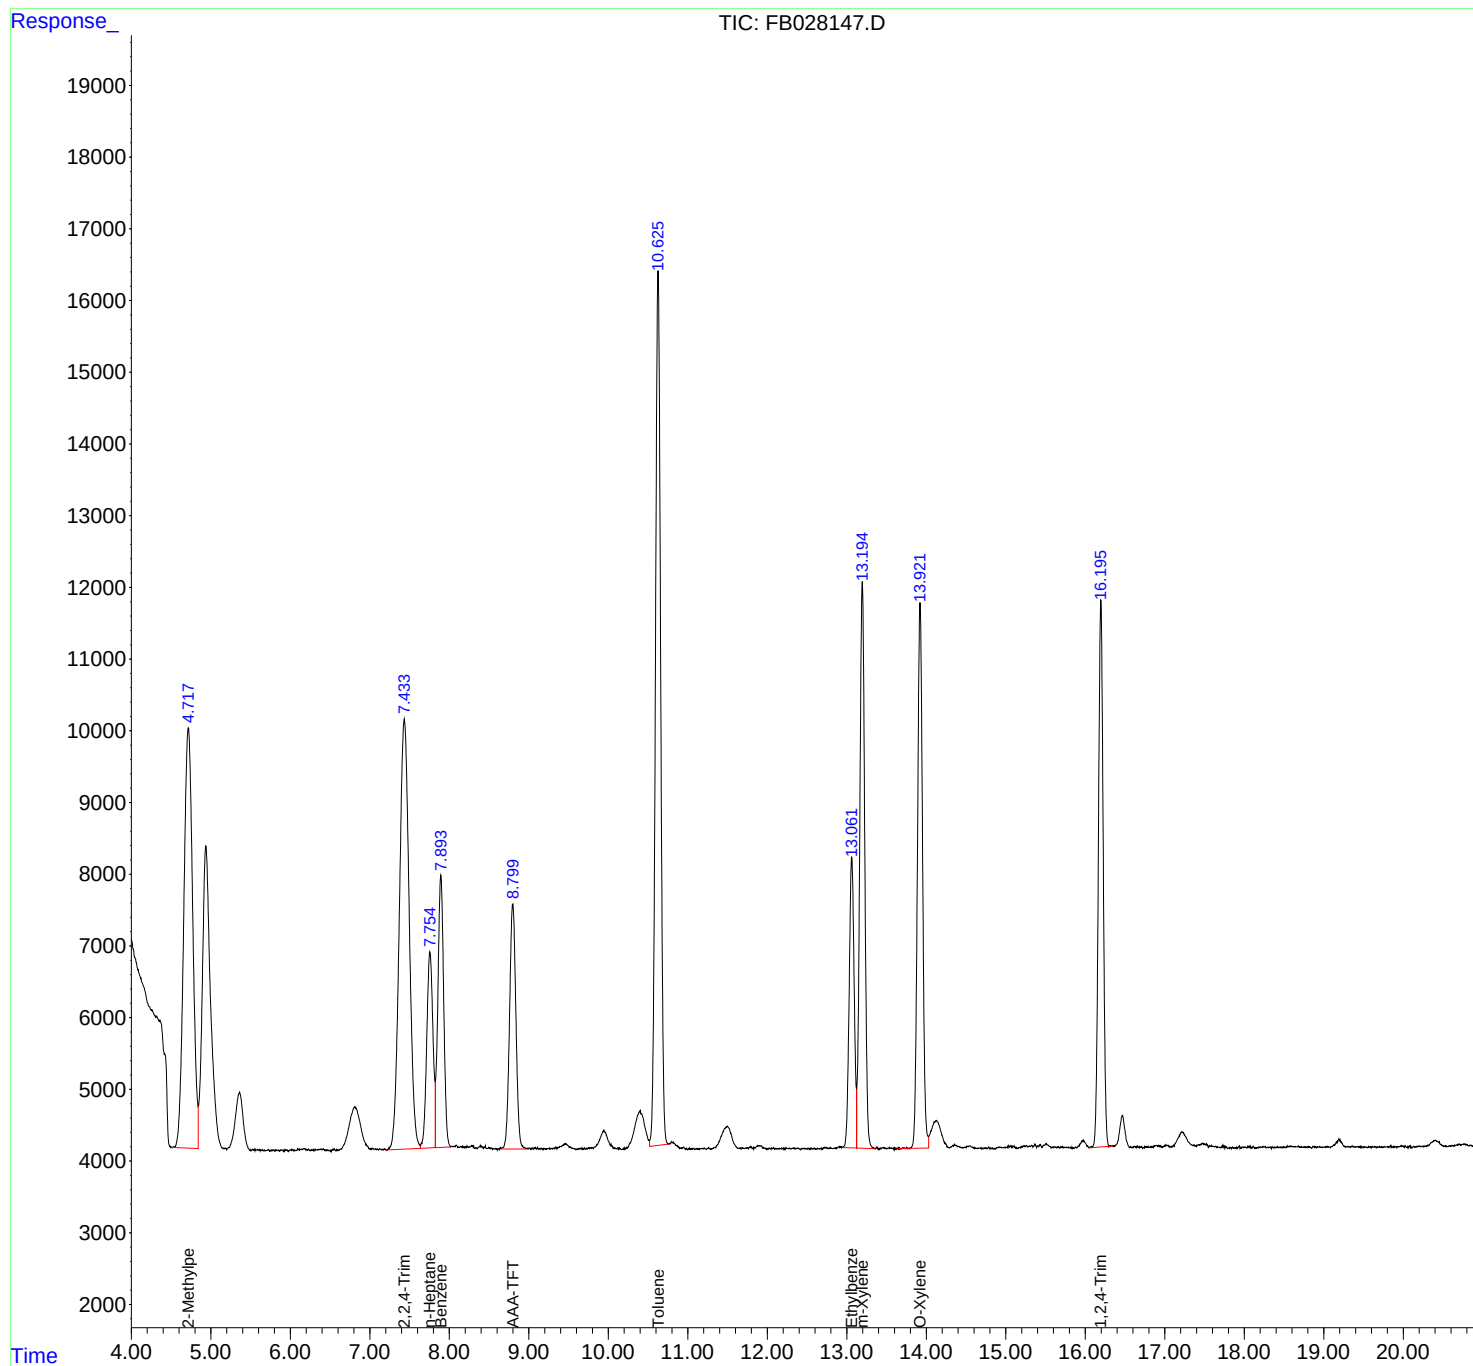


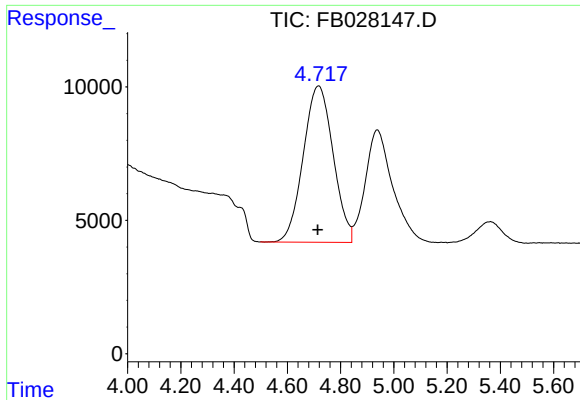

#1 2-Methylpentane


R.T.: 4.718 min
Delta R.T.: 0.003 min
Response: 456560
Conc: 25.24 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0907W1

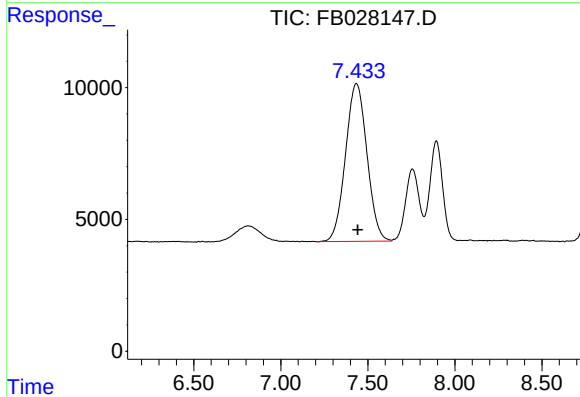


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min
Delta R.T.: -0.008 min
Response: 513293
Conc: 26.17 ng/ml

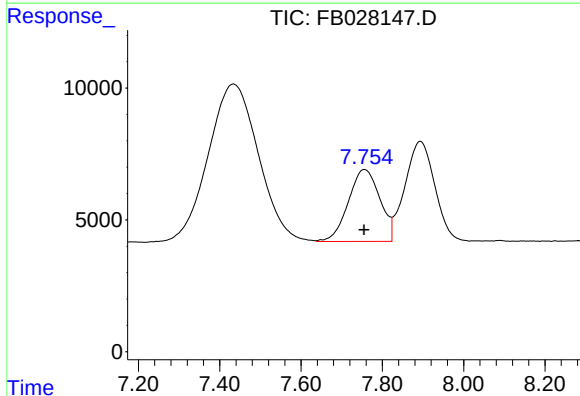


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 147359
Conc: 7.65 ng/ml

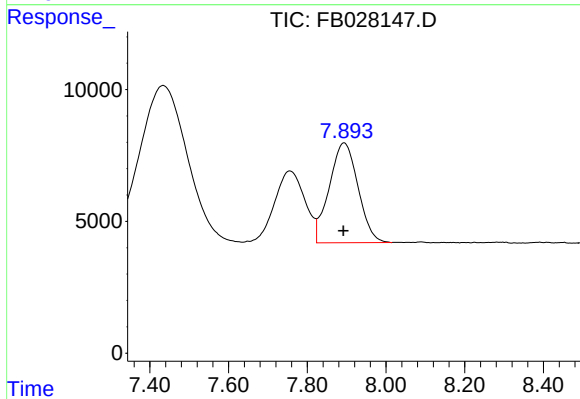

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.002 min
Response: 192540
Conc: 8.28 ng/ml

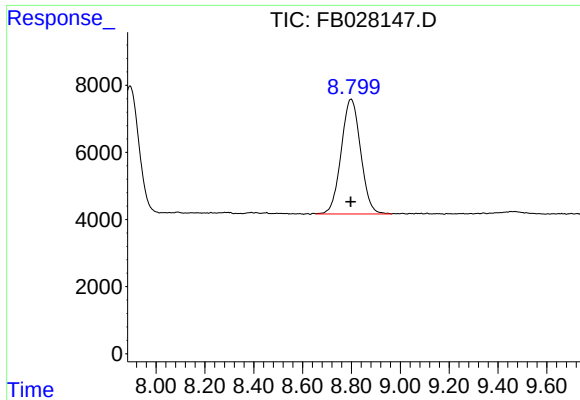

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.001 min
Response: 188577
Conc: 16.27 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0907W1

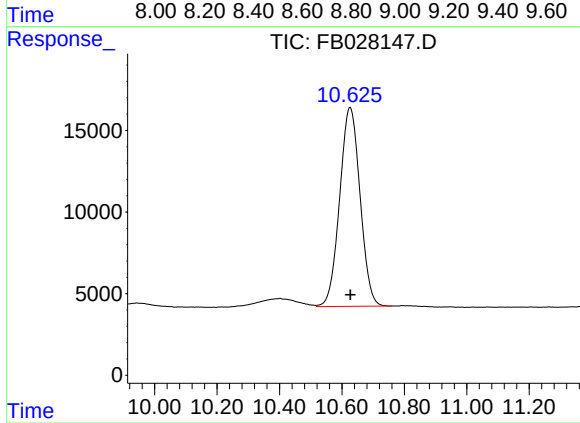


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.000 min
Response: 553424
Conc: 25.24 ng/ml

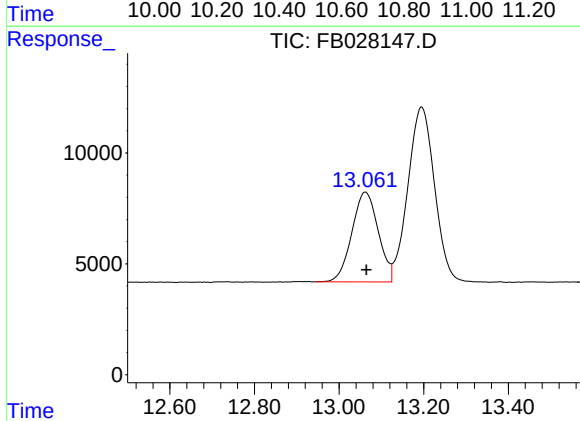


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.002 min
Response: 175331
Conc: 8.51 ng/ml

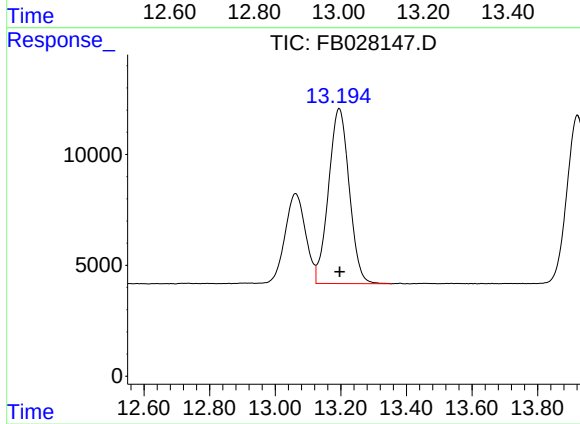

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: -0.001 min
Response: 345857
Conc: 16.90 ng/ml

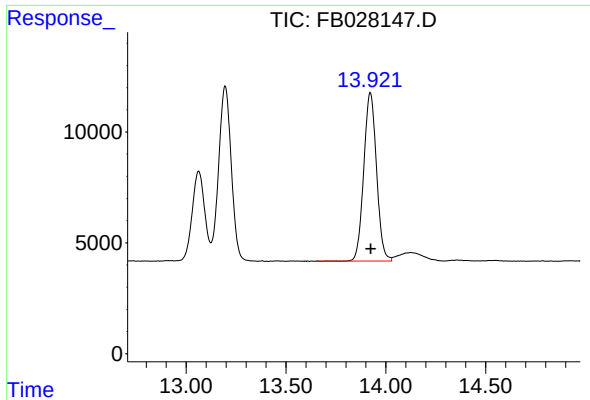

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.002 min
Response: 336775
Conc: 17.00 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0907W1

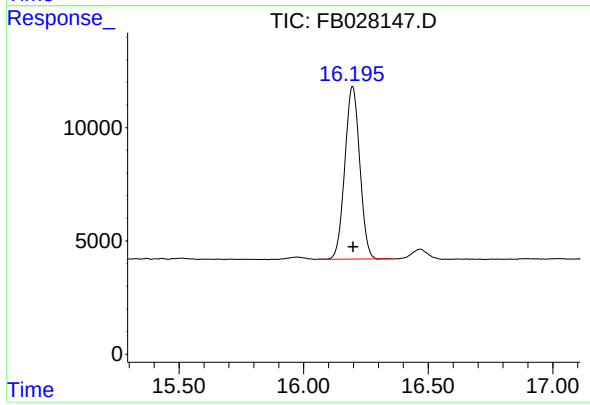

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: -0.003 min
Response: 318148
Conc: 16.31 ng/ml